

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090123\
 Data File : PD077518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2023 10:21
 Operator : AR\AJ
 Sample : 04175-15MS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYC9MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/01/2023
 Supervised By :Ankita Jodhani 09/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 00:56:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.761	36424268	23068540	16.591	18.518
27)	SA Decachlor...	9.086	7.902	77563699	35442508	30.482	28.433
Target Compounds							
2)	A alpha-BHC	3.998	3.263	187.3E6	108.8E6	51.844m	59.187
3)	MA gamma-BHC...	4.332	3.592	163.1E6	106.5E6	47.792m	61.724 #
4)	MA Heptachlor	4.924	3.932	170.6E6	104.7E6	48.778	60.750
5)	MB Aldrin	5.267	4.211	165.3E6	98997509	47.697	57.205
6)	B beta-BHC	4.531	3.889	66137162	42641719	42.617	52.234
7)	B delta-BHC	4.779	4.119	171.3E6	100.6E6	51.669	57.932
8)	B Heptachlo...	5.695	4.713	144.4E6	84776346	45.260	51.822
9)	A Endosulfan I	6.082	5.084	131.5E6	69659242	46.524	49.441
10)	B trans-Chl...	5.952	4.964	136.6E6	80244999	44.230	51.957
11)	B cis-Chlor...	6.031	5.028	140.3E6	77891534	43.818	48.365
12)	B 4,4'-DDE	6.204	5.217	284.4E6	161.8E6	99.308	118.840
13)	MA Dieldrin	6.358	5.349	305.1E6	166.6E6	97.893	105.043
14)	MA Endrin	6.589	5.625	258.4E6	142.7E6	101.645	102.774
15)	B Endosulfa...	6.809	5.919	256.4E6	128.8E6	90.717	96.285
16)	A 4,4'-DDD	6.722	5.772	226.7E6	116.8E6	104.311	117.424
17)	MA 4,4'-DDT	7.038	6.023	251.0E6	120.0E6	113.771	115.934
18)	B Endrin al...	6.939	6.098	181.1E6	94045229	84.154	86.574
19)	B Endosulfa...	7.174	6.321	233.7E6	115.0E6	93.897	91.866
20)	A Methoxychlor	7.514	6.598	693.2E6	317.0E6	538.815	561.937
21)	B Endrin ke...	7.661	6.828	257.3E6	123.4E6	91.413	83.797

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090123\
Data File : PD077518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2023 10:21
Operator : AR\AJ
Sample : 04175-15MS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 00:56:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

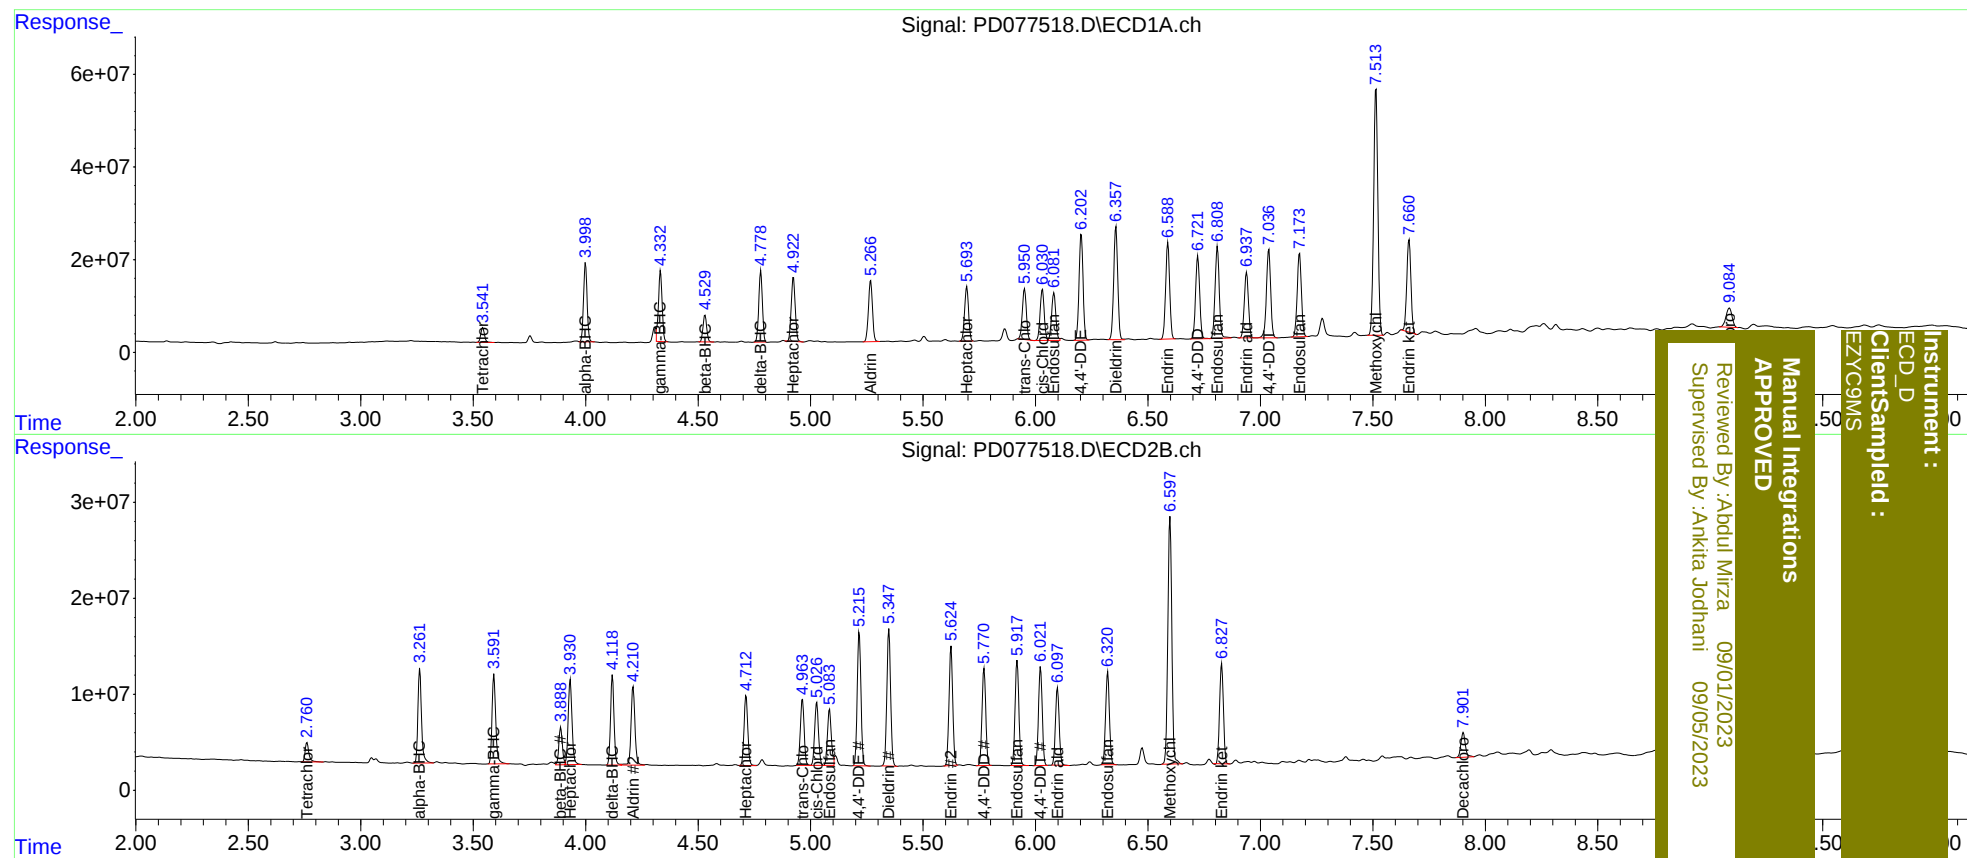

Instrument :
ECD_D
ClientSampled :
EZYC9MS

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/01/2023
Supervised By : Ankita Jodhani 09/05/2023