

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090124\
 Data File : PD084844.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2024 09:44
 Operator : AR\AJ
 Sample : PIBLK089
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 00:18:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.907	24634203	86517125	24.356	24.448
2) SA Decachlor...	9.034	8.106	33949348	89703474	25.994	25.798
Target Compounds						
7) B delta-BHC	4.762	0.000	1824348	0	1.112	N.D. #
8) B Heptachlo...	5.660	0.000	2065988	0	1.385	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090124\
Data File : PD084844.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2024 09:44
Operator : AR\AJ
Sample : PIBLK089
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 00:18:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

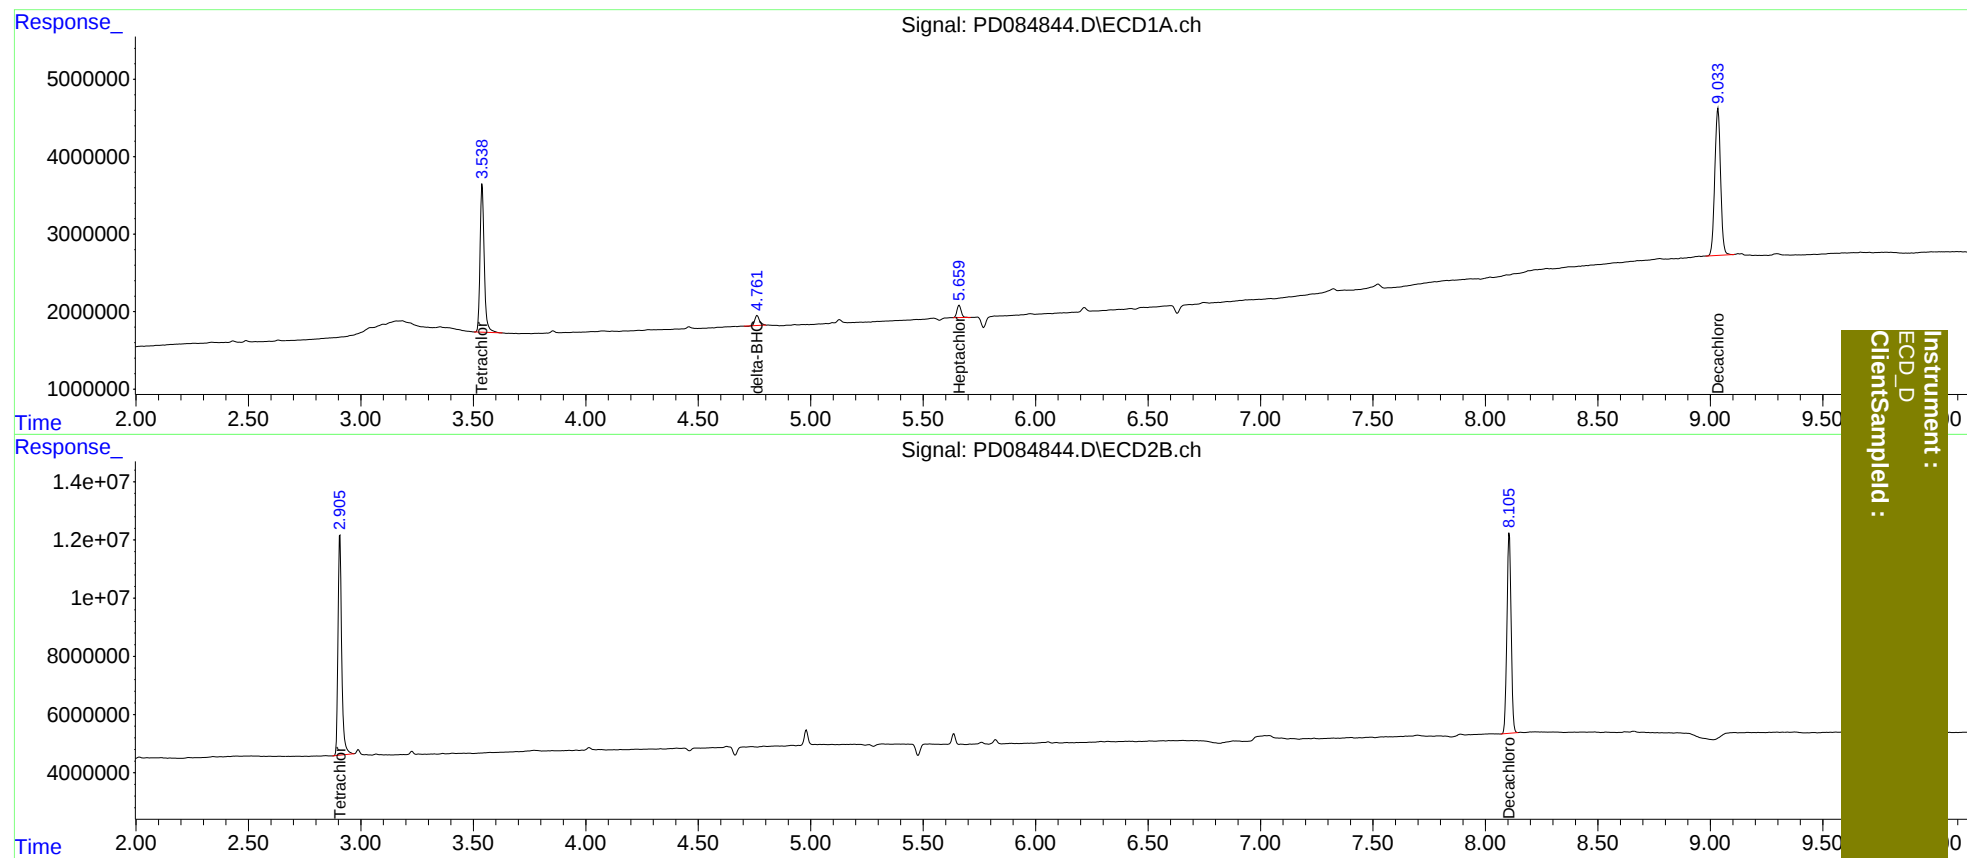


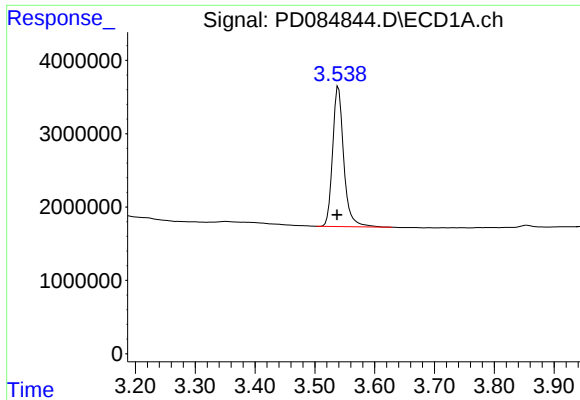

#1 Tetrachloro-m-xylene


R.T.: 3.540 min
Delta R.T.: 0.003 min
Response: 24634203
Conc: 24.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

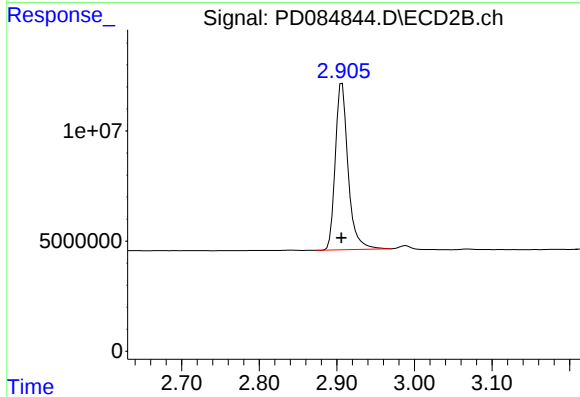


#1 Tetrachloro-m-xylene

R.T.: 2.907 min
Delta R.T.: 0.000 min
Response: 86517125
Conc: 24.45 ng/ml

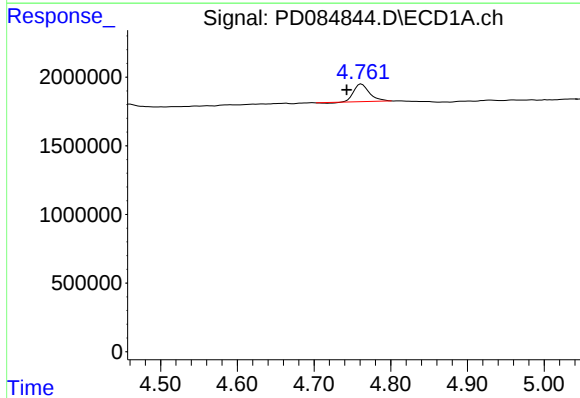


#7 delta-BHC

R.T.: 4.762 min
Delta R.T.: 0.019 min
Response: 1824348
Conc: 1.11 ng/ml

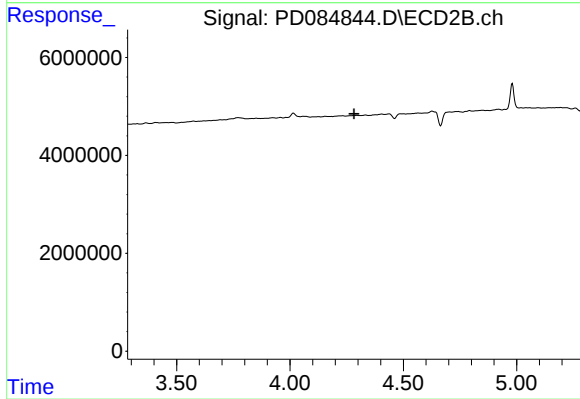

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

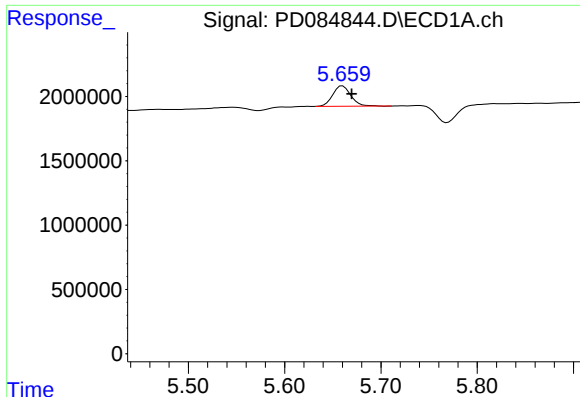

#8 Heptachlor epoxide


R.T.: 5.660 min
Delta R.T.: -0.009 min
Response: 2065988
Conc: 1.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

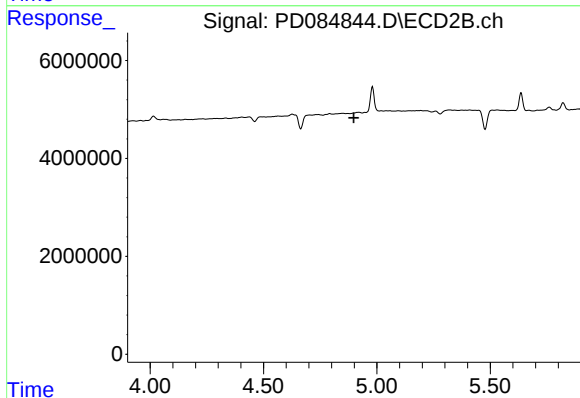


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.898 min
Response: 0
Conc: N.D.

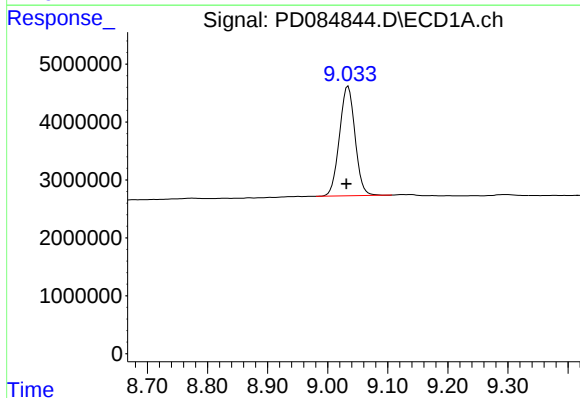

#27 Decachlorobiphenyl

R.T.: 9.034 min
Delta R.T.: 0.003 min
Response: 33949348
Conc: 25.99 ng/ml

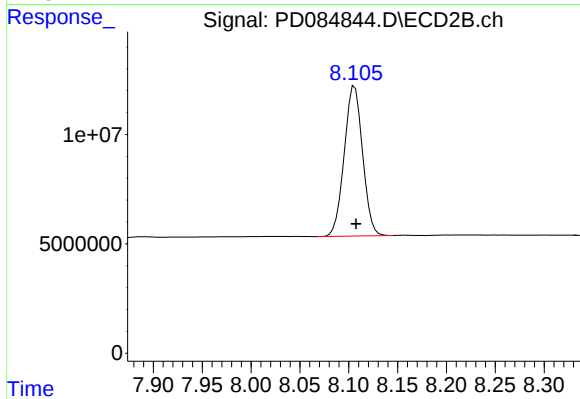

#27 Decachlorobiphenyl

R.T.: 8.106 min
Delta R.T.: -0.001 min
Response: 89703474
Conc: 25.80 ng/ml