

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090124\
 Data File : PD084848.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2024 12:38
 Operator : AR\AJ
 Sample : P3722-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 00:19:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.904	12805405	44313482	12.661	12.522
27)	SA Decachlor...	9.041	8.109	14146528	41143371	10.832	11.832
Target Compounds							
15)	B Endosulfa...	6.803f	6.132	4112082	8199752	3.115	2.212 #
19)	B Endosulfa...	0.000	6.533	0	119.3E6	N.D.	33.402


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090124\
Data File : PD084848.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2024 12:38
Operator : AR\AJ
Sample : P3722-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 00:19:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

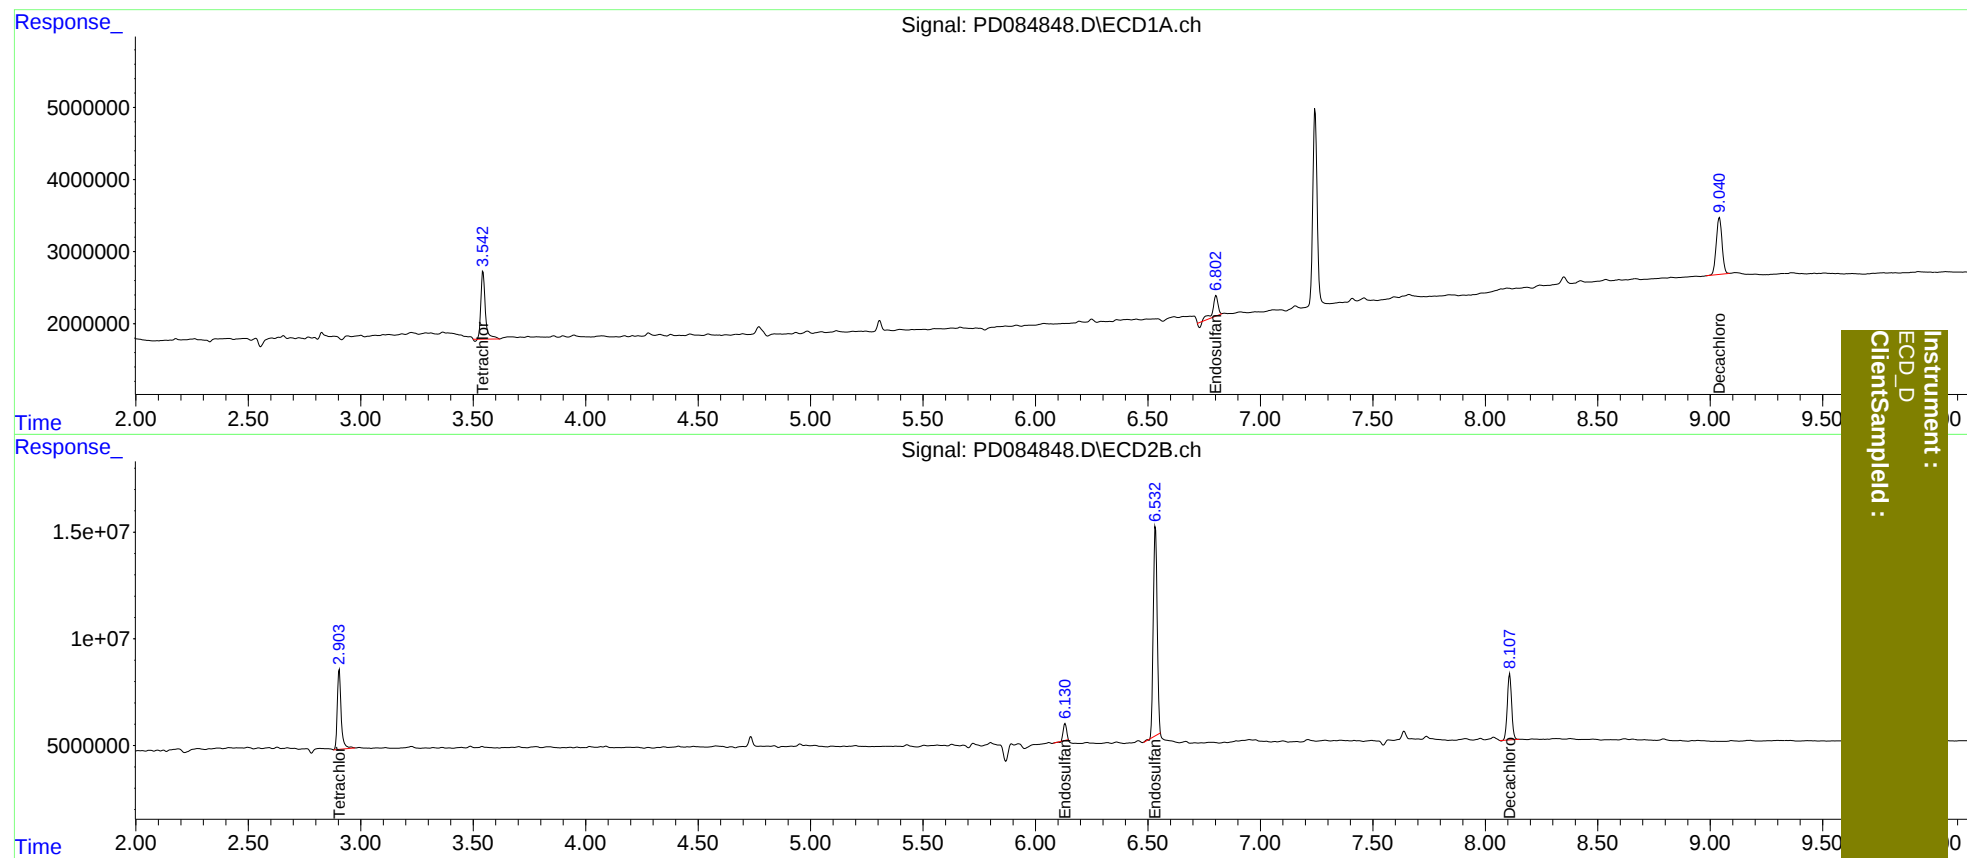


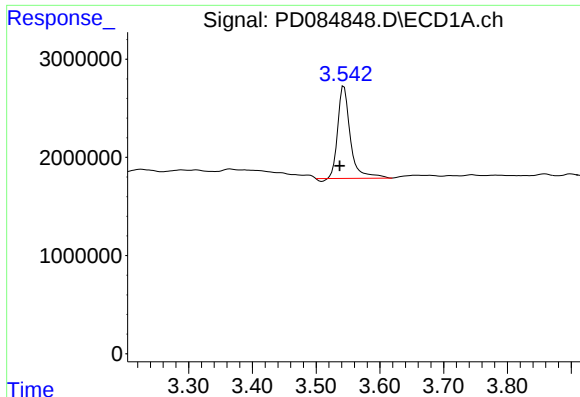

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.007 min
Response: 12805405
Conc: 12.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

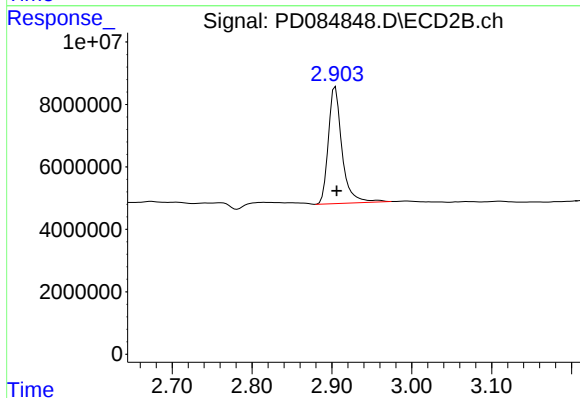


#1 Tetrachloro-m-xylene

R.T.: 2.904 min
Delta R.T.: -0.001 min
Response: 44313482
Conc: 12.52 ng/ml

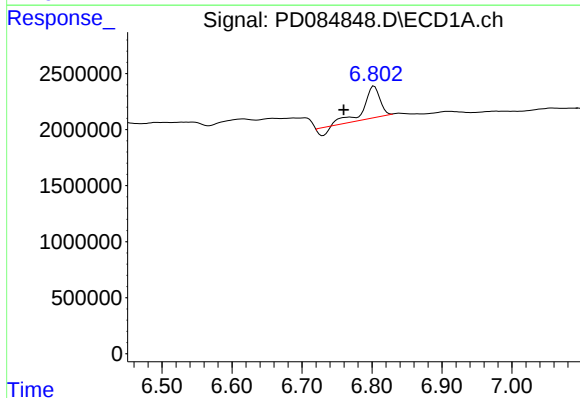


#15 Endosulfan II

R.T.: 6.803 min
Delta R.T.: 0.043 min
Response: 4112082
Conc: 3.12 ng/ml

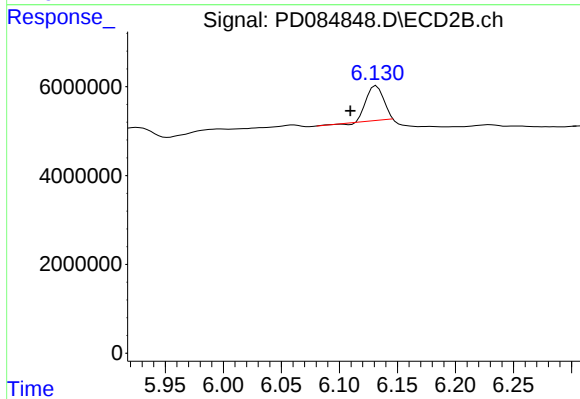

#15 Endosulfan II


R.T.: 6.132 min
Delta R.T.: 0.022 min
Response: 8199752
Conc: 2.21 ng/ml

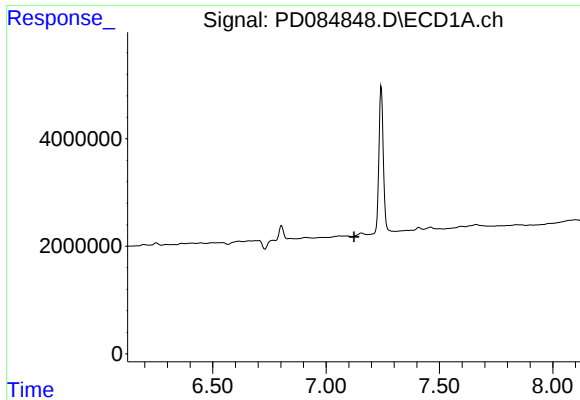

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.123 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

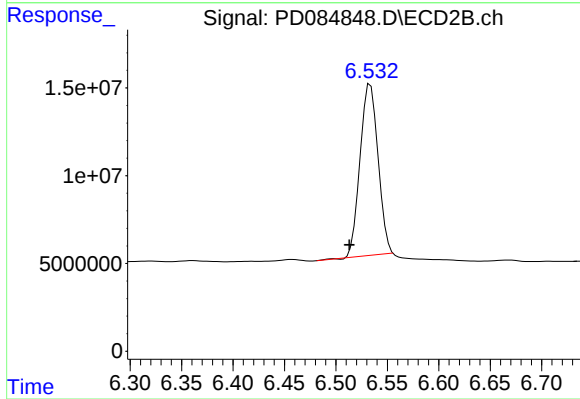


#19 Endosulfan Sulfate

R.T.: 6.533 min
Delta R.T.: 0.021 min
Response: 119296905
Conc: 33.40 ng/ml

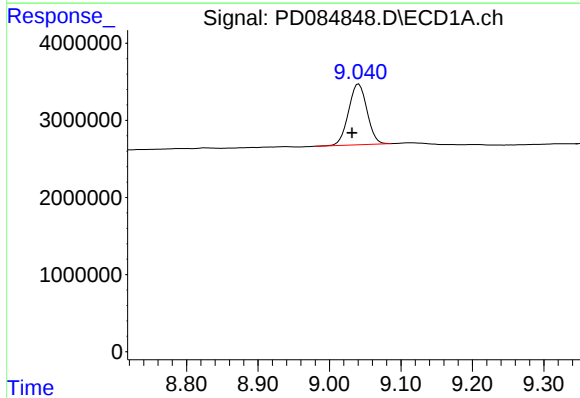

#27 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.010 min
Response: 14146528
Conc: 10.83 ng/ml

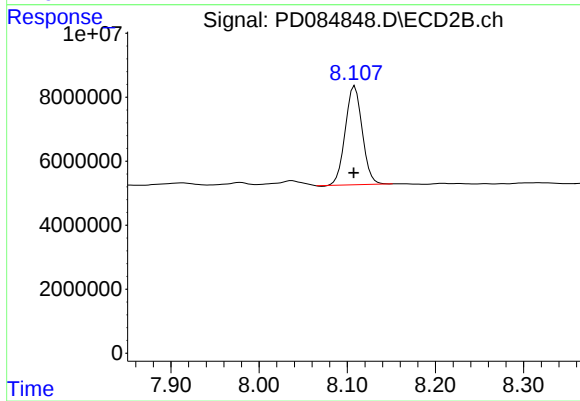

#27 Decachlorobiphenyl

R.T.: 8.109 min
Delta R.T.: 0.001 min
Response: 41143371
Conc: 11.83 ng/ml