

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090124\
 Data File : PD084851.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2024 13:41
 Operator : AR\AJ
 Sample : PIBLK090
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 00:20:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.904	24180326	83932697	23.908	23.718
2) SA Decachlor...	9.040	8.108	34468522	92648572	26.392	26.645
Target Compounds						
7) B delta-BHC	4.768f	0.000	1718068	0	1.048	N.D. #
8) B Heptachlo...	5.667	0.000	1743649	0	1.169	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090124\
Data File : PD084851.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2024 13:41
Operator : AR\AJ
Sample : PIBLK090
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 00:20:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

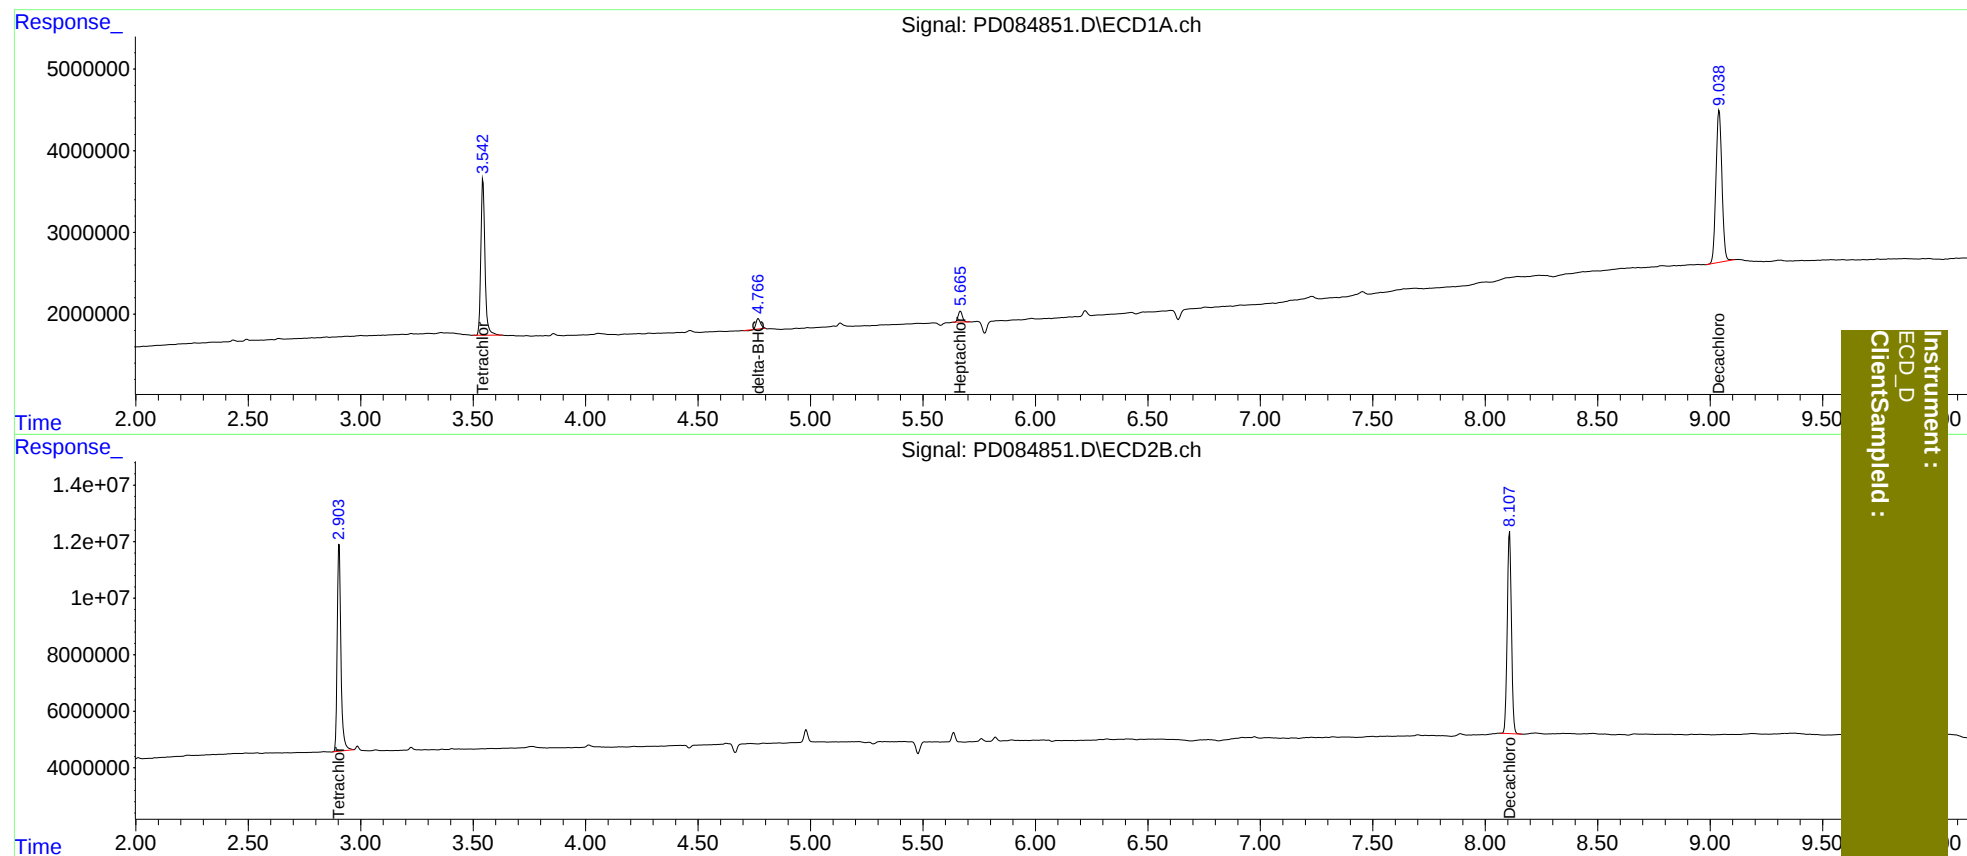


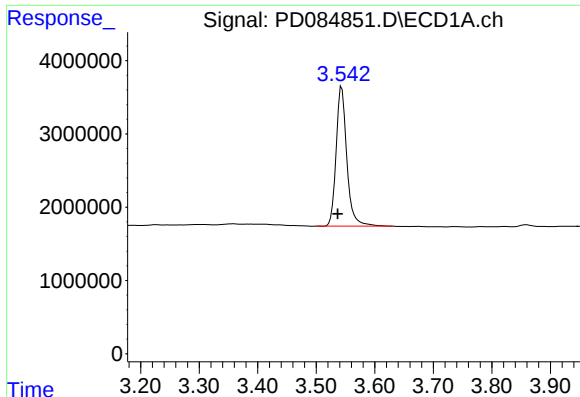

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.007 min
Response: 24180326
Conc: 23.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

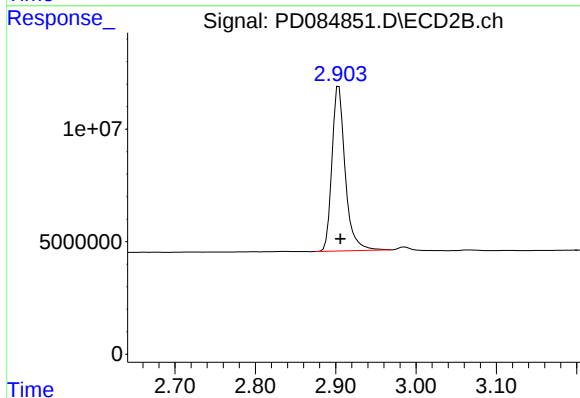


#1 Tetrachloro-m-xylene

R.T.: 2.904 min
Delta R.T.: -0.002 min
Response: 83932697
Conc: 23.72 ng/ml

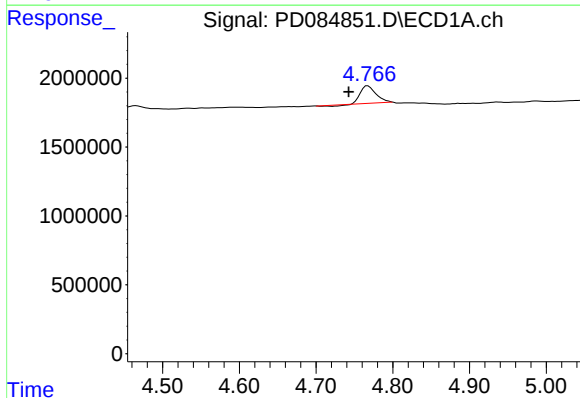


#7 delta-BHC

R.T.: 4.768 min
Delta R.T.: 0.025 min
Response: 1718068
Conc: 1.05 ng/ml

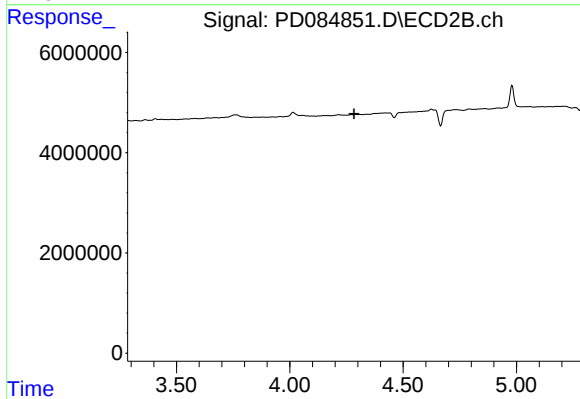

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.283 min
Response: 0
Conc: N.D.

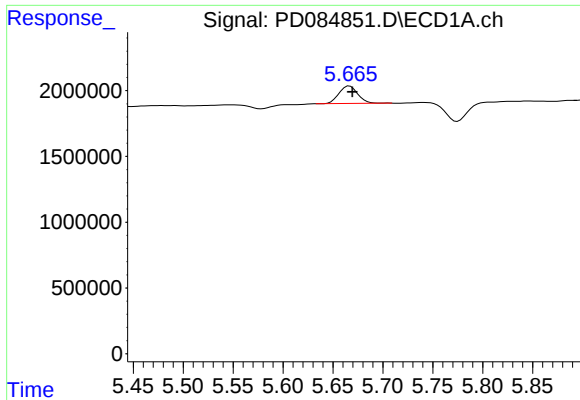

#8 Heptachlor epoxide


R.T.: 5.667 min
Delta R.T.: -0.003 min
Response: 1743649
Conc: 1.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

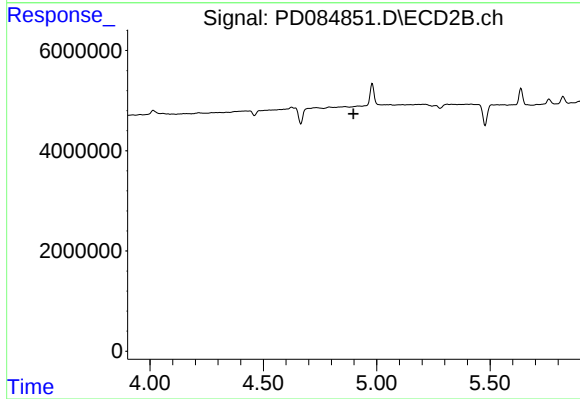


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.898 min
Response: 0
Conc: N.D.

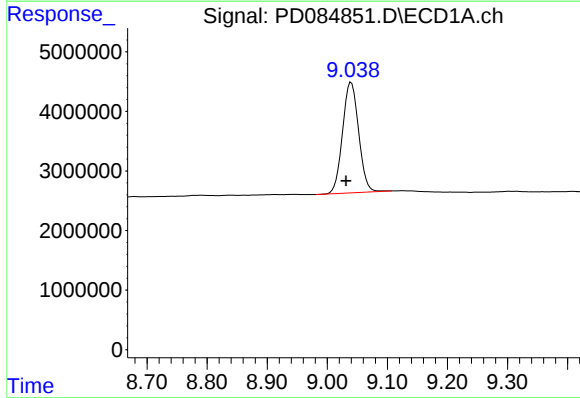

#27 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.009 min
Response: 34468522
Conc: 26.39 ng/ml

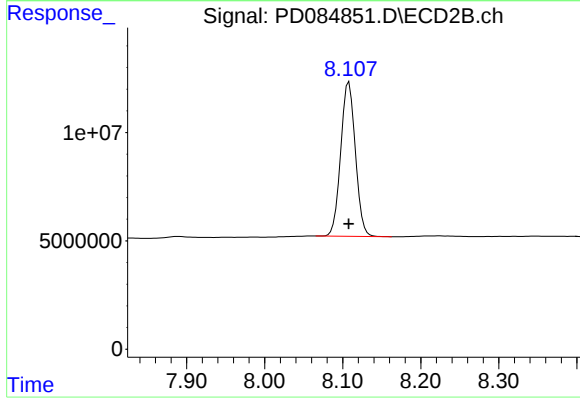

#27 Decachlorobiphenyl

R.T.: 8.108 min
Delta R.T.: 0.000 min
Response: 92648572
Conc: 26.64 ng/ml