

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090124\
 Data File : PD084850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Aug 2024 13:05
 Operator : AR\AJ
 Sample : P3722-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCYD5MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/03/2024
 Supervised By :Ankita Jodhani 09/03/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 31 00:20:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.906	14668424	47141433	14.503	13.321
27)	SA Decachlor...	9.034	8.107	15060237	44653657	11.531	12.842
Target Compounds							
2)	A alpha-BHC	3.984	3.417	95869252	269.1E6	56.388	53.074
3)	MA gamma-BHC...	4.313	3.752	91555453	255.9E6	56.591	52.805
4)	MA Heptachlor	4.910	4.106	89998727	230.8E6	58.494	54.218
5)	MB Aldrin	5.251	4.393	85792339	232.2E6	53.642	52.288
6)	B beta-BHC	4.495	4.044	36464853	110.1E6	50.201	50.789m
7)	B delta-BHC	4.743	4.283	91872877	260.2E6	56.020	52.410
8)	B Heptachlo...	5.670	4.897	77190182	213.4E6	51.755	50.379
9)	A Endosulfan I	6.051	5.271	72570920	203.3E6	52.748m	53.046m
10)	B trans-Chl...	5.924	5.150	75095736	215.7E6	53.245	52.443m
11)	B cis-Chlor...	6.004	5.215	77165114	211.1E6	52.189m	50.313
12)	B 4,4'-DDE	6.174	5.401	143.2E6	411.3E6	114.818	104.850
13)	MA Dieldrin	6.325	5.540	160.3E6	441.1E6	108.667	102.669
14)	MA Endrin	6.552	5.816	136.2E6	415.0E6	120.740	112.099m
15)	B Endosulfa...	6.762	6.108	138.9E6	394.1E6	105.257m	106.282m
16)	A 4,4'-DDD	6.682	5.957	115.3E6	343.6E6	116.780	101.252
17)	MA 4,4'-DDT	6.996	6.213	109.2E6	348.8E6	122.039m	109.026
18)	B Endrin al...	6.891	6.288	97857008	288.2E6	108.356	100.942
19)	B Endosulfa...	7.125	6.512	126.8E6	501.8E6	110.034	140.505m#
20)	A Methoxychlor	7.468	6.785	304.0E6	831.6E6	583.521	502.689
21)	B Endrin ke...	7.605	7.023	134.3E6	428.0E6	109.859	97.203

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090124\
Data File : PD084850.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Aug 2024 13:05
Operator : AR\AJ
Sample : P3722-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 31 00:20:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

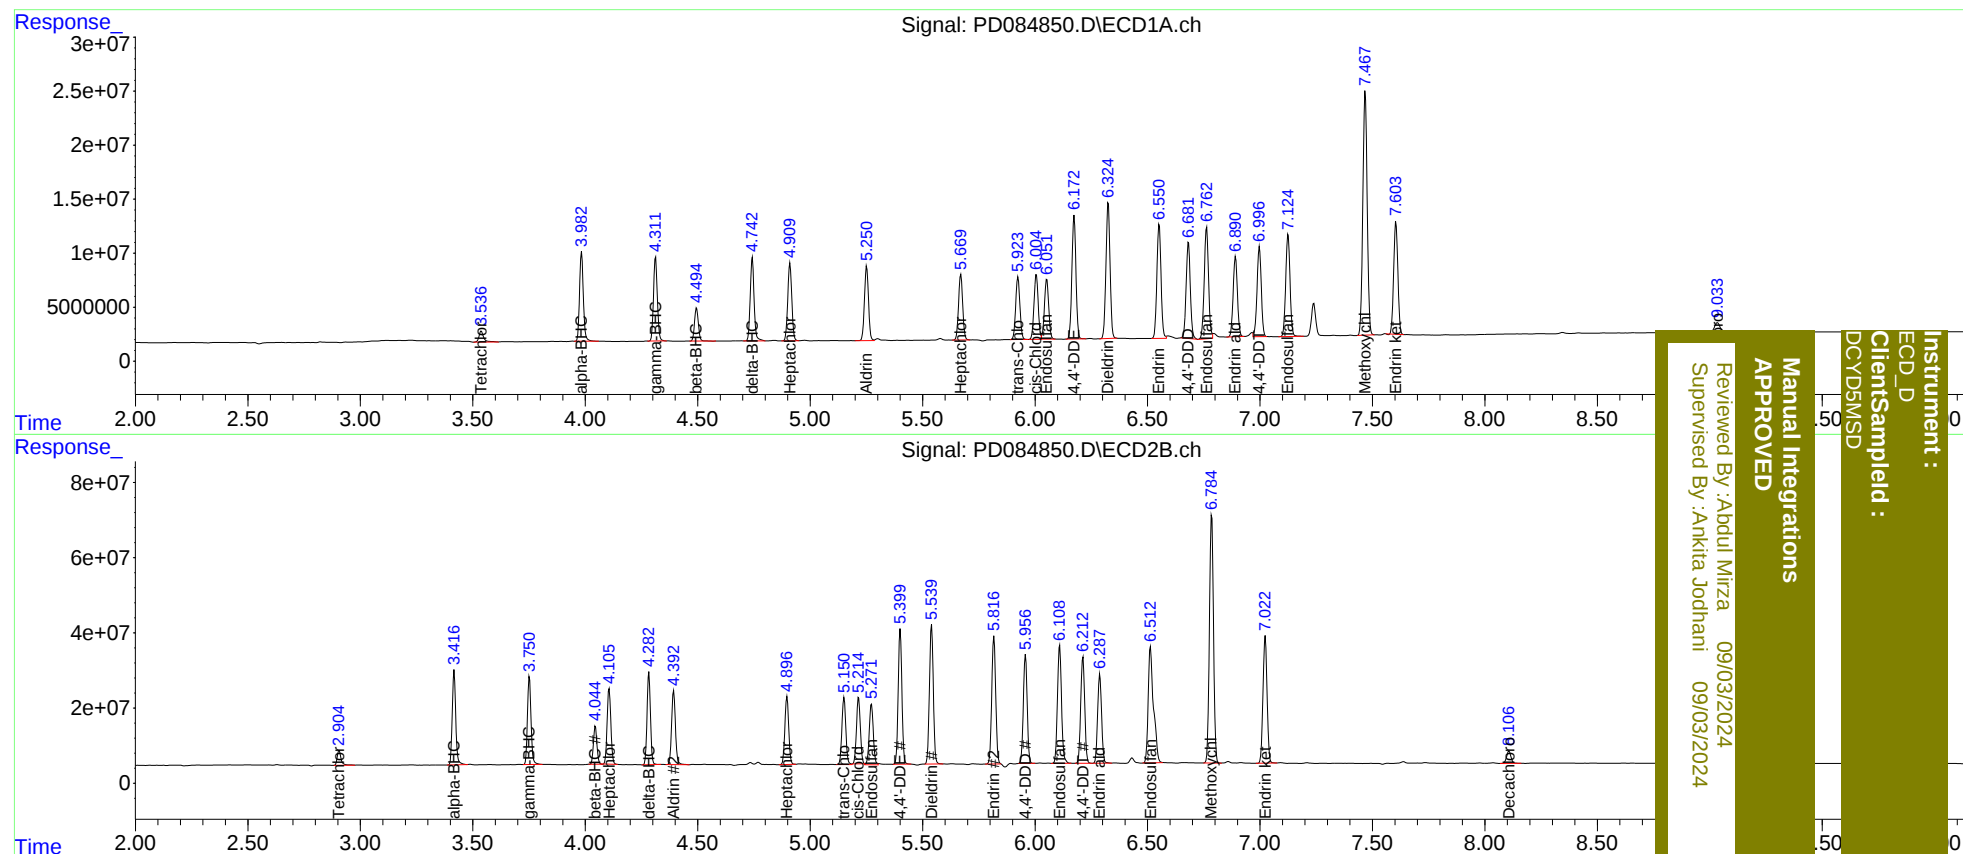

Instrument :
ECD_D
Client Sampled :
DCYD5MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 09/03/2024
Supervised By: Ankita Jodhani 09/03/2024