

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090221\
 Data File : PD065515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2021 10:11
 Operator : AR\AJ
 Sample : M3263-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 MDL-WATER-QT4-2021-08

Manual Integrations
 APPROVED

Ankita
 9/2/2021 1:02:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 05:16:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082921CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 28 03:49:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.014	21875459	159.5E6	19.350	19.686
2)	SA Decachlor...	8.242	9.087	53257847	198.4E6	36.866	38.363
Target Compounds							
2)	A alpha-BHC	3.935	4.409	2248815	15270506	1.461	1.398
3)	MA gamma-BHC...	4.219	4.696	2809652	14538767	1.717	1.382
4)	MA Heptachlor	4.517	5.200	1968810	14524391	1.343	1.443
5)	MB Aldrin	4.763	5.505	1860941	13536980	1.318m	1.415
6)	B beta-BHC	4.467	4.873	1063413	6827635	1.442	1.422
7)	B delta-BHC	4.672	5.088	1878455	15603157	1.251	1.514
8)	B Heptachlo...	5.207	5.895	1892405	10826766	1.403	1.327
9)	A Endosulfan I	5.546	6.253	1760282	10413380	1.381	1.404
10)	B trans-Chl...	5.431	6.129	1893316	11144147	1.382m	1.374
11)	B cis-Chlor...	5.491	6.200	1865367	10922408	1.371	1.378
12)	B 4,4'-DDE	5.654	6.358	1695593	10454053	1.356	1.413
13)	MA Dieldrin	5.789	6.511	2042483	11089669	1.526	1.450
14)	MA Endrin	6.047	6.730	1646368	8768132	1.352	1.384
15)	B Endosulfa...	6.319	6.943	1694686	9026145	1.345	1.392
16)	A 4,4'-DDD	6.170	6.852	1217315	7916369	1.109	1.315
17)	MA 4,4'-DDT	6.409	7.150	1392445	7443537	1.161	1.220
18)	B Endrin al...	6.488	7.067	1538412	8008451	1.534	1.565
19)	B Endosulfa...	6.700	7.289	1867693	8250012	1.459	1.328m
20)	A Methoxychlor	6.957	7.609	750205	4241313	1.147	1.453 #
21)	B Endrin ke...	7.194	7.763	2185038	10080695	1.406	1.419

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090221\
Data File : PD065515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2021 10:11
Operator : AR\AJ
Sample : M3263-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 05:16:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082921CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 28 03:49:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

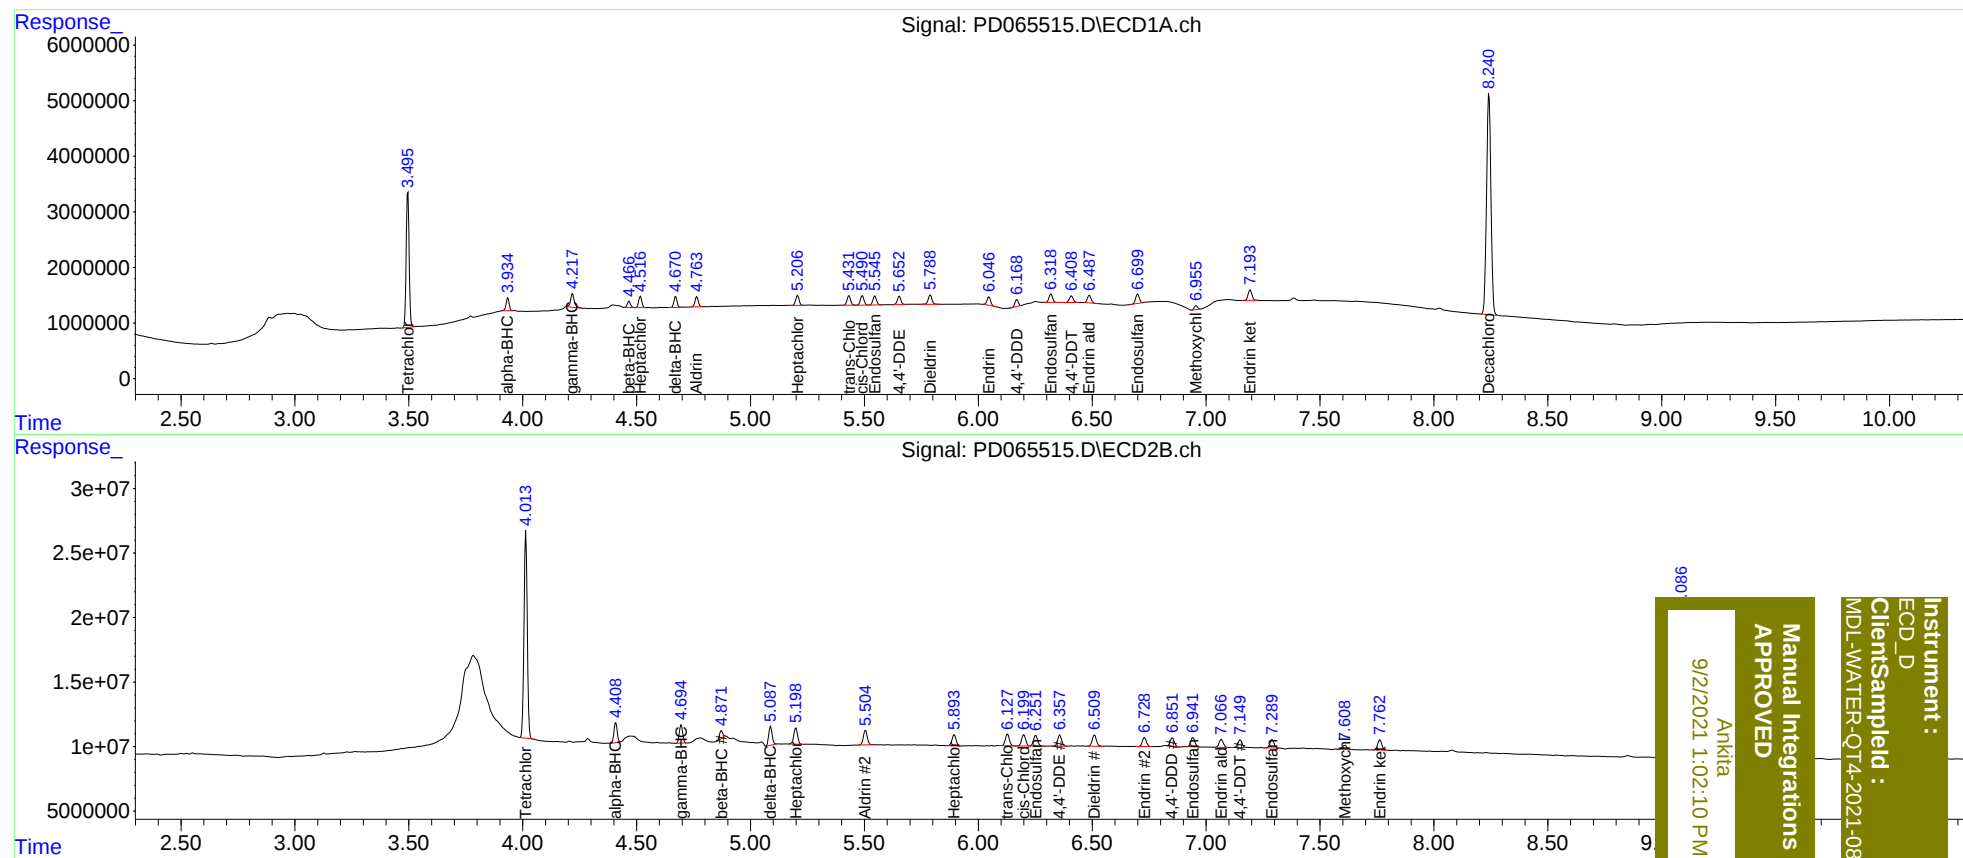

Manual Integrations
APPROVED

Ankita

9/2/2021 1:02:10 PM

Instrument :
ECD_D
Client Sample :
MDL-WATER-QT4-2021-08