

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090222\
 Data File : PD071734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 20:41
 Operator : AR\AJ
 Sample : N4484-02MS
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 02:09:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 07:11:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.805	3.562	47376358	601.5E6	18.166	18.358
27)	SA Decachlor...	7.992	9.084	103.6E6	383.8E6	39.486	40.148
Target Compounds							
2)	A alpha-BHC	3.313	4.028	211.5E6	2155.5E6	54.835	48.855
3)	MA gamma-BHC...	3.646	4.364	200.4E6	1794.2E6	54.282	48.242
4)	MA Heptachlor	3.992	4.941	189.8E6	1228.6E6	49.872	45.499
5)	MB Aldrin	4.276	5.283	199.5E6	1054.6E6	56.045	48.817
6)	B beta-BHC	3.944	4.570	75008348	695.3E6	47.219	48.582
7)	B delta-BHC	4.177	4.818	199.3E6	1394.6E6	57.049	53.058
8)	B Heptachlo...	4.782	5.714	183.6E6	865.2E6	56.345	51.163
9)	A Endosulfan I	5.155	6.102	168.9E6	762.7E6	53.586	48.564
10)	B trans-Chl...	5.034	5.968	186.0E6	815.1E6	54.933	48.154
11)	B cis-Chlor...	5.098	6.046	183.1E6	781.2E6	54.900	47.926
12)	B 4,4'-DDE	5.290	6.219	352.6E6	1492.3E6	114.970	102.267
13)	MA Dieldrin	5.422	6.379	384.6E6	1620.0E6	111.070	101.222
14)	MA Endrin	5.699	6.612	337.6E6	1359.4E6	112.739	103.319
15)	B Endosulfa...	5.994	6.837	319.0E6	1308.3E6	120.027	108.540
16)	A 4,4'-DDD	5.848	6.743	297.2E6	1245.4E6	112.912	101.772
17)	MA 4,4'-DDT	6.101	7.054	318.3E6	1276.1E6	116.936	105.755
18)	B Endrin al...	6.175	6.968	249.5E6	1021.8E6	107.863	100.156
19)	B Endosulfa...	6.399	7.201	292.7E6	1155.4E6	109.865	101.736
20)	A Methoxychlor	6.680	7.530	766.4E6	2783.4E6	533.602	507.275
21)	B Endrin ke...	6.908	7.693	360.6E6	1359.4E6	120.508	109.817
22)	Toxaphene-1	5.382	5.875	-116202	8962110	N.D.	150.946
23)	Toxaphene-2	5.699f	6.300	337.6E6	328352	18342.433	2.762 #
24)	Toxaphene-3	5.994f	7.054f	319.0E6	1276.1E6	15000.555	6986.420 #
25)	Toxaphene-4	6.754f	7.201	2916941	1155.4E6	33.245	4399.607 #
26)	Toxaphene-5	7.104	7.613	758465	20210690	19.838	135.515 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090222\
Data File : PD071734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 20:41
Operator : AR\AJ
Sample : N4484-02MS
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 02:09:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

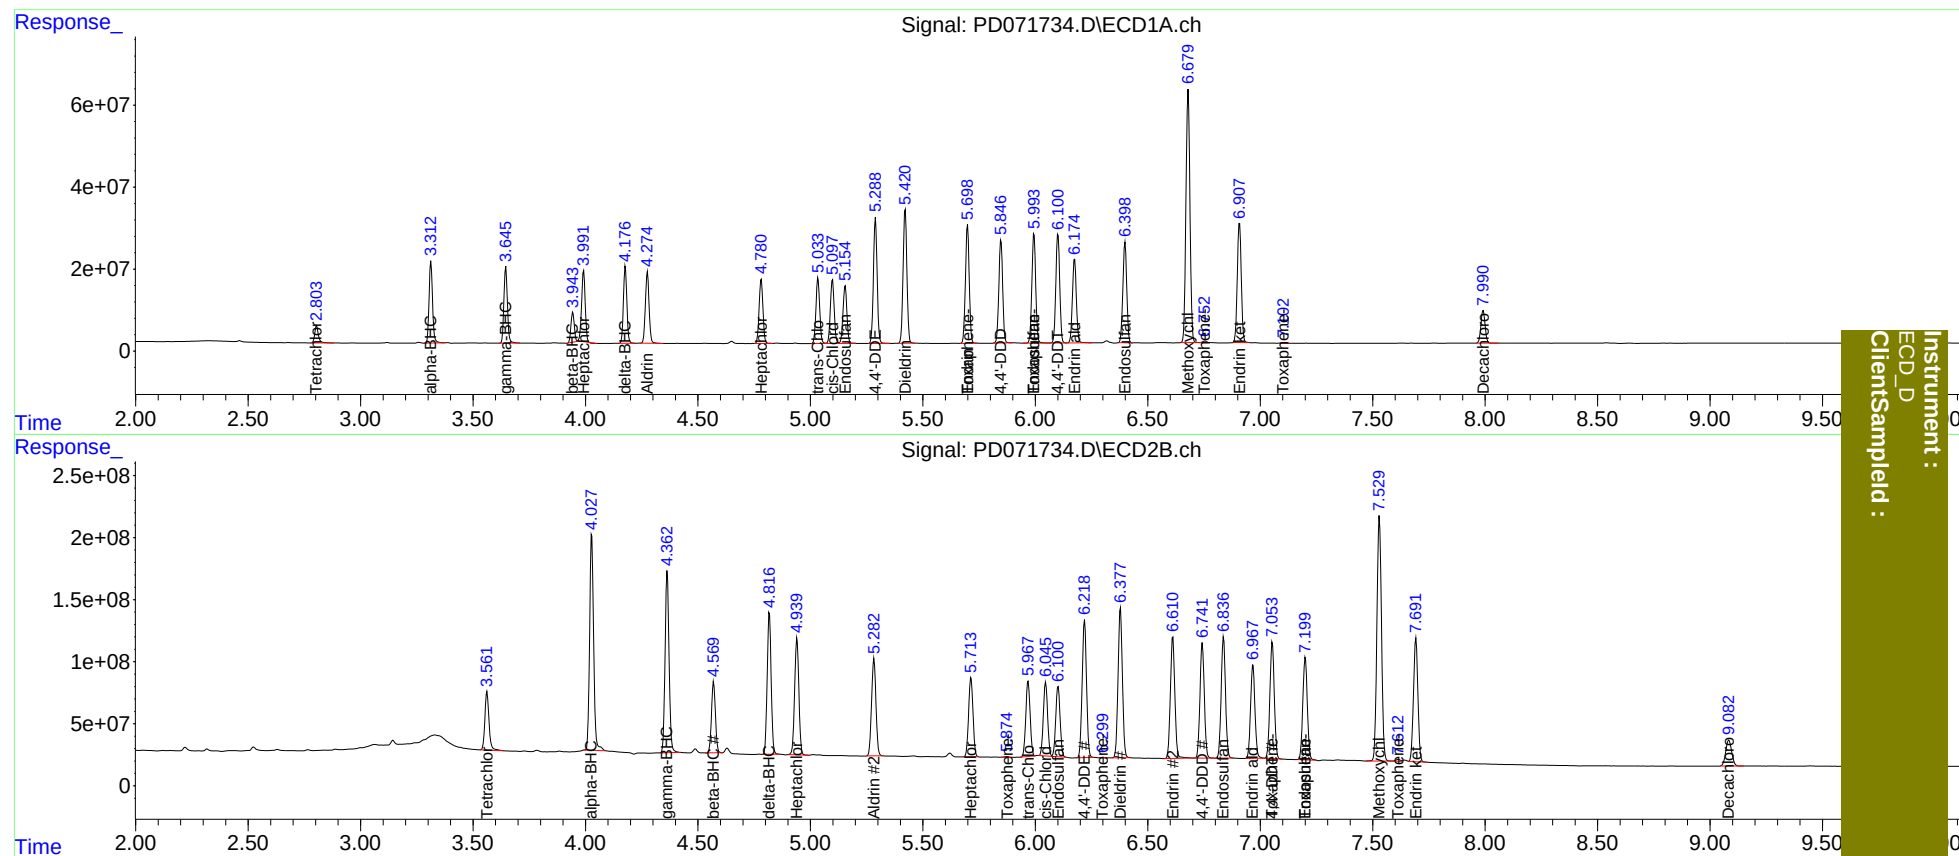

Instrument :
ECD_D
ClientSampled :