

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090222\
 Data File : PD071716.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 15:50
 Operator : AR\AJ
 Sample : PB147447BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS447

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/06/2022
 Supervised By : Ankita Jodhani 09/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 02:05:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 07:11:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.814	3.563	39740247	541.8E6	15.238	16.534
27)	SA Decachlor...	8.004	9.091	84509861	334.6E6	32.204	35.007
Target Compounds							
2)	A alpha-BHC	3.323	4.029	14158827	190.2E6	3.671	4.310
3)	MA gamma-BHC...	3.657	4.365	14065260	166.0E6	3.810	4.463
4)	MA Heptachlor	4.002	4.942	14363948	124.8E6	3.774m	4.623
5)	MB Aldrin	4.287	5.285	14749388	107.9E6	4.143	4.994
6)	B beta-BHC	3.954	4.572	7066625	65964165	4.449m	4.609
7)	B delta-BHC	4.189	4.818	12181722	109.8E6	3.486	4.178m
8)	B Heptachlo...	4.793	5.717	14071356	88103311	4.317	5.210
9)	A Endosulfan I	5.167	6.106	12665083	75756612	4.019	4.824
10)	B trans-Chl...	5.046	5.972	14156199	80841886	4.181	4.776
11)	B cis-Chlor...	5.111	6.050	13966750	80515938	4.187	4.940
12)	B 4,4'-DDE	5.302	6.223	24888761	144.0E6	8.114	9.869
13)	MA Dieldrin	5.434	6.382	28400408	156.0E6	8.201	9.749
14)	MA Endrin	5.711	6.614	24425500	125.6E6	8.156	9.546
15)	B Endosulfa...	6.006	6.841	23410825	127.7E6	8.807	10.597
16)	A 4,4'-DDD	5.860	6.747	20759181	126.0E6	7.887	10.299 #
17)	MA 4,4'-DDT	6.113	7.059	22549664	121.1E6	8.283	10.036
18)	B Endrin al...	6.187	6.972	18849401	93879579	8.149	9.202
19)	B Endosulfa...	6.411	7.205	22544377	106.0E6	8.463	9.331
20)	A Methoxychlor	6.693	7.535	65514683	302.4E6	45.614	55.119
21)	B Endrin ke...	6.919	7.697	29841551	125.1E6	9.972m	10.102

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090222\
Data File : PD071716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 15:50
Operator : AR\AJ
Sample : PB147447BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 02:05:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

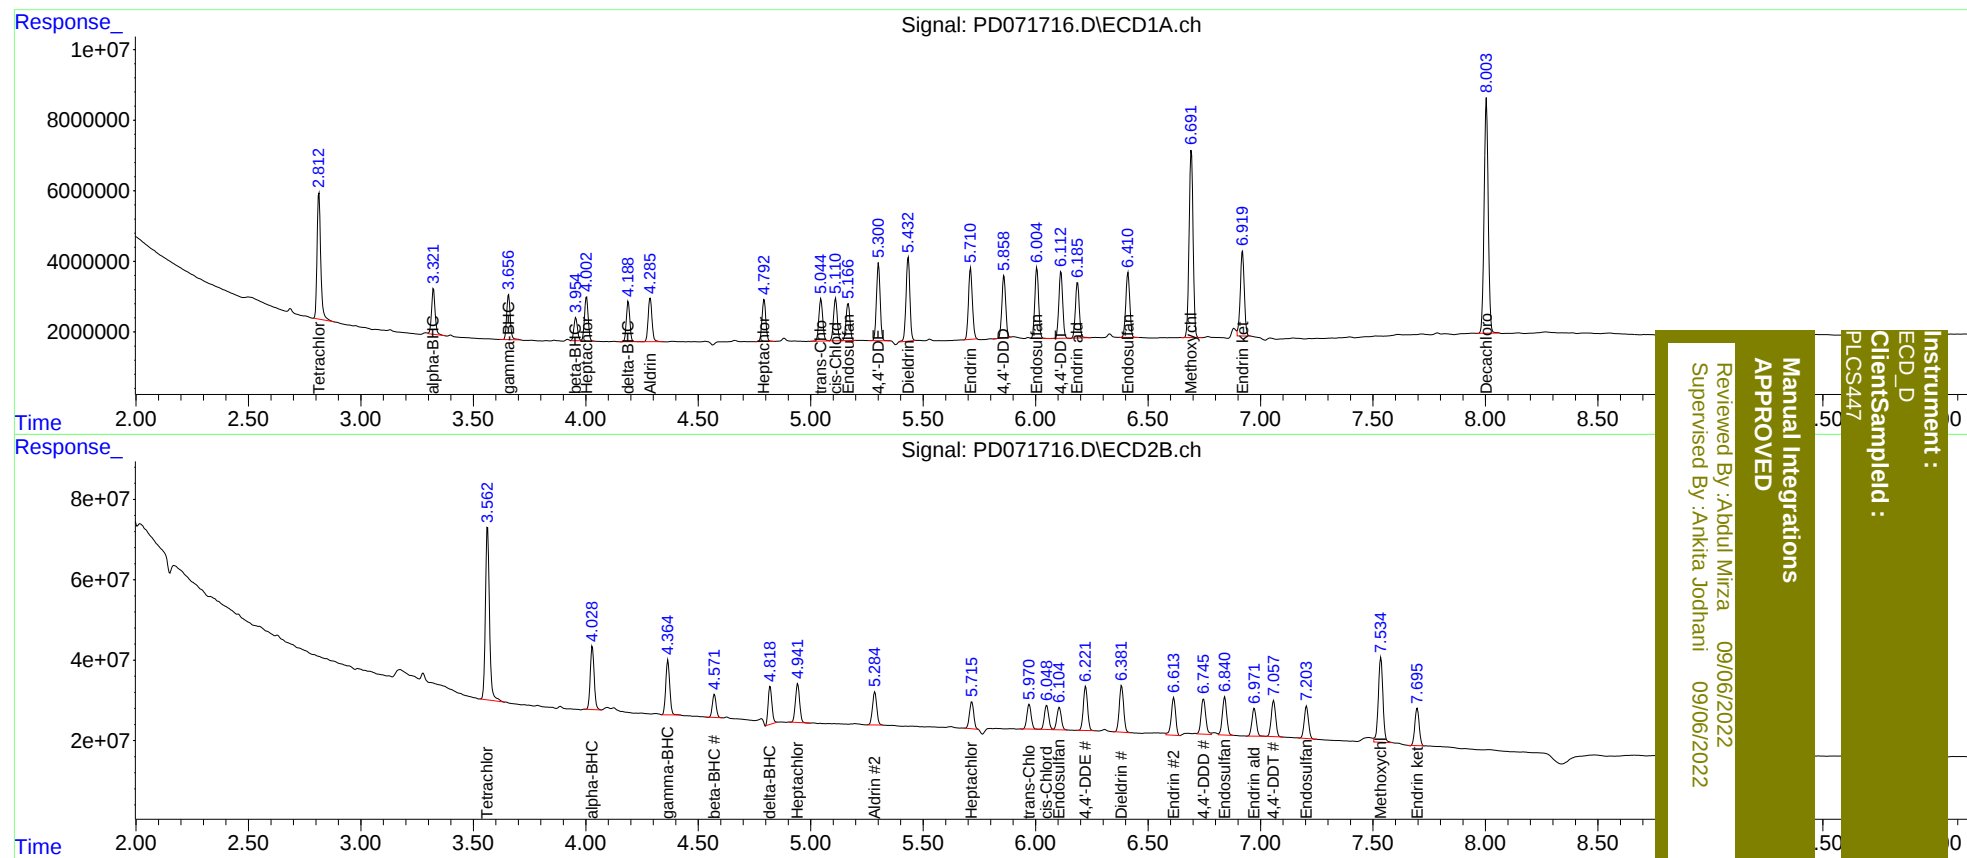

Reviewed By: Abdul Mirza 09/06/2022
Supervised By: Ankita Jodhani 09/06/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
PLCS447