

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090222\
 Data File : PD071735.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 20:55
 Operator : AR\AJ
 Sample : N4484-03MSD
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0KR2MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/06/2022
 Supervised By :Ankita Jodhani 09/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 02:09:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 07:11:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.805	3.563	45557616	589.1E6	17.469	17.977
27)	SA Decachlor...	7.993	9.084	99573823	364.3E6	37.944	38.106
Target Compounds							
2)	A alpha-BHC	3.313	4.028	214.1E6	2166.6E6	55.499	49.105
3)	MA gamma-BHC...	3.646	4.364	202.3E6	1809.1E6	54.805	48.641
4)	MA Heptachlor	3.991	4.941	201.6E6	1217.0E6	52.960m	45.069
5)	MB Aldrin	4.276	5.282	198.6E6	1037.1E6	55.775	48.008
6)	B beta-BHC	3.943	4.570	82450302	698.1E6	51.904m	48.775
7)	B delta-BHC	4.178	4.818	200.3E6	1400.9E6	57.327	53.298
8)	B Heptachlo...	4.782	5.715	182.5E6	853.8E6	55.998	50.491
9)	A Endosulfan I	5.156	6.102	167.7E6	754.7E6	53.207	48.056
10)	B trans-Chl...	5.035	5.969	184.5E6	807.8E6	54.482	47.718
11)	B cis-Chlor...	5.099	6.046	180.5E6	774.6E6	54.127	47.526
12)	B 4,4'-DDE	5.290	6.219	350.3E6	1480.6E6	114.194	101.465
13)	MA Dieldrin	5.422	6.379	383.6E6	1616.1E6	110.775	100.982
14)	MA Endrin	5.699	6.612	337.5E6	1354.9E6	112.688	102.982
15)	B Endosulfa...	5.995	6.837	315.9E6	1307.9E6	118.863	108.504
16)	A 4,4'-DDD	5.848	6.743	297.6E6	1241.0E6	113.081	101.415
17)	MA 4,4'-DDT	6.101	7.054	319.4E6	1270.6E6	117.342	105.299
18)	B Endrin al...	6.175	6.968	249.0E6	1015.9E6	107.628	99.578
19)	B Endosulfa...	6.399	7.201	291.4E6	1162.6E6	109.399	102.374
20)	A Methoxychlor	6.681	7.530	765.5E6	2770.8E6	532.958	504.991
21)	B Endrin ke...	6.908	7.692	359.5E6	1352.2E6	120.130	109.236

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090222\
Data File : PD071735.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 20:55
Operator : AR\AJ
Sample : N4484-03MSD
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 02:09:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

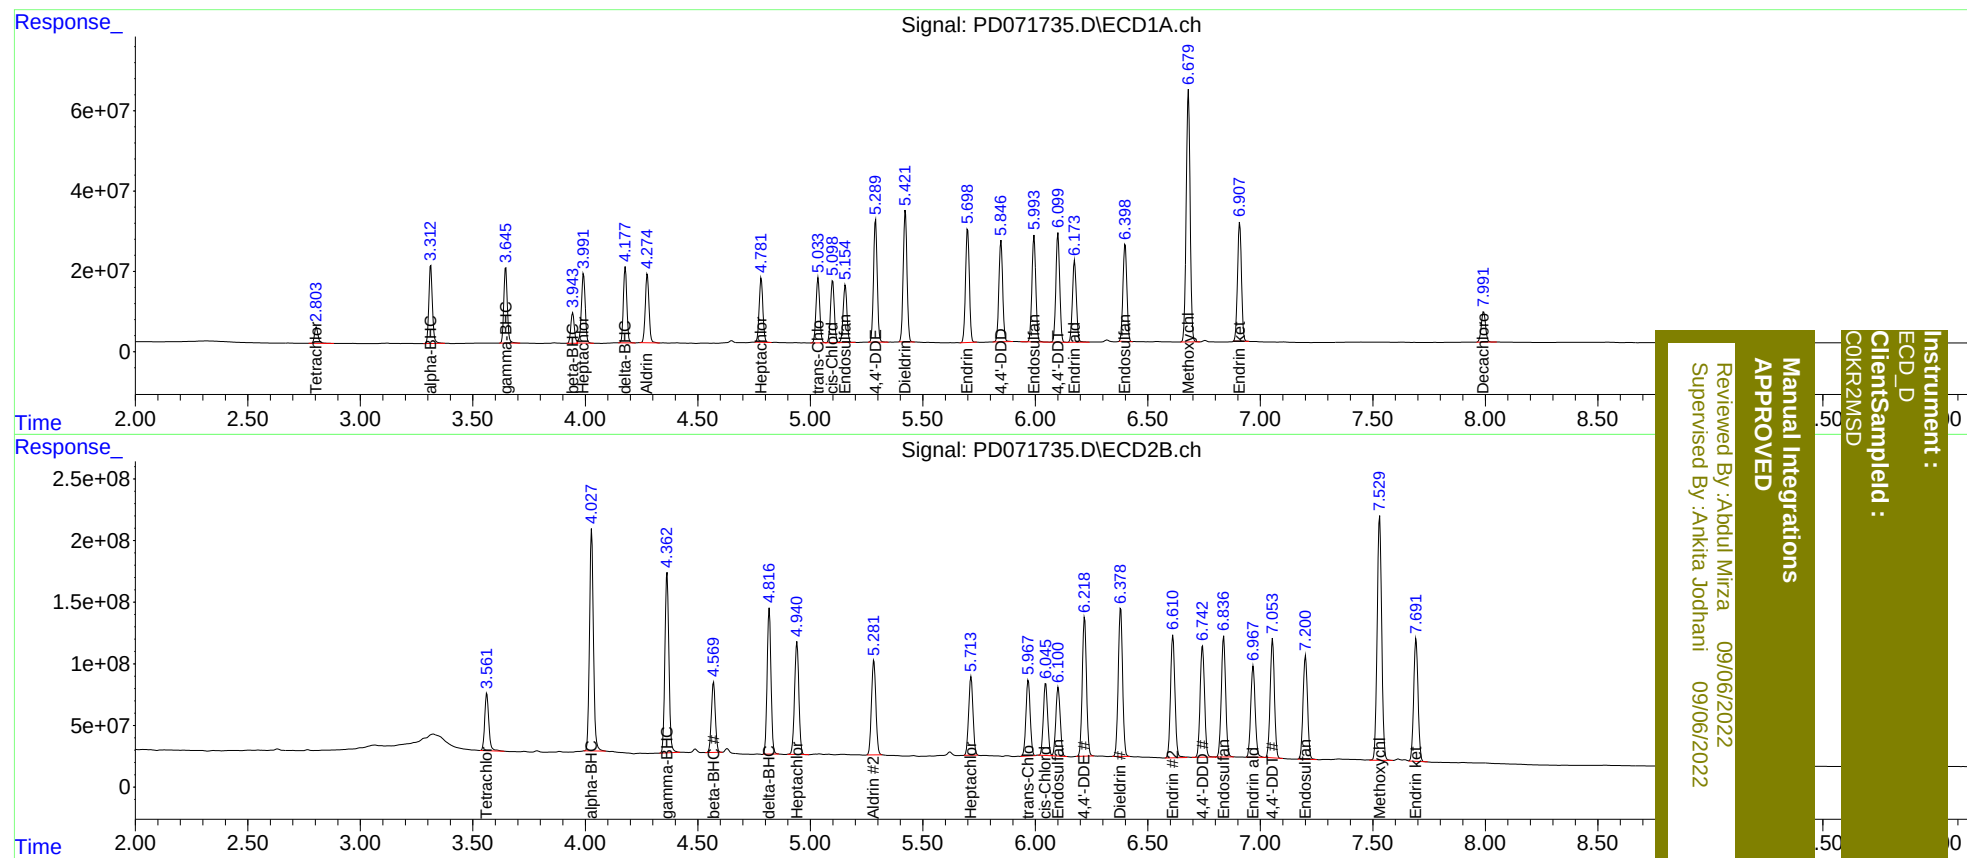

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/06/2022
Supervised By: Ankita Jodhani 09/06/2022

Instrument :
ECD_D
Client Sampled :
COKR2MSD