

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090222\
 Data File : PD071724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 18:27
 Operator : AR\AJ
 Sample : N4482-05MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW345MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/06/2022
 Supervised By : Ankita Jodhani 09/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 02:07:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 07:11:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.812	3.563	42892487	556.2E6	16.447	16.974
27)	SA Decachlor...	8.001	9.088	83072377	316.9E6	31.656	33.154
Target Compounds							
2)	A alpha-BHC	3.321	4.029	215.8E6	2221.5E6	55.951	50.350
3)	MA gamma-BHC...	3.655	4.365	203.8E6	1828.4E6	55.205	49.160
4)	MA Heptachlor	3.999	4.942	200.5E6	1232.8E6	52.684m	45.656
5)	MB Aldrin	4.285	5.285	198.7E6	1053.1E6	55.819	48.748
6)	B beta-BHC	3.952	4.571	80526974	701.9E6	50.694m	49.038
7)	B delta-BHC	4.187	4.819	202.6E6	1288.7E6	57.991	49.031
8)	B Heptachlo...	4.791	5.716	184.5E6	853.0E6	56.600	50.443
9)	A Endosulfan I	5.164	6.104	169.3E6	781.3E6	53.732	49.750
10)	B trans-Chl...	5.043	5.971	183.7E6	825.6E6	54.261	48.773
11)	B cis-Chlor...	5.108	6.048	180.6E6	811.0E6	54.137	49.755
12)	B 4,4'-DDE	5.299	6.221	346.0E6	1481.4E6	112.795	101.518
13)	MA Dieldrin	5.431	6.381	385.0E6	1625.5E6	111.187	101.567
14)	MA Endrin	5.708	6.614	338.1E6	1376.2E6	112.905	104.597
15)	B Endosulfa...	6.003	6.839	318.7E6	1328.0E6	119.884	110.171
16)	A 4,4'-DDD	5.857	6.745	291.5E6	1248.6E6	110.742	102.036
17)	MA 4,4'-DDT	6.109	7.057	310.9E6	1262.7E6	114.189	104.652
18)	B Endrin al...	6.183	6.970	249.0E6	1038.2E6	107.626	101.758
19)	B Endosulfa...	6.407	7.203	297.0E6	1189.7E6	111.468	104.757
20)	A Methoxychlor	6.689	7.533	774.2E6	2770.1E6	539.053	504.851
21)	B Endrin ke...	6.917	7.694	363.4E6	1363.6E6	121.434	110.157

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090222\
Data File : PD071724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 18:27
Operator : AR\AJ
Sample : N4482-05MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 02:07:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

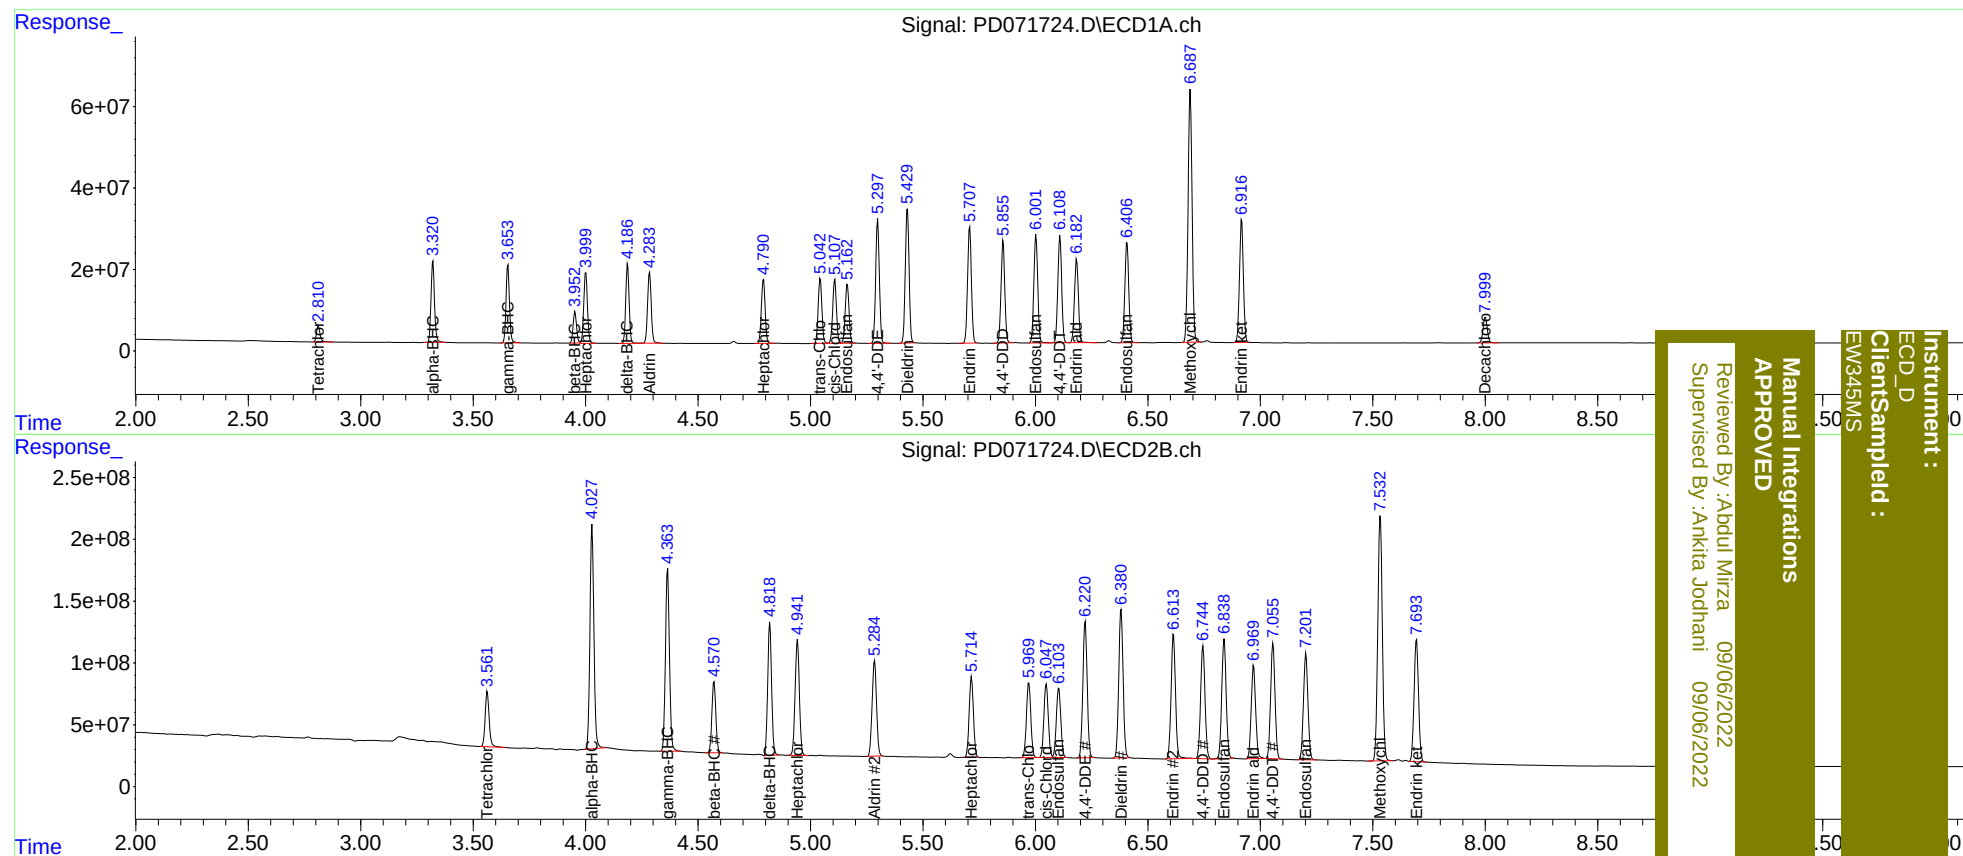

Reviewed By: Abdul Mirza 09/06/2022
Supervised By: Ankita Jodhani 09/06/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EW/345MS