

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090222\
 Data File : PD071732.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Sep 2022 20:14
 Operator : AR\AJ
 Sample : PB147465BS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS465

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/06/2022
 Supervised By : Ankita Jodhani 09/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 03 02:09:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 07:11:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.804	3.562	42120496	531.9E6	16.151	16.232
27)	SA Decachlor...	7.993	9.083	89358459	335.2E6	34.051	35.070m
Target Compounds							
2)	A alpha-BHC	3.312	4.028	14430955	193.5E6	3.741	4.387
3)	MA gamma-BHC...	3.645	4.363	14943119	172.7E6	4.048	4.644
4)	MA Heptachlor	3.990	4.940	15011309	129.5E6	3.944m	4.796
5)	MB Aldrin	4.275	5.282	15426436	111.2E6	4.333	5.145
6)	B beta-BHC	3.943	4.570	7275446	68232201	4.580m	4.767
7)	B delta-BHC	4.177	4.816	12771531	111.0E6	3.655	4.222m
8)	B Heptachlo...	4.781	5.714	14715577	103.7E6	4.515	6.132 #
9)	A Endosulfan I	5.155	6.102	13644952	77613197	4.329	4.942
10)	B trans-Chl...	5.035	5.969	15008045	82957638	4.433	4.901
11)	B cis-Chlor...	5.099	6.046	15002305	81777515	4.498	5.017
12)	B 4,4'-DDE	5.290	6.219	25817778	146.1E6	8.417	10.010
13)	MA Dieldrin	5.422	6.379	29305338	156.8E6	8.462	9.795
14)	MA Endrin	5.699	6.609	26341580	114.1E6	8.795	8.675m
15)	B Endosulfa...	5.994	6.837	25452713	127.1E6	9.576	10.548
16)	A 4,4'-DDD	5.848	6.743	22644395	119.9E6	8.603	9.802
17)	MA 4,4'-DDT	6.101	7.055	22972090	121.0E6	8.439	10.025
18)	B Endrin al...	6.175	6.968	20333308	95739952	8.790	9.384
19)	B Endosulfa...	6.399	7.201	23842141	108.3E6	8.950	9.537
20)	A Methoxychlor	6.680	7.531	68518332	303.6E6	47.705	55.335
21)	B Endrin ke...	6.908	7.693	29012387	133.5E6	9.695	10.783

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090222\
Data File : PD071732.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Sep 2022 20:14
Operator : AR\AJ
Sample : PB147465BS
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 03 02:09:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

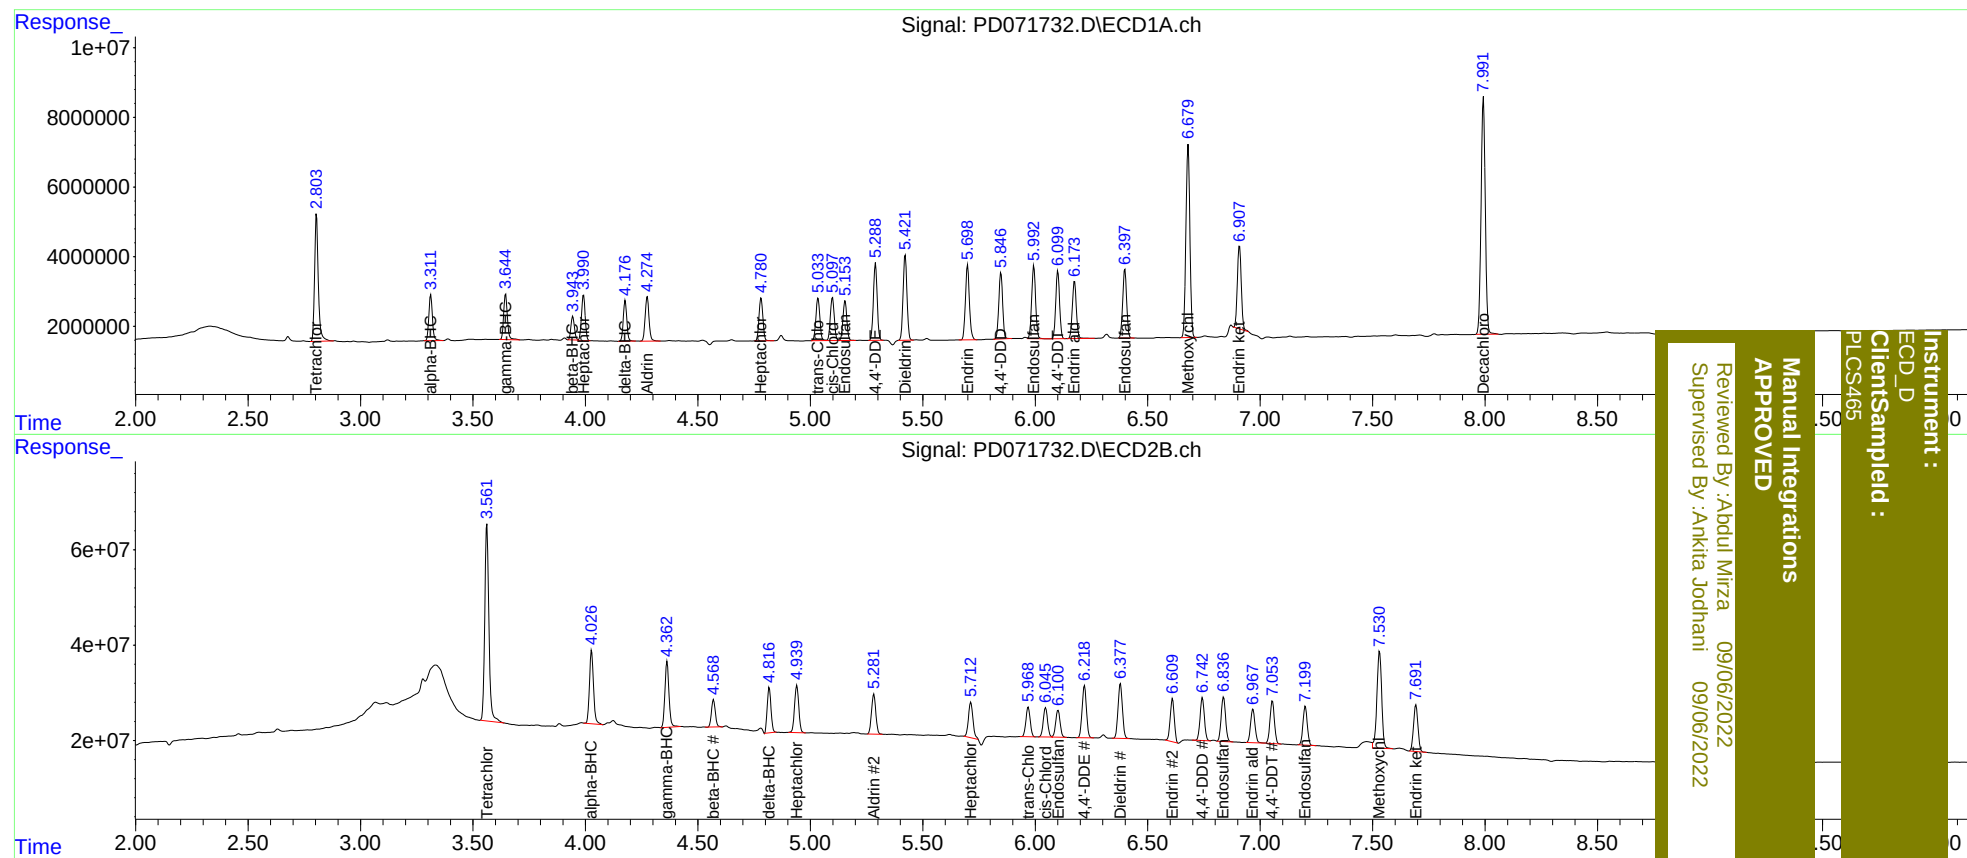

Reviewed By: Abdul Mirza 09/06/2022
Supervised By: Ankita Jodhani 09/06/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
PLCS465