

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090223\
 Data File : PD077553.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2023 01:28
 Operator : AR\AJ
 Sample : 04227-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 05:46:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.761	40581556	24813677	18.485	19.919
27)	SA Decachlor...	9.081	7.899	36555905	20013767	14.366	16.056
Target Compounds							
6)	B beta-BHC	0.000	3.845f	0	401527	N.D.	0.492
9)	A Endosulfan I	0.000	5.124f	0	371166	N.D.	0.263


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090223\
Data File : PD077553.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2023 01:28
Operator : AR\AJ
Sample : 04227-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 05:46:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

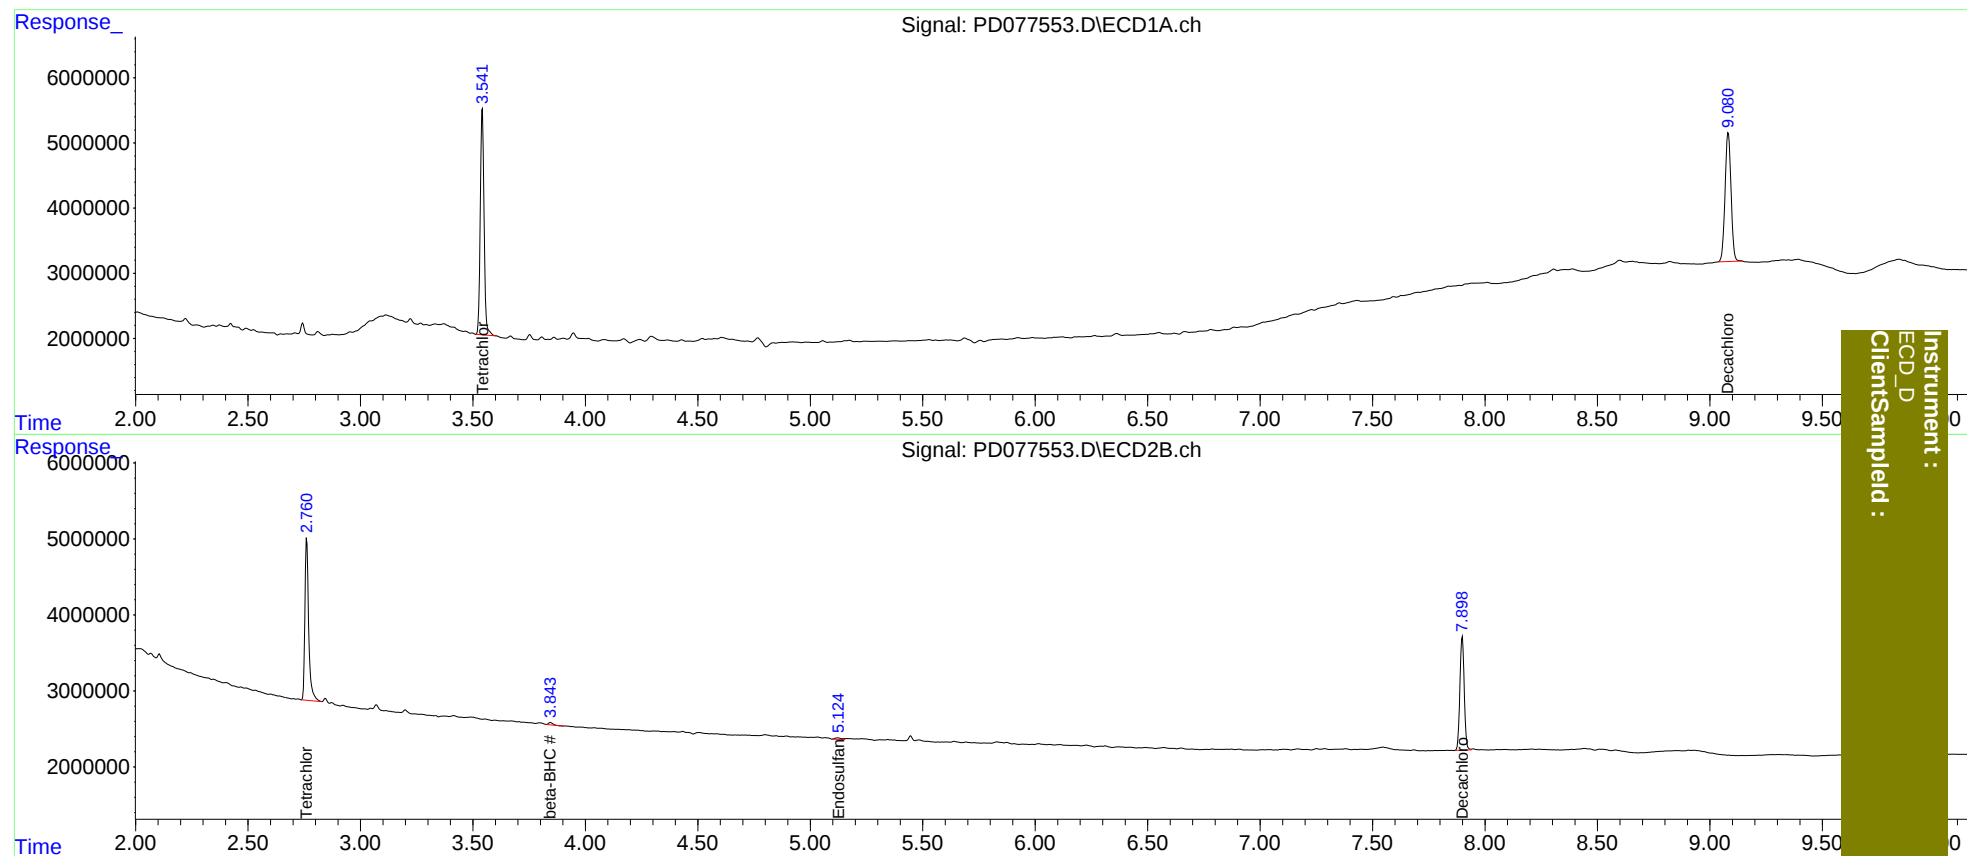


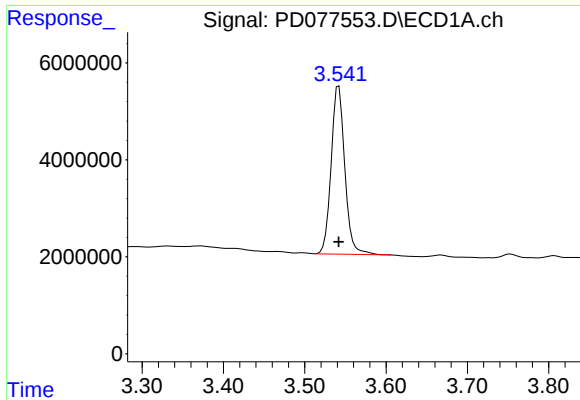

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 40581556
Conc: 18.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

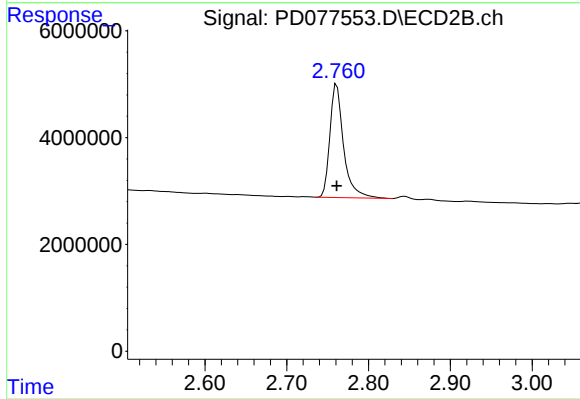


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 24813677
Conc: 19.92 ng/ml

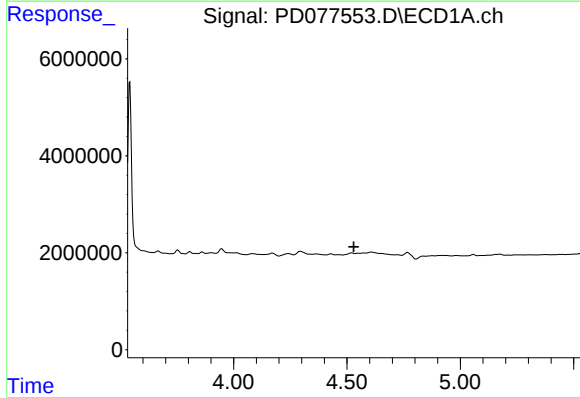


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.530 min
Response: 0
Conc: N.D.

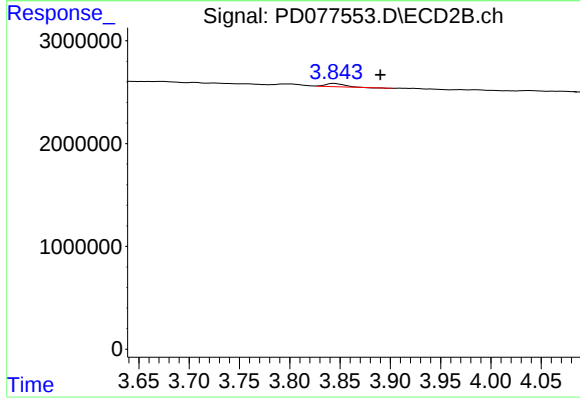

#6 beta-BHC


R.T.: 3.845 min
Delta R.T.: -0.045 min
Response: 401527
Conc: 0.49 ng/ml

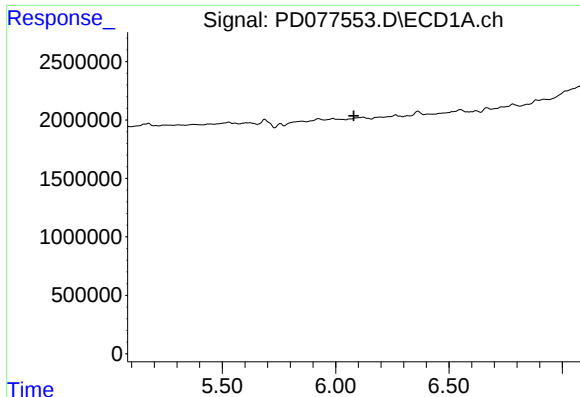

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.080 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

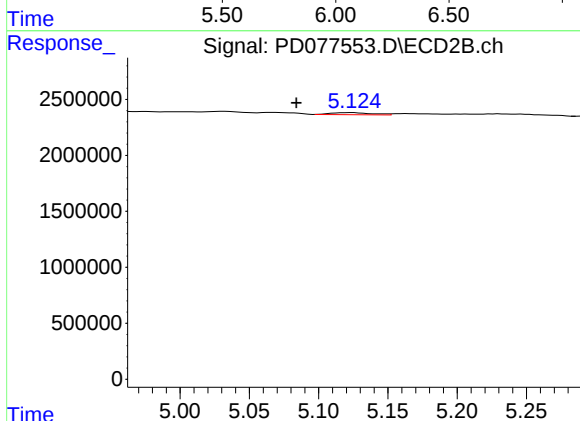


#9 Endosulfan I

R.T.: 5.124 min
Delta R.T.: 0.040 min
Response: 371166
Conc: 0.26 ng/ml

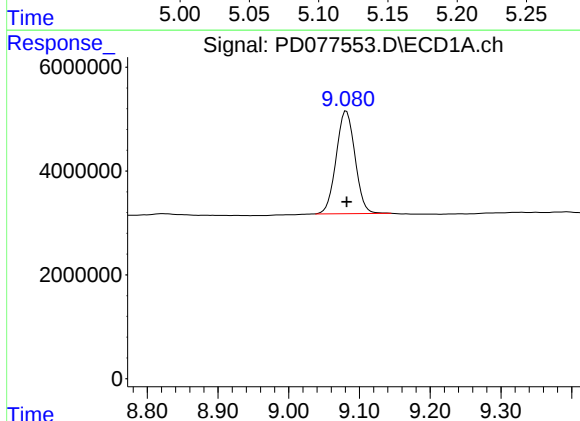

#27 Decachlorobiphenyl

R.T.: 9.081 min
Delta R.T.: 0.000 min
Response: 36555905
Conc: 14.37 ng/ml

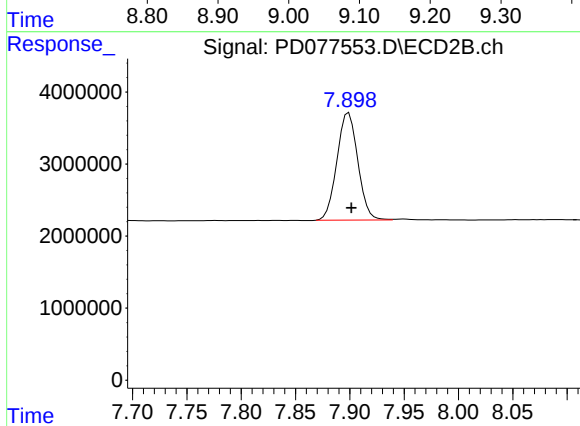

#27 Decachlorobiphenyl

R.T.: 7.899 min
Delta R.T.: -0.002 min
Response: 20013767
Conc: 16.06 ng/ml