

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090223\
 Data File : PD077543.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2023 23:15
 Operator : AR\AJ
 Sample : 04227-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BBKE0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/01/2023
 Supervised By : Ankita Jodhani 09/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 01:00:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.762	45606209	32181622	20.774	25.833
27)	SA Decachlor...	9.081	7.900	51861891	29623443	20.381	23.765
Target Compounds							
9)	A Endosulfan I	6.090	5.054	6985728	2465298	2.471m	1.750 #
11)	B cis-Chlor...	6.023	5.029	2322462	2774653	0.725m	1.723m#
13)	MA Dieldrin	6.352	5.348	9504908	4628374	3.049m	2.918
16)	A 4,4'-DDD	6.719	5.769	11525933	6217390	5.303m	6.252m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090223\
Data File : PD077543.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2023 23:15
Operator : AR\AJ
Sample : 04227-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 01:00:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

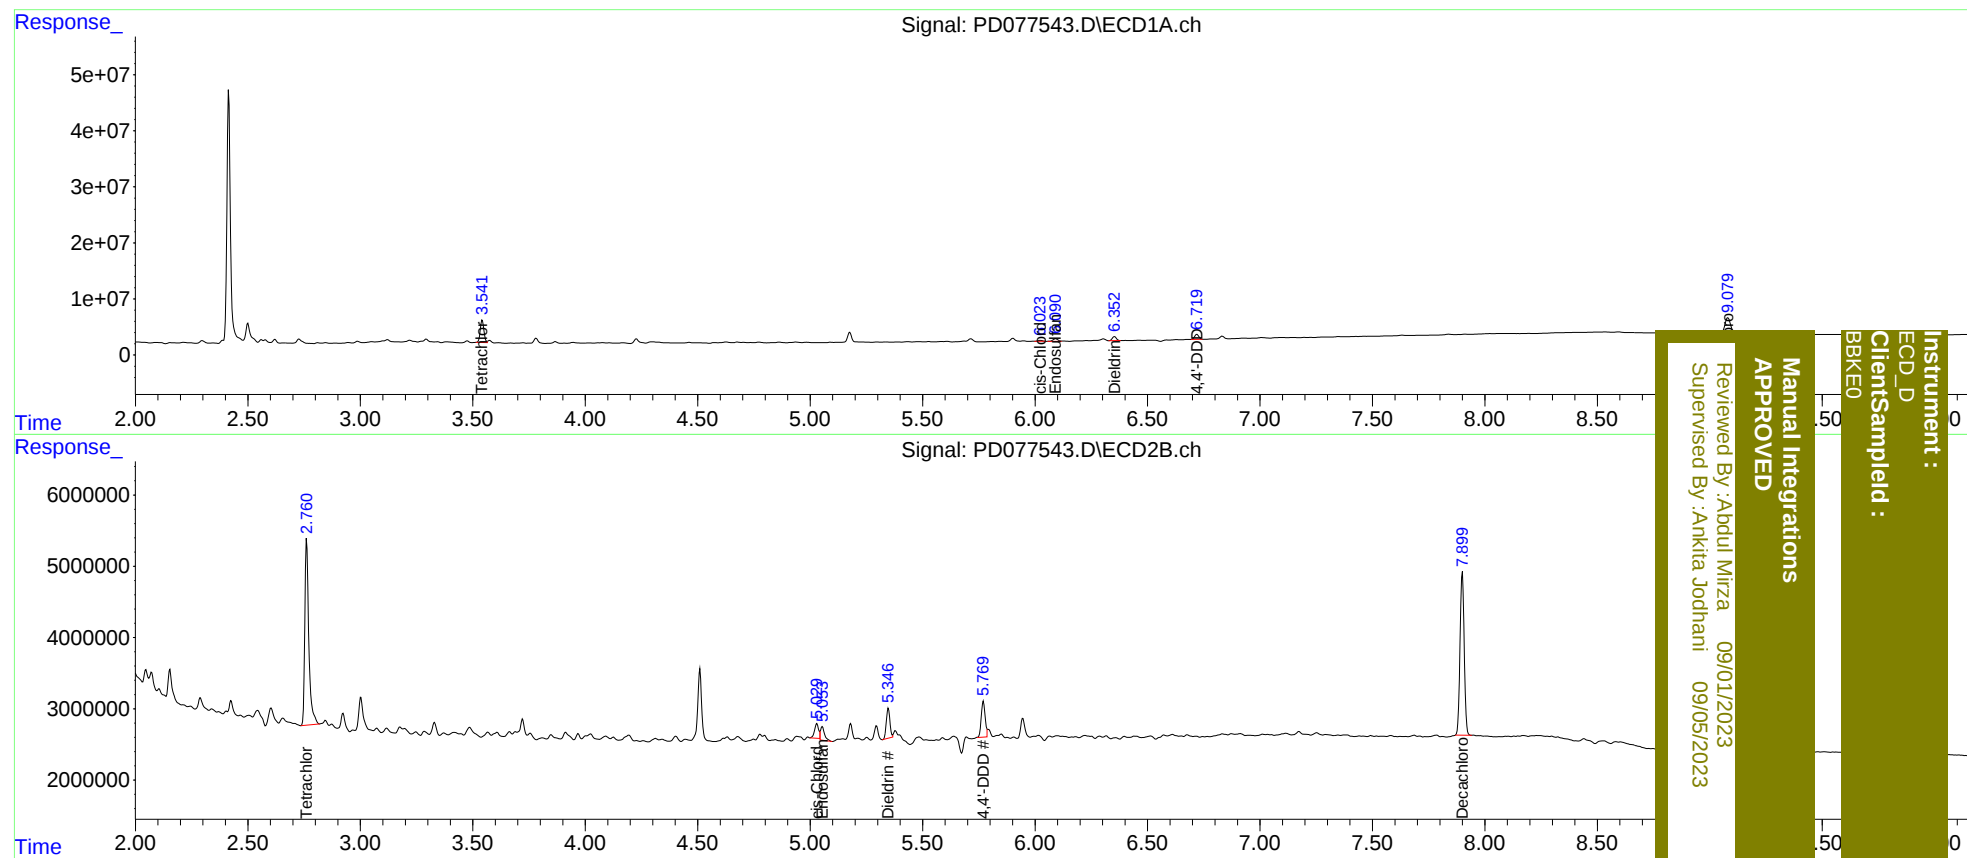

Reviewed By: Abdul Mirza 09/01/2023
Supervised By: Ankita Jodhani 09/05/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BBKEO