

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090324\
 Data File : PD084857.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2024 10:37
 Operator : AR\AJ
 Sample : P3673-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:08:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.903	11100484	38153965	10.975	10.782
2)	SA Decachlor...	9.040	8.110	13272646	27992157	10.163	8.050
Target Compounds							
7)	B delta-BHC	4.768f	0.000	4288343	0	2.615	N.D. #
19)	B Endosulfa...	0.000	6.532	0	9392941	N.D.	2.630


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090324\
Data File : PD084857.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2024 10:37
Operator : AR\AJ
Sample : P3673-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:08:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

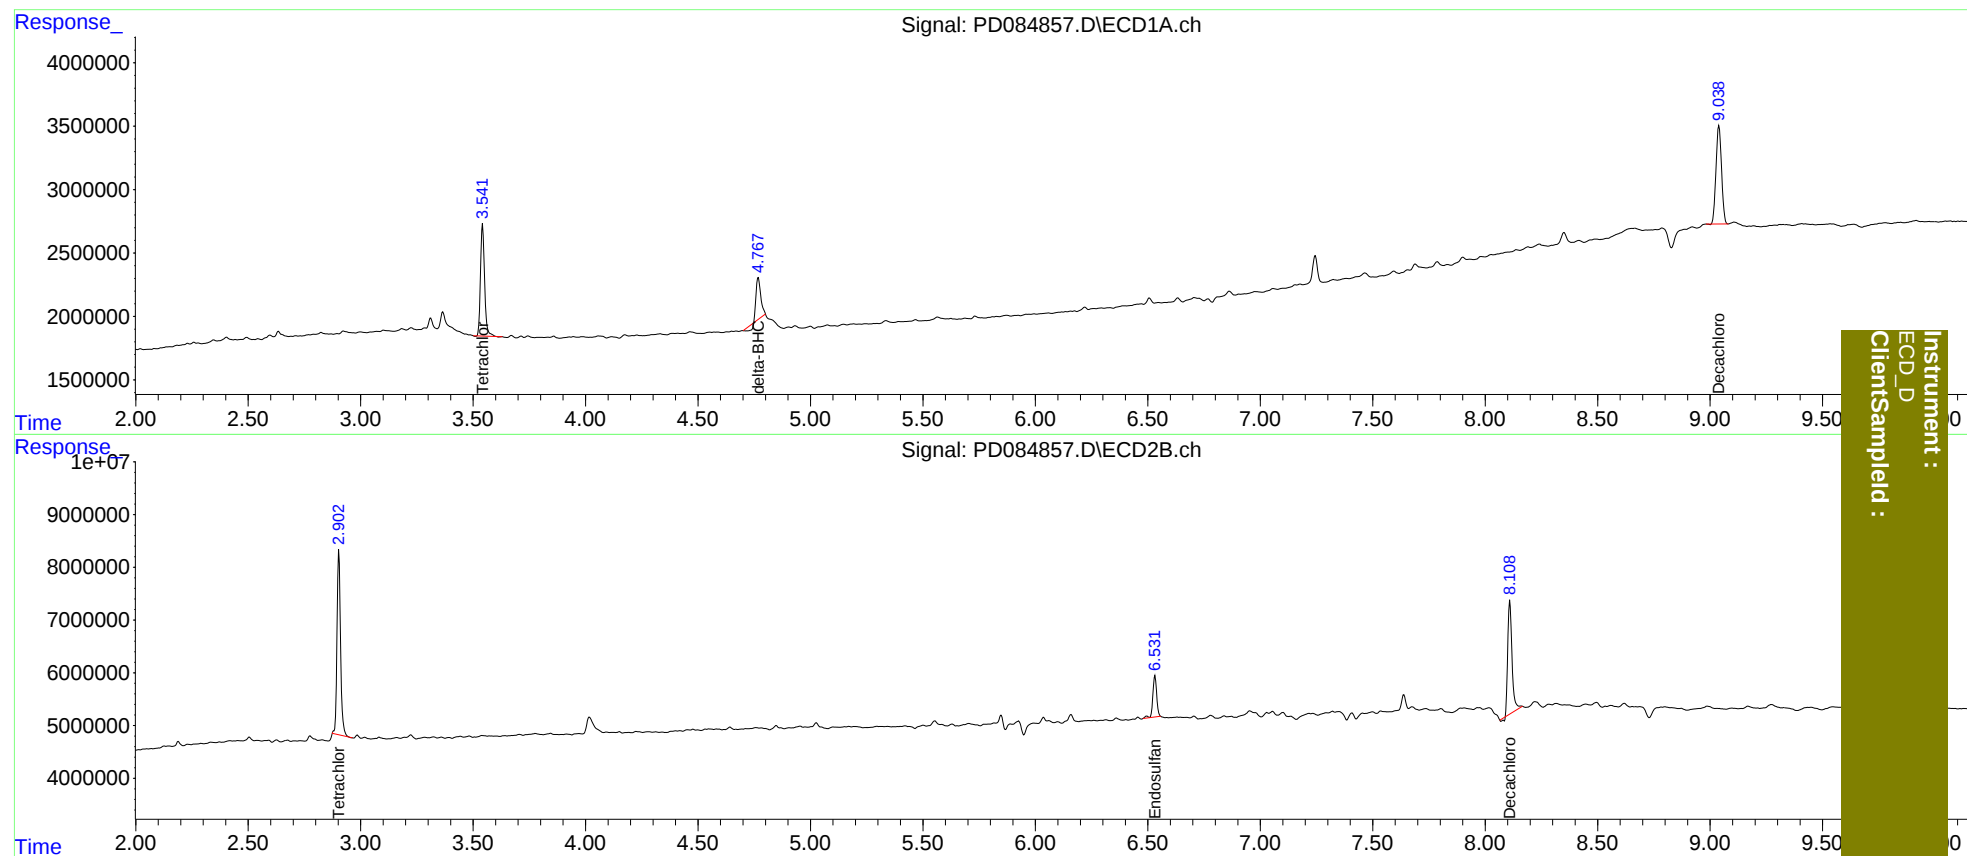


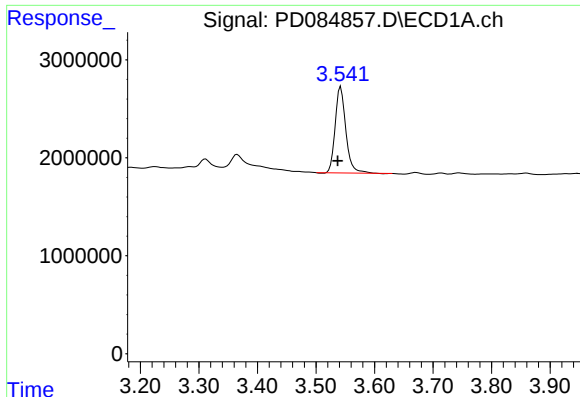

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.005 min
Response: 11100484
Conc: 10.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

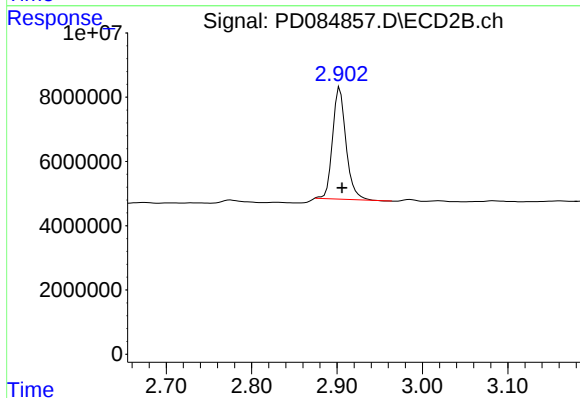


#1 Tetrachloro-m-xylene

R.T.: 2.903 min
Delta R.T.: -0.002 min
Response: 38153965
Conc: 10.78 ng/ml

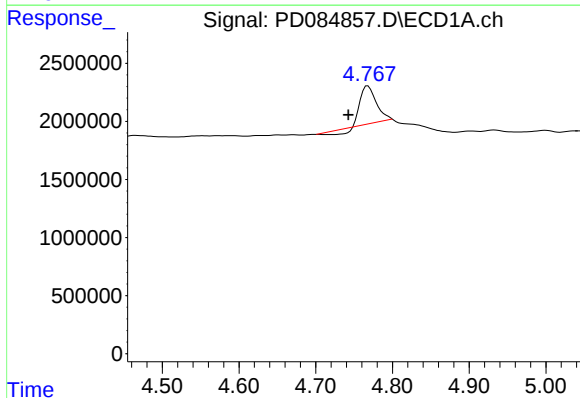


#7 delta-BHC

R.T.: 4.768 min
Delta R.T.: 0.026 min
Response: 4288343
Conc: 2.61 ng/ml

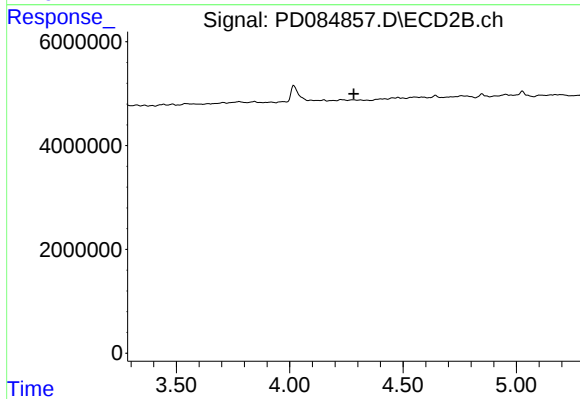

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

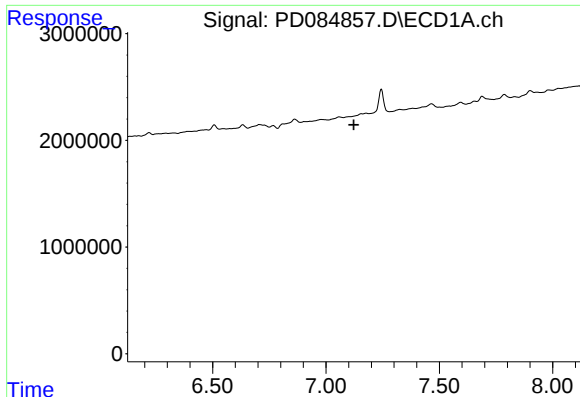

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.123 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

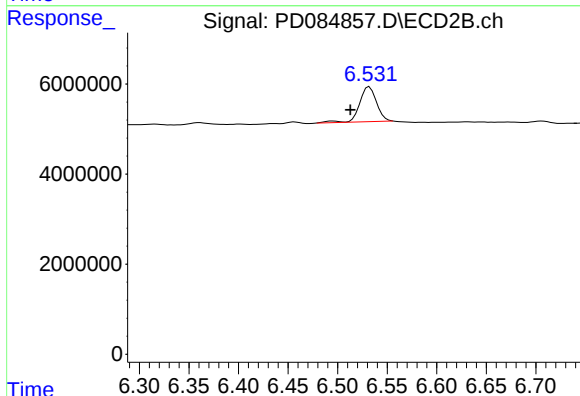


#19 Endosulfan Sulfate

R.T.: 6.532 min
Delta R.T.: 0.019 min
Response: 9392941
Conc: 2.63 ng/ml

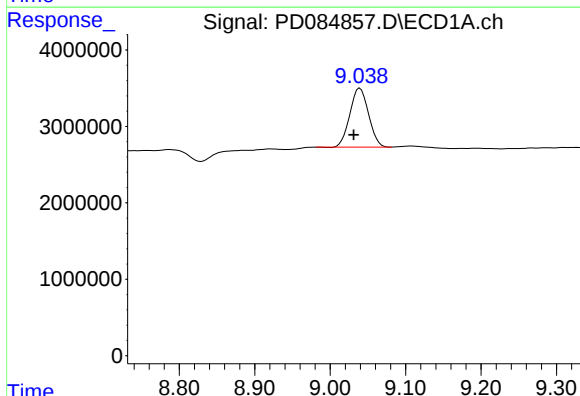

#27 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.008 min
Response: 13272646
Conc: 10.16 ng/ml

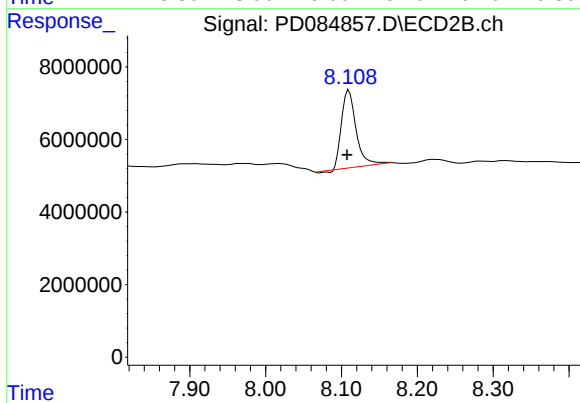

#27 Decachlorobiphenyl

R.T.: 8.110 min
Delta R.T.: 0.002 min
Response: 27992157
Conc: 8.05 ng/ml