

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090324\
 Data File : PD084867.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2024 14:10
 Operator : AR\AJ
 Sample : P3675-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:10:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.906	17505976	60779989	17.309	17.175
27)	SA Decachlor...	9.041	8.109	18314496	49772865	14.023	14.314
Target Compounds							
4)	MA Heptachlor	4.904	0.000	2442777	0	1.588	N.D. #
7)	B delta-BHC	4.765	0.000	32547257	0	19.846	N.D. #
10)	B trans-Chl...	5.930	5.179	3004153	23638489	2.130	5.747 #
11)	B cis-Chlor...	0.000	5.179f	0	23638489	N.D.	5.634
22)	Toxaphene-1	0.000	5.179	0	23638489	N.D.	932.347


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090324\
Data File : PD084867.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2024 14:10
Operator : AR\AJ
Sample : P3675-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:10:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

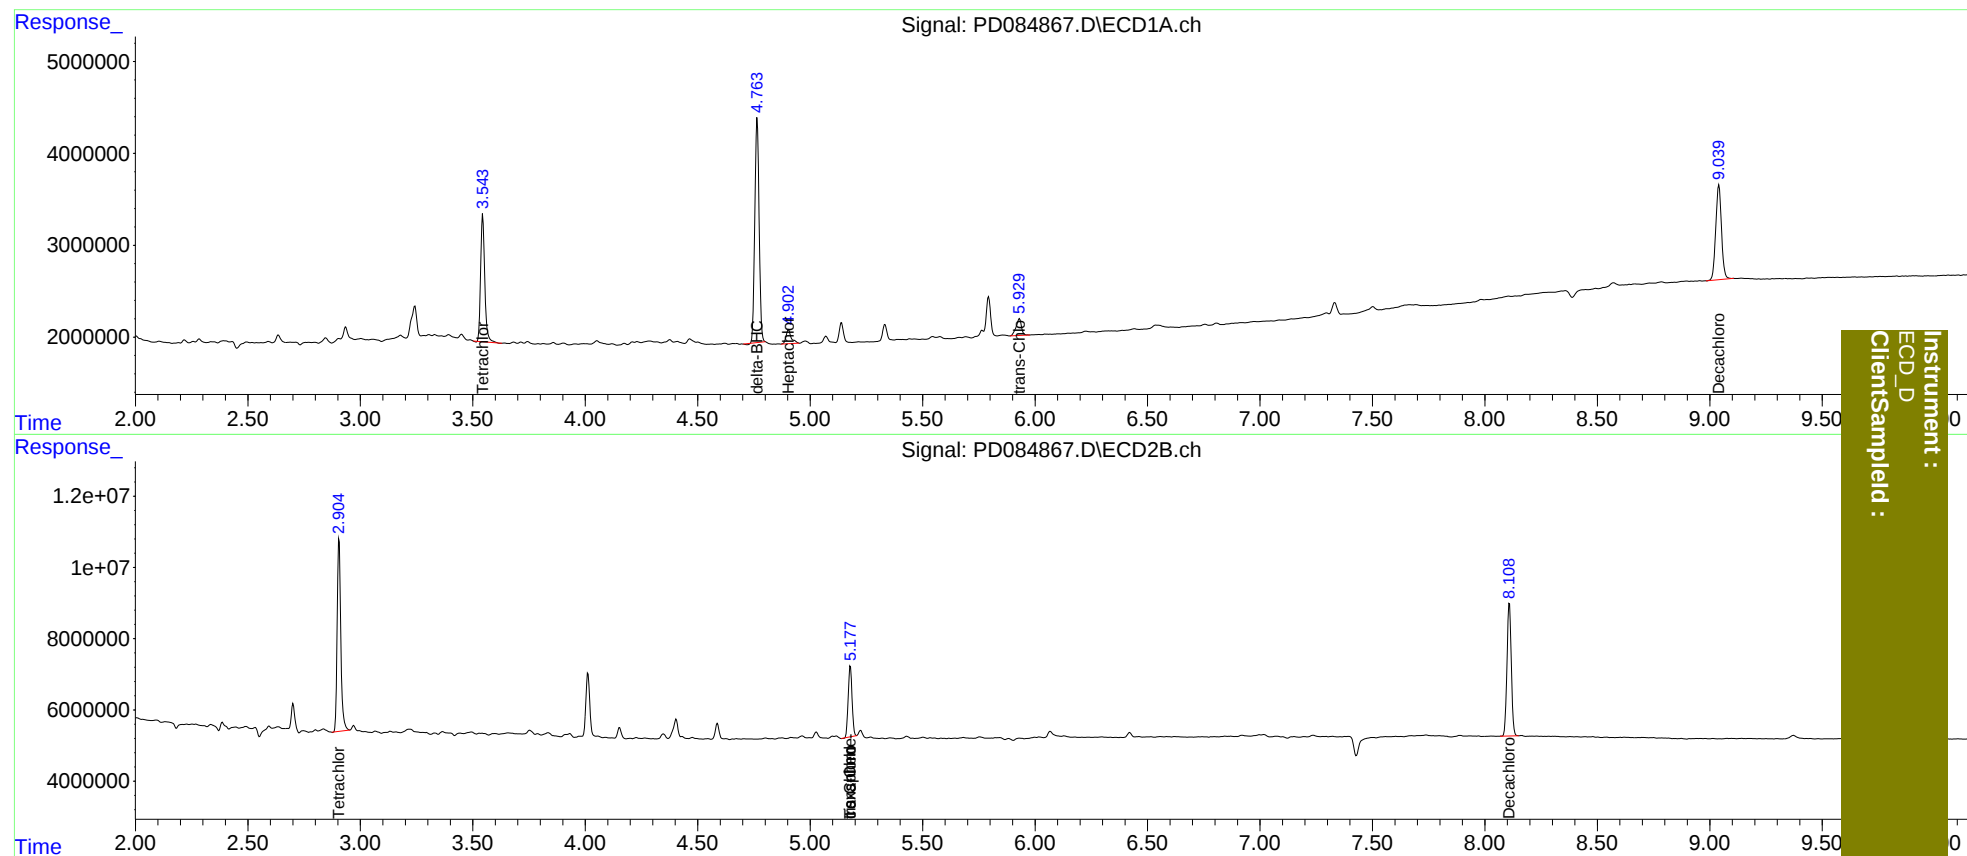


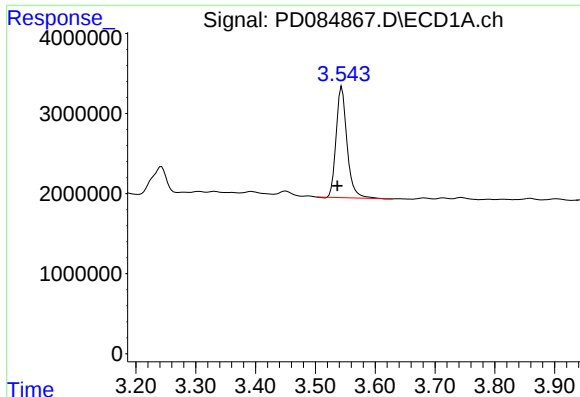

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.007 min
Response: 17505976
Conc: 17.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

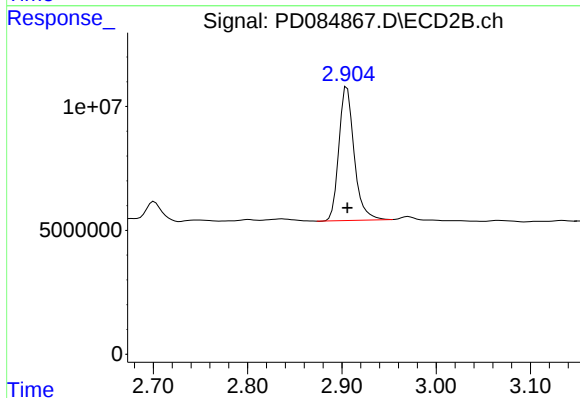


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 60779989
Conc: 17.18 ng/ml

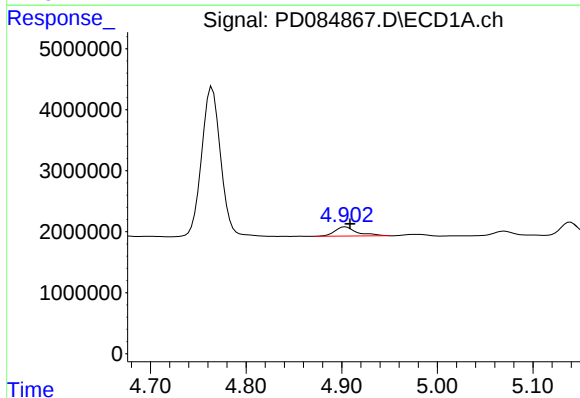


#4 Heptachlor

R.T.: 4.904 min
Delta R.T.: -0.005 min
Response: 2442777
Conc: 1.59 ng/ml

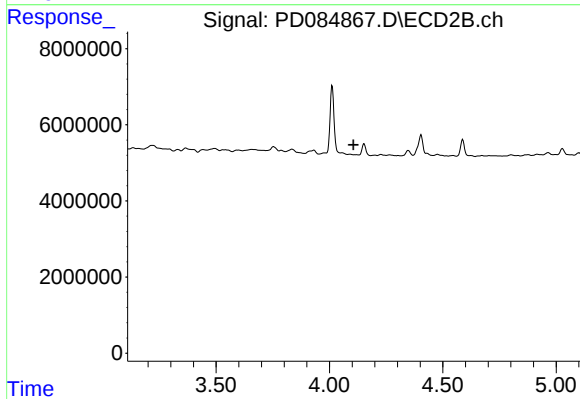

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.107 min
Response: 0
Conc: N.D.

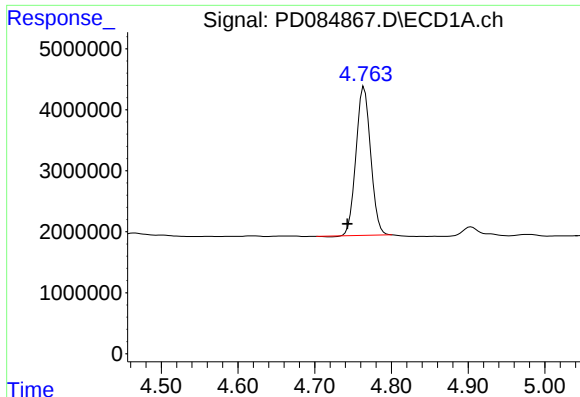

#7 delta-BHC


R.T.: 4.765 min
Delta R.T.: 0.022 min
Response: 32547257
Conc: 19.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

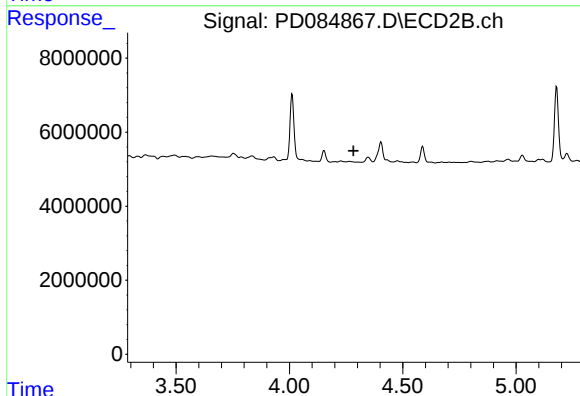


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

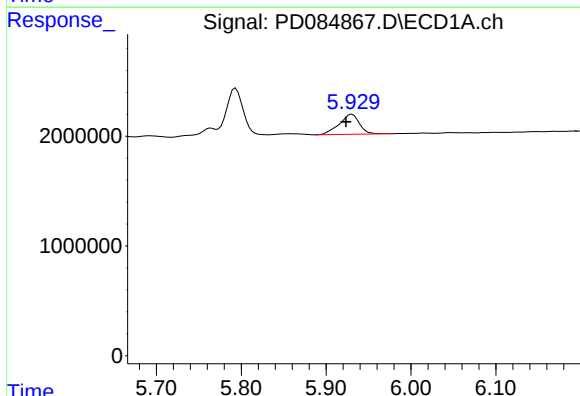


#10 trans-Chlordane

R.T.: 5.930 min
Delta R.T.: 0.007 min
Response: 3004153
Conc: 2.13 ng/ml

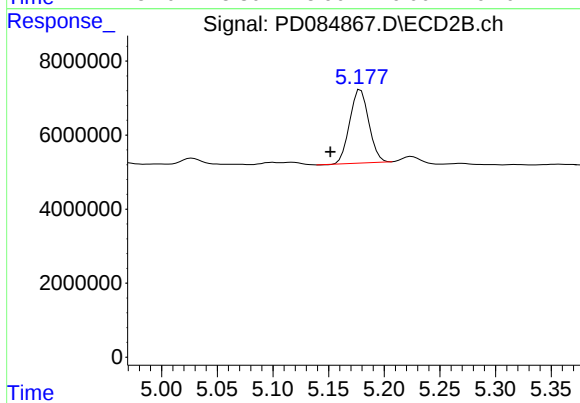

#10 trans-Chlordane


R.T.: 5.179 min
Delta R.T.: 0.027 min
Response: 23638489
Conc: 5.75 ng/ml

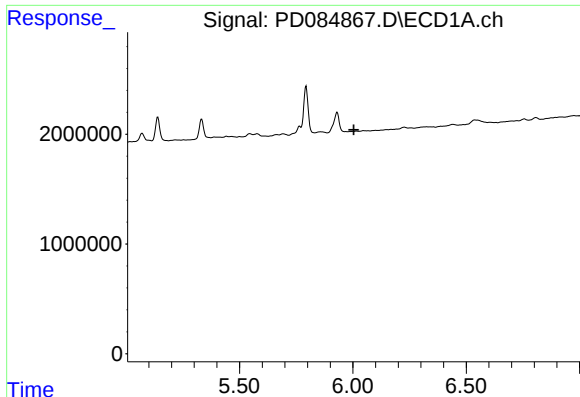

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

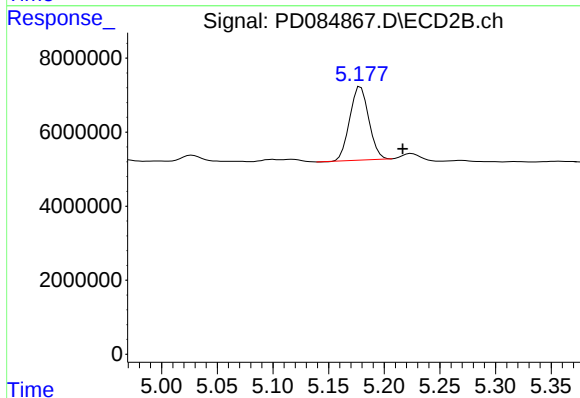


#11 cis-Chlordane

R.T.: 5.179 min
Delta R.T.: -0.038 min
Response: 23638489
Conc: 5.63 ng/ml

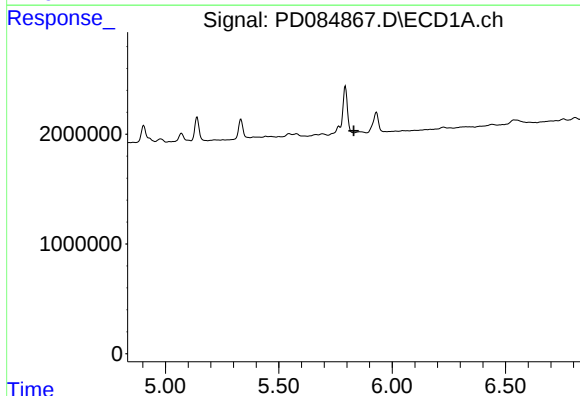


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T.: 5.831 min
Response: 0
Conc: N.D.

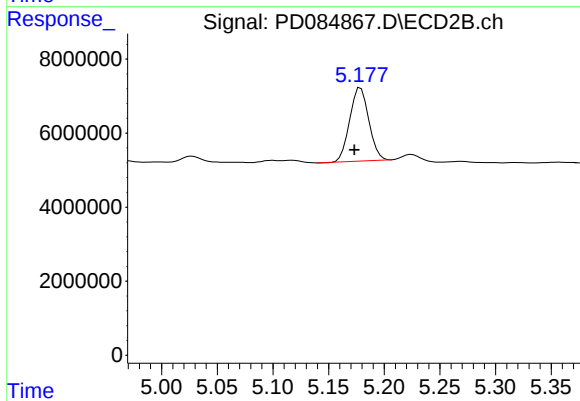

#22 Toxaphene-1


R.T.: 5.179 min
Delta R.T.: 0.006 min
Response: 23638489
Conc: 932.35 ng/ml

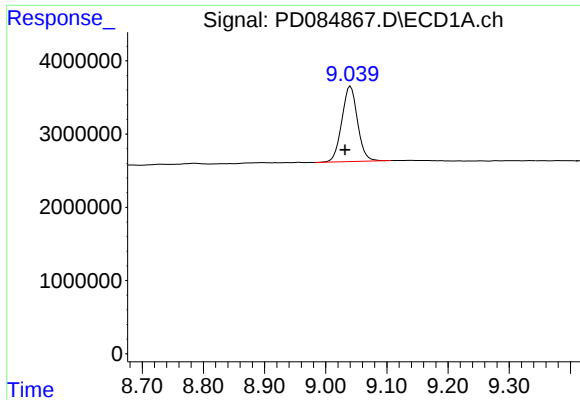

#27 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.009 min
Response: 18314496
Conc: 14.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

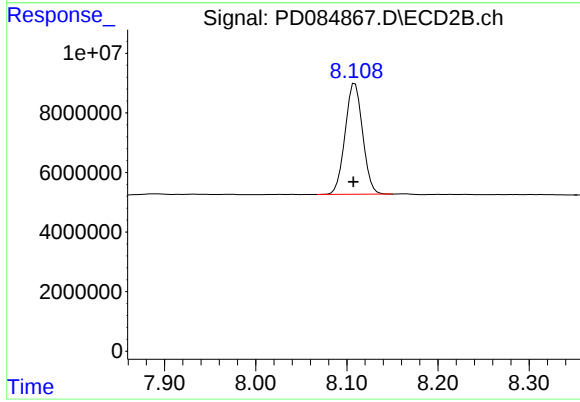

#27 Decachlorobiphenyl

R.T.: 8.109 min
Delta R.T.: 0.002 min
Response: 49772865
Conc: 14.31 ng/ml