

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090324\
 Data File : PD084873.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2024 15:30
 Operator : AR\AJ
 Sample : P3711-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:12:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.907	20028820	69695570	19.803	19.695
27)	SA Decachlor...	9.033	8.106	28686861	77930771	21.965	22.412
Target Compounds							
20)	A Methoxychlor	7.490	0.000	597813	0	1.148	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090324\
Data File : PD084873.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2024 15:30
Operator : AR\AJ
Sample : P3711-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:12:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

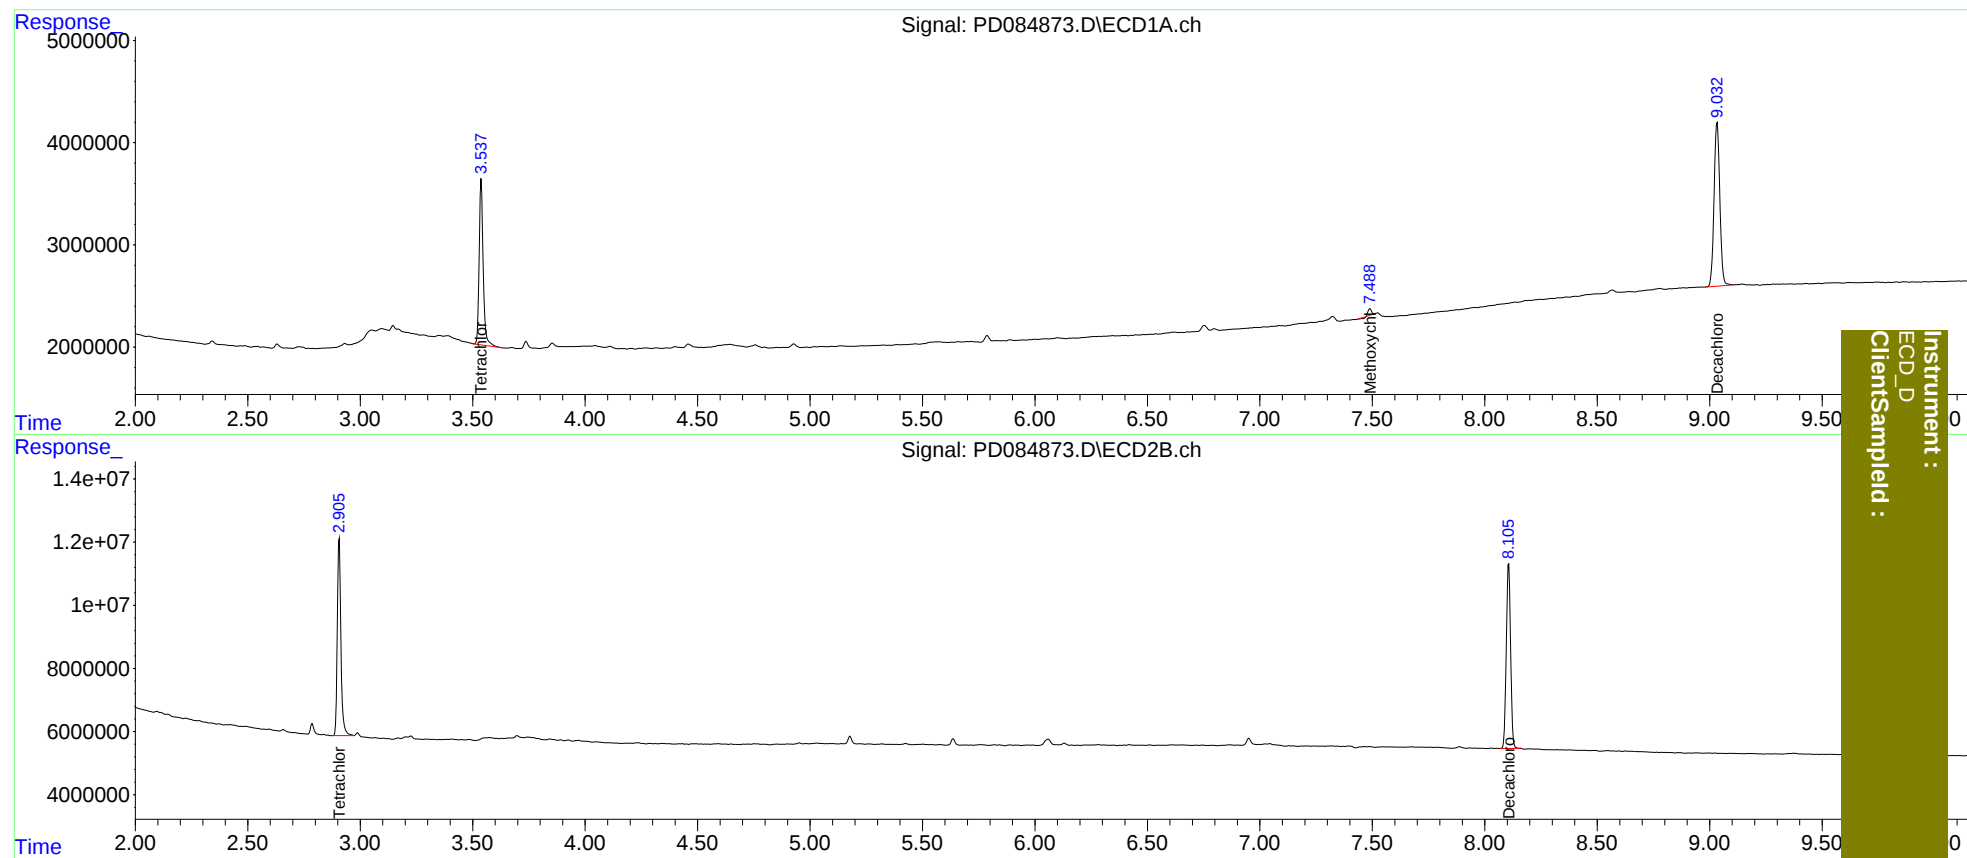


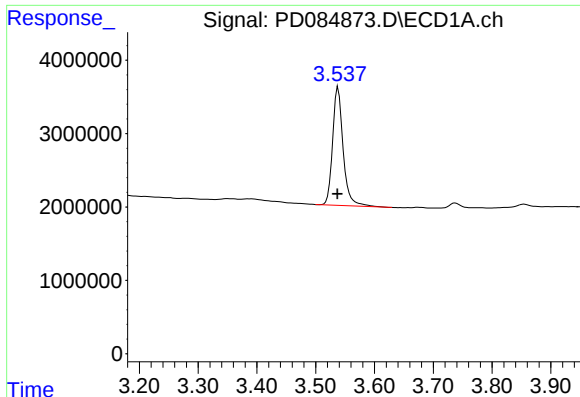

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.001 min
Response: 20028820
Conc: 19.80 ng/ml

Instrument :
ECD_D
ClientSampleId :

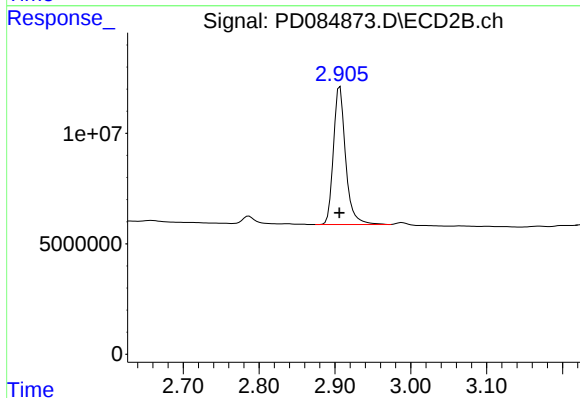


#1 Tetrachloro-m-xylene

R.T.: 2.907 min
Delta R.T.: 0.000 min
Response: 69695570
Conc: 19.69 ng/ml

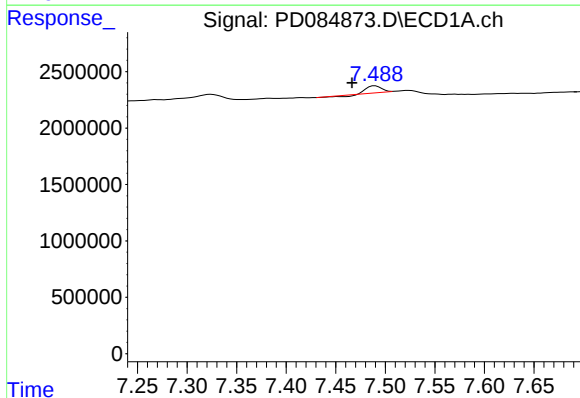


#20 Methoxychlor

R.T.: 7.490 min
Delta R.T.: 0.023 min
Response: 597813
Conc: 1.15 ng/ml

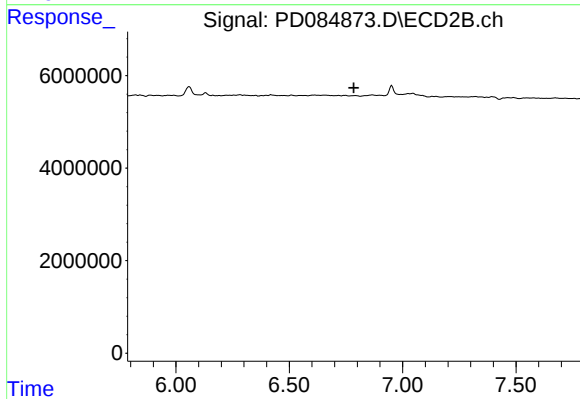

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.785 min
Response: 0
Conc: N.D.

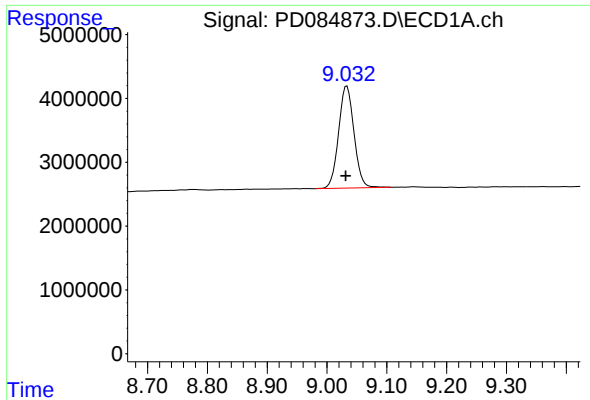

#27 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: 0.002 min
Response: 28686861
Conc: 21.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

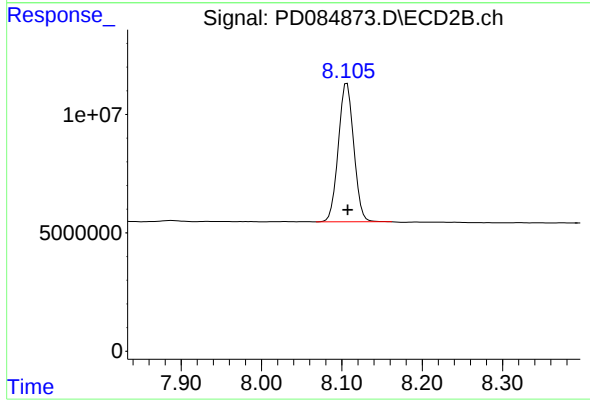

#27 Decachlorobiphenyl

R.T.: 8.106 min
Delta R.T.: 0.000 min
Response: 77930771
Conc: 22.41 ng/ml