

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090324\
 Data File : PD084888.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2024 18:50
 Operator : AR\AJ
 Sample : PIBLK092
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:14:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.537	2.906	21417955	75443357	21.176	21.319
2) SA Decachlor...	9.030	8.105	31080812	86343618	23.798	24.831
Target Compounds						
7) B delta-BHC	4.759	0.000	3775886	0	2.302	N.D. #
14) MA Endrin	6.584	0.000	4239953	0	3.758	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090324\
Data File : PD084888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2024 18:50
Operator : AR\AJ
Sample : PIBLK092
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:14:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

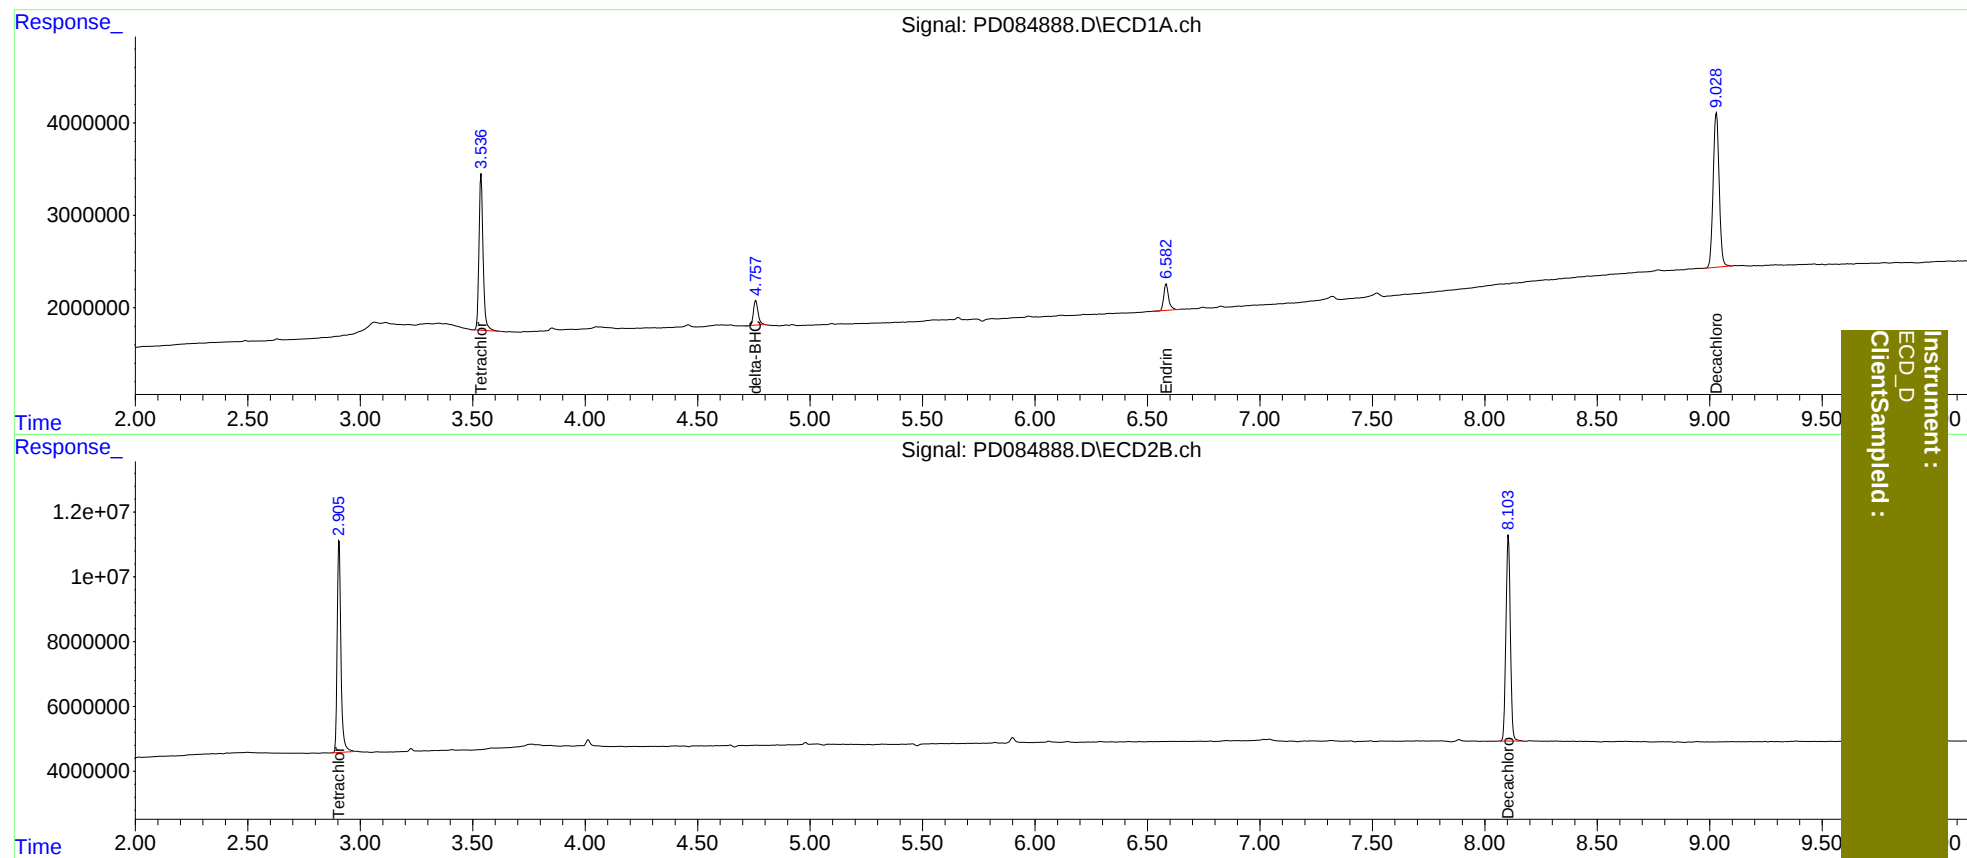


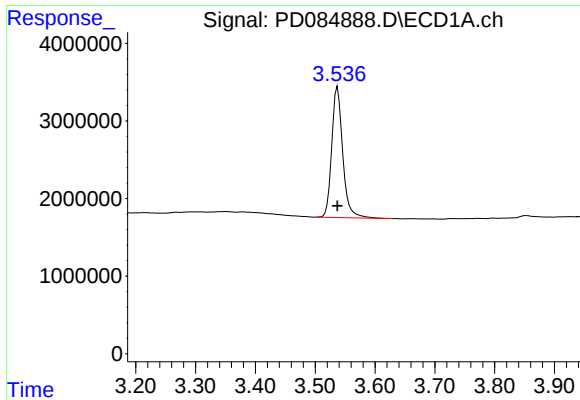

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 21417955
Conc: 21.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

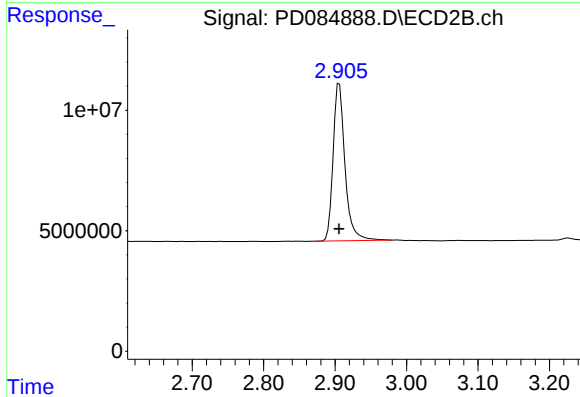


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 75443357
Conc: 21.32 ng/ml

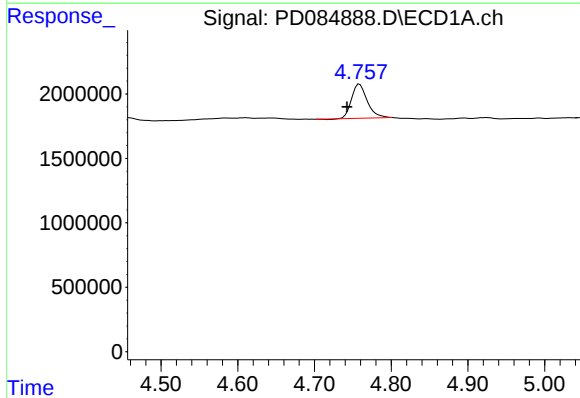


#7 delta-BHC

R.T.: 4.759 min
Delta R.T.: 0.016 min
Response: 3775886
Conc: 2.30 ng/ml

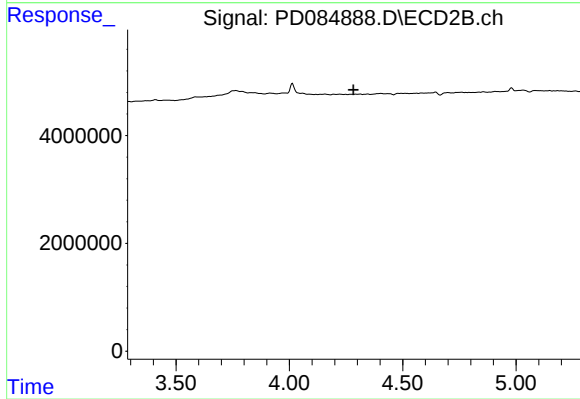

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

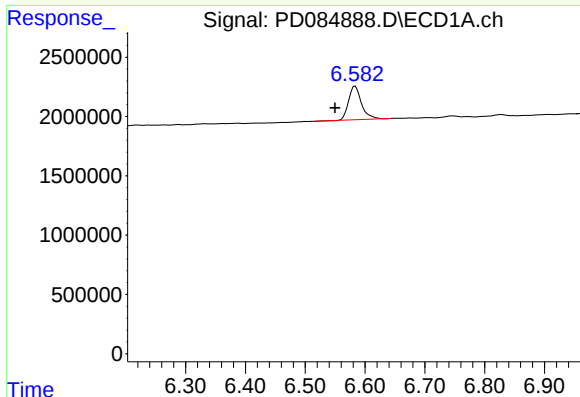

#14 Endrin


R.T.: 6.584 min
Delta R.T.: 0.033 min
Response: 4239953
Conc: 3.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

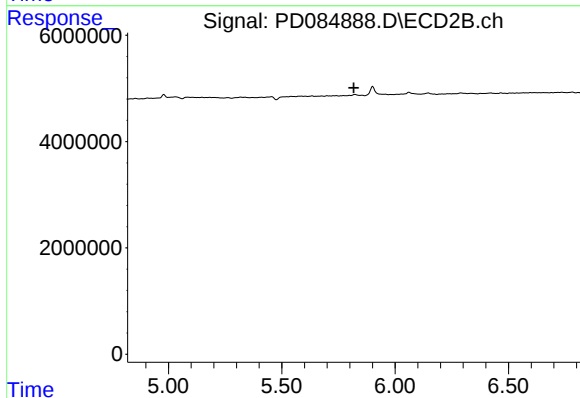


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.817 min
Response: 0
Conc: N.D.

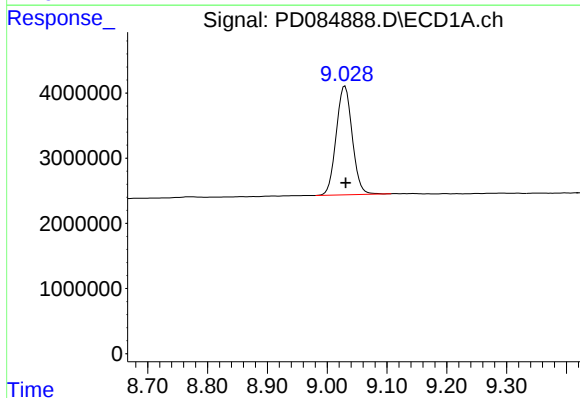

#27 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.002 min
Response: 31080812
Conc: 23.80 ng/ml

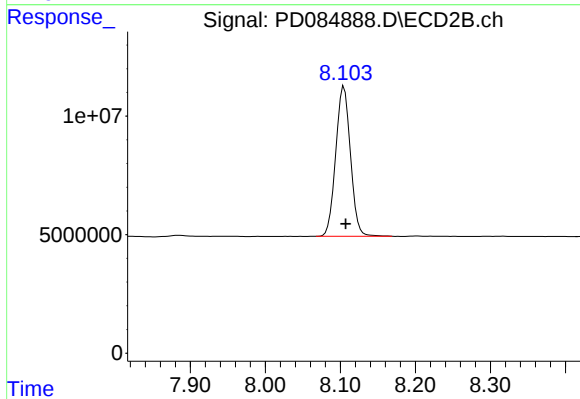

#27 Decachlorobiphenyl

R.T.: 8.105 min
Delta R.T.: -0.003 min
Response: 86343618
Conc: 24.83 ng/ml