

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090324\
 Data File : PD084864.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2024 12:41
 Operator : AR\AJ
 Sample : P3673-22MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCXZ4MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/04/2024
 Supervised By :Ankita Jodhani 09/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:10:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.906	13430129	48360985	13.279	13.666
27)	SA Decachlor...	9.037	8.107	14291552	42496012	10.943	12.221
Target Compounds							
2)	A alpha-BHC	3.985	3.417	109.1E6	298.7E6	64.199m	58.905
3)	MA gamma-BHC...	4.314	3.752	106.5E6	284.1E6	65.849m	58.632
4)	MA Heptachlor	4.913	4.105	102.5E6	260.1E6	66.613	61.098m
5)	MB Aldrin	5.253	4.393	97619122	254.4E6	61.036	57.282
6)	B beta-BHC	4.498	4.044	40314075	122.0E6	55.501	56.261m
7)	B delta-BHC	4.746	4.283	105.0E6	287.9E6	64.033	57.998
8)	B Heptachlo...	5.672	4.897	87226575	233.3E6	58.484	55.079
9)	A Endosulfan I	6.054	5.272	82198816	221.8E6	59.746m	57.852m
10)	B trans-Chl...	5.927	5.152	85501023	234.2E6	60.623	56.930
11)	B cis-Chlor...	6.006	5.216	88220875	235.1E6	59.667m	56.032
12)	B 4,4'-DDE	6.176	5.401	164.7E6	460.3E6	132.048	117.334
13)	MA Dieldrin	6.327	5.540	181.8E6	485.7E6	123.228	113.066
14)	MA Endrin	6.553	5.818	156.2E6	450.1E6	138.442m	121.583
15)	B Endosulfa...	6.765	6.110	149.6E6	419.4E6	113.306	113.105
16)	A 4,4'-DDD	6.684	5.958	126.9E6	383.3E6	128.479	112.956
17)	MA 4,4'-DDT	6.998	6.213	125.5E6	379.2E6	140.208m	118.532
18)	B Endrin al...	6.893	6.288	103.4E6	294.7E6	114.540	103.213
19)	B Endosulfa...	7.127	6.513	142.8E6	404.7E6	123.983	113.309
20)	A Methoxychlor	7.470	6.786	342.5E6	890.3E6	657.491	538.200
21)	B Endrin ke...	7.607	7.024	150.6E6	462.0E6	123.172	104.922

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090324\
Data File : PD084864.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2024 12:41
Operator : AR\AJ
Sample : P3673-22MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:10:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

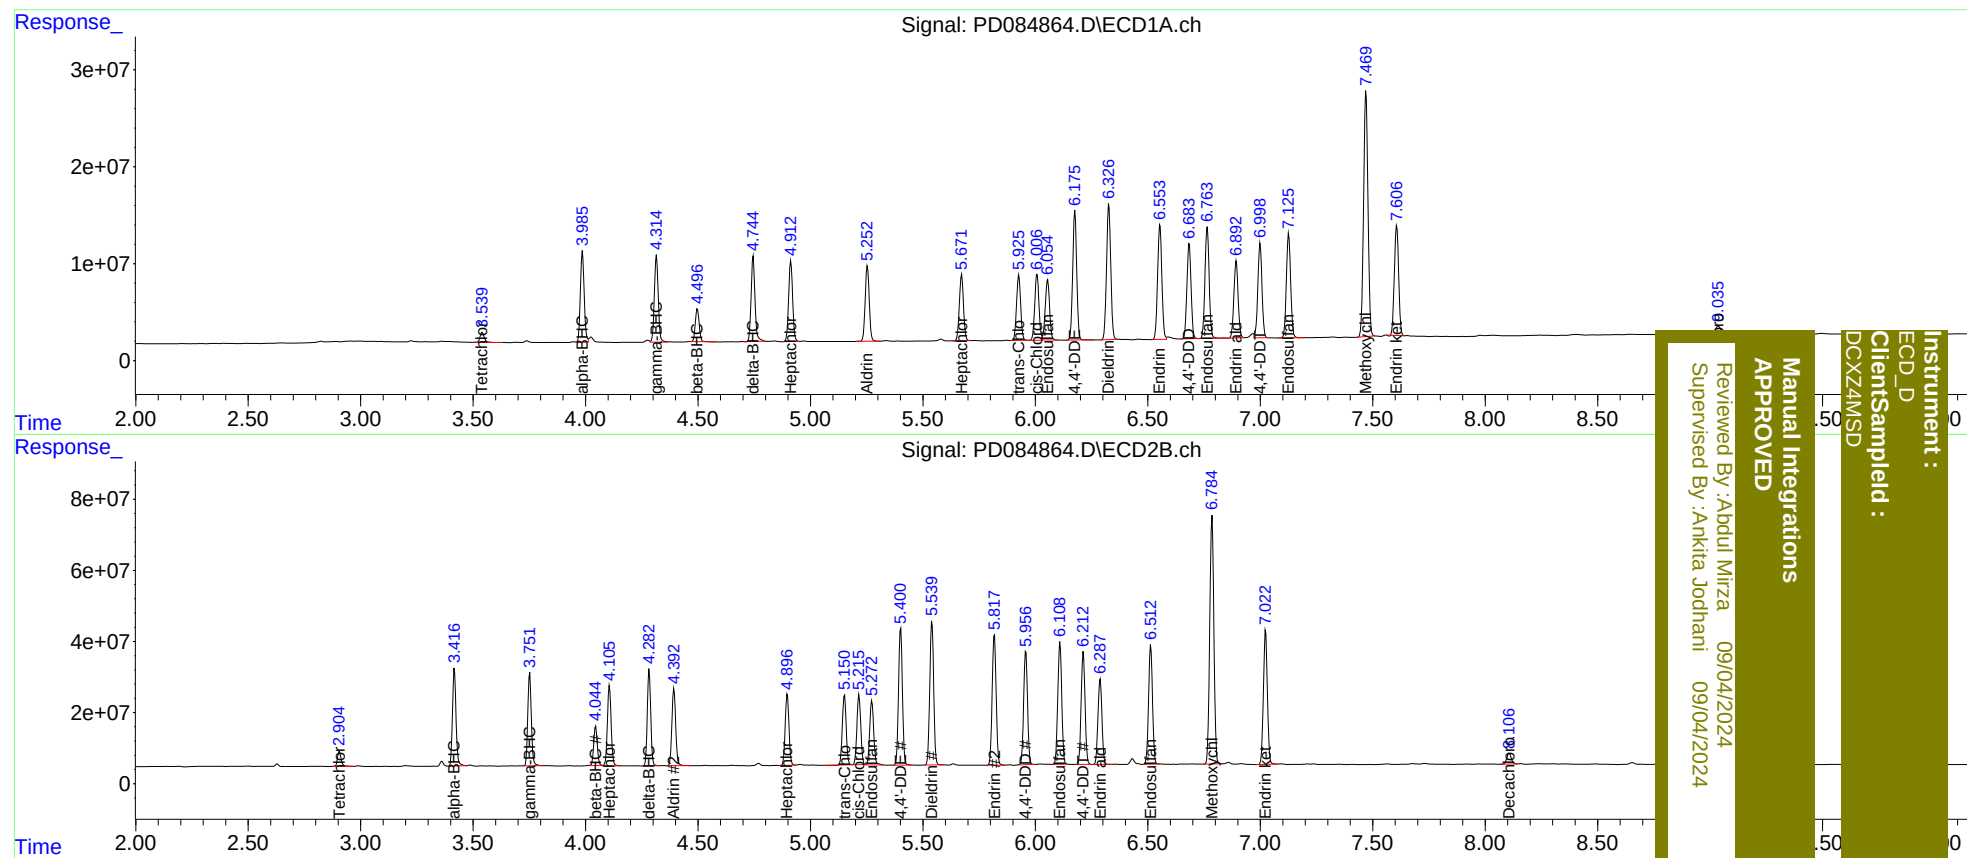

Instrument :
ECD_D
ClientSampled :
DCXZ4MSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 09/04/2024
Supervised By: Ankita Jodhani 09/04/2024