

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090324\
 Data File : PD084876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2024 16:10
 Operator : AR\AJ
 Sample : P3711-09MS
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E24A0MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/04/2024
 Supervised By :Ankita Jodhani 09/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:12:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.906	20644666	72368729	20.412	20.450
27)	SA Decachlor...	9.031	8.105	29522146	80349550	22.604	23.108
Target Compounds							
2)	A alpha-BHC	3.983	3.417	100.7E6	278.3E6	59.230	54.880
3)	MA gamma-BHC...	4.312	3.752	95363008	261.1E6	58.944	53.886
4)	MA Heptachlor	4.909	4.106	90592723	229.0E6	58.880	53.784
5)	MB Aldrin	5.250	4.393	86680000	229.5E6	54.197	51.672
6)	B beta-BHC	4.494	4.043	37054787	112.4E6	51.014	51.824m
7)	B delta-BHC	4.742	4.283	92081746	265.7E6	56.147	53.534
8)	B Heptachlo...	5.669	4.896	80214777	217.9E6	53.782	51.445
9)	A Endosulfan I	6.050	5.271	75685312	204.2E6	55.012m	53.268m
10)	B trans-Chl...	5.923	5.150	77803617	224.6E6	55.165	54.600
11)	B cis-Chlor...	6.003	5.215	80628911	218.8E6	54.532m	52.154
12)	B 4,4'-DDE	6.173	5.400	148.3E6	423.3E6	118.851	107.910
13)	MA Dieldrin	6.324	5.539	167.4E6	455.2E6	113.484	105.958
14)	MA Endrin	6.549	5.816	142.4E6	418.6E6	126.236m	113.057
15)	B Endosulfa...	6.761	6.108	141.6E6	396.4E6	107.278	106.918
16)	A 4,4'-DDD	6.680	5.956	117.2E6	374.0E6	118.715	110.223
17)	MA 4,4'-DDT	6.994	6.212	111.6E6	349.8E6	124.723m	109.348
18)	B Endrin al...	6.889	6.287	101.8E6	300.4E6	112.744	105.198
19)	B Endosulfa...	7.123	6.511	131.8E6	382.8E6	114.452	107.190
20)	A Methoxychlor	7.467	6.784	306.2E6	838.5E6	587.884	506.861
21)	B Endrin ke...	7.603	7.022	140.8E6	450.9E6	115.120	102.406

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090324\
Data File : PD084876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2024 16:10
Operator : AR\AJ
Sample : P3711-09MS
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:12:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

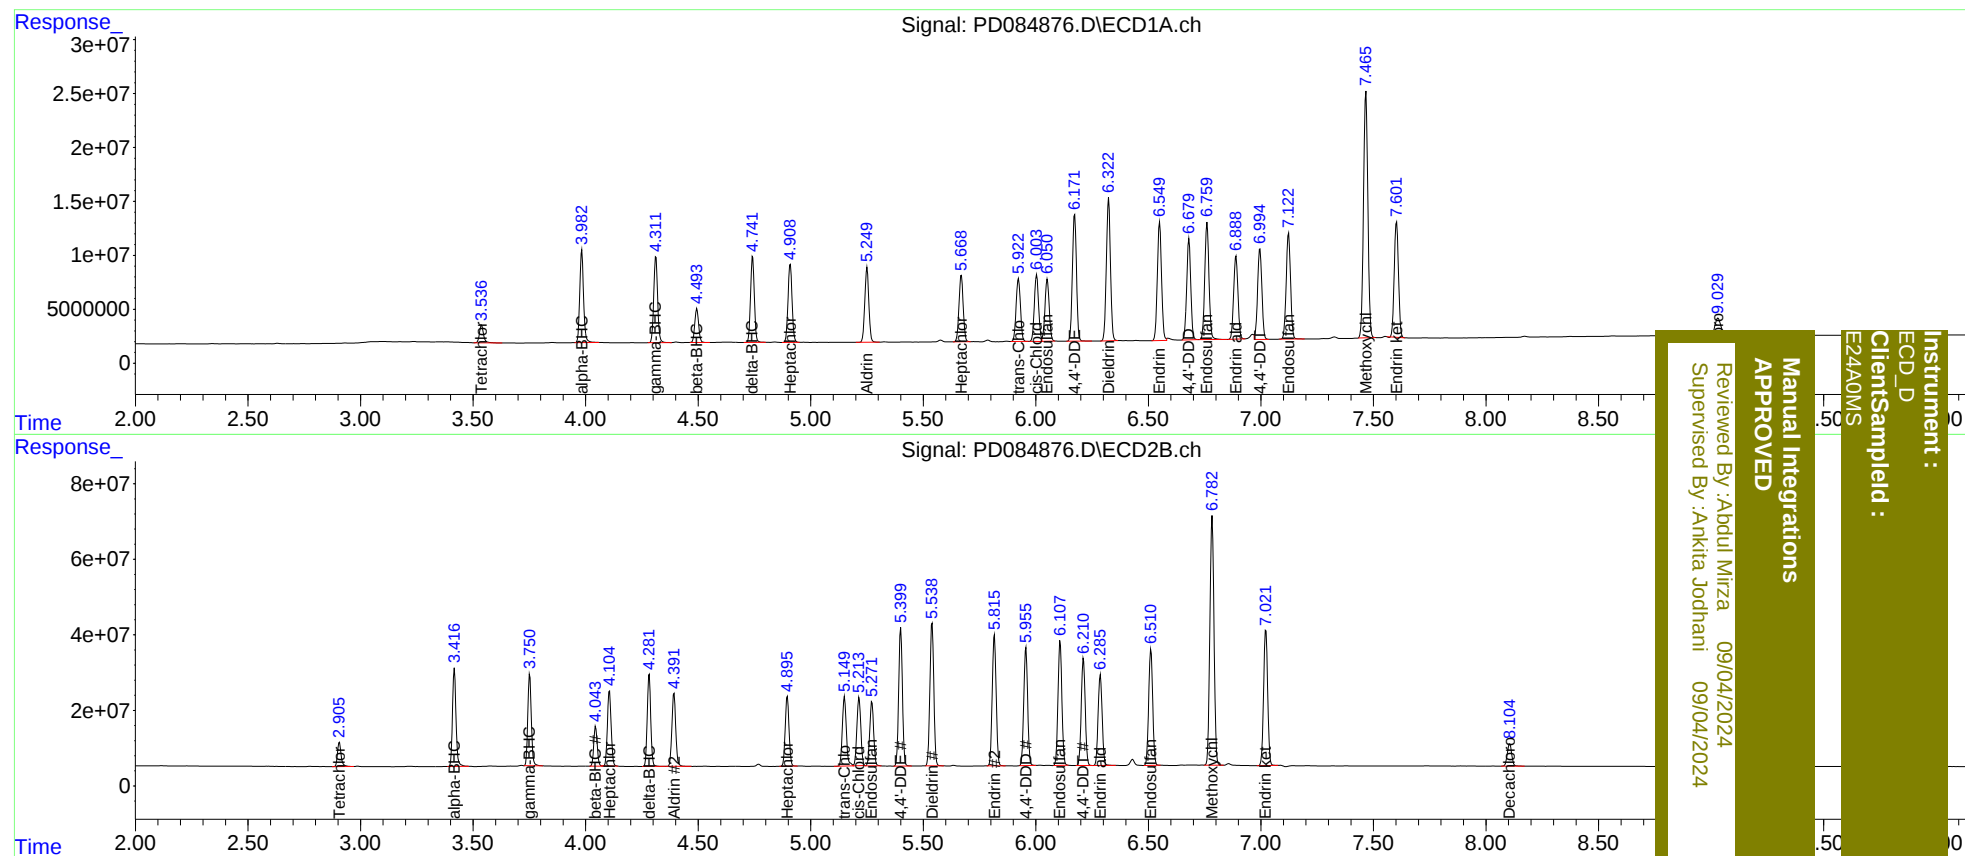

Instrument :
ECD_D
ClientSampled :
E24A0MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 09/04/2024
Supervised By: Ankita Jodhani 09/04/2024