

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090324\
 Data File : PD084880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2024 17:03
 Operator : AR\AJ
 Sample : P3711-10MSD
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E24A0MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/04/2024
 Supervised By :Ankita Jodhani 09/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:13:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.906	20777389	73670073	20.543	20.818
27)	SA Decachlor...	9.031	8.105	29744740	81606023	22.775	23.469
Target Compounds							
2)	A alpha-BHC	3.983	3.417	102.4E6	281.6E6	60.206	55.536
3)	MA gamma-BHC...	4.311	3.751	97056317	264.9E6	59.991	54.672
4)	MA Heptachlor	4.909	4.106	91680447	233.0E6	59.587	54.731
5)	MB Aldrin	5.249	4.393	87674161	233.1E6	54.818	52.478
6)	B beta-BHC	4.494	4.043	37694852	114.2E6	51.895	52.664m
7)	B delta-BHC	4.742	4.283	93434064	268.4E6	56.972	54.064
8)	B Heptachlo...	5.668	4.896	81475173	221.8E6	54.628	52.365
9)	A Endosulfan I	6.049	5.271	76280231	207.8E6	55.444m	54.200m
10)	B trans-Chl...	5.922	5.150	79015299	228.4E6	56.024	55.539
11)	B cis-Chlor...	6.002	5.215	82669074	222.2E6	55.912m	52.949
12)	B 4,4'-DDE	6.172	5.401	150.1E6	431.2E6	120.356	109.927
13)	MA Dieldrin	6.323	5.539	169.9E6	462.2E6	115.173	107.578
14)	MA Endrin	6.548	5.816	144.8E6	424.9E6	128.329m	114.759
15)	B Endosulfa...	6.760	6.108	143.5E6	402.0E6	108.704	108.427
16)	A 4,4'-DDD	6.680	5.957	118.7E6	380.5E6	120.189	112.128
17)	MA 4,4'-DDT	6.994	6.212	113.1E6	357.2E6	126.331m	111.662
18)	B Endrin al...	6.889	6.287	102.9E6	305.6E6	113.981	107.018
19)	B Endosulfa...	7.123	6.511	133.5E6	388.5E6	115.897	108.779
20)	A Methoxychlor	7.466	6.784	309.2E6	851.0E6	593.601	514.425
21)	B Endrin ke...	7.602	7.021	142.6E6	457.5E6	116.596	103.893

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090324\
Data File : PD084880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2024 17:03
Operator : AR\AJ
Sample : P3711-10MSD
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:13:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

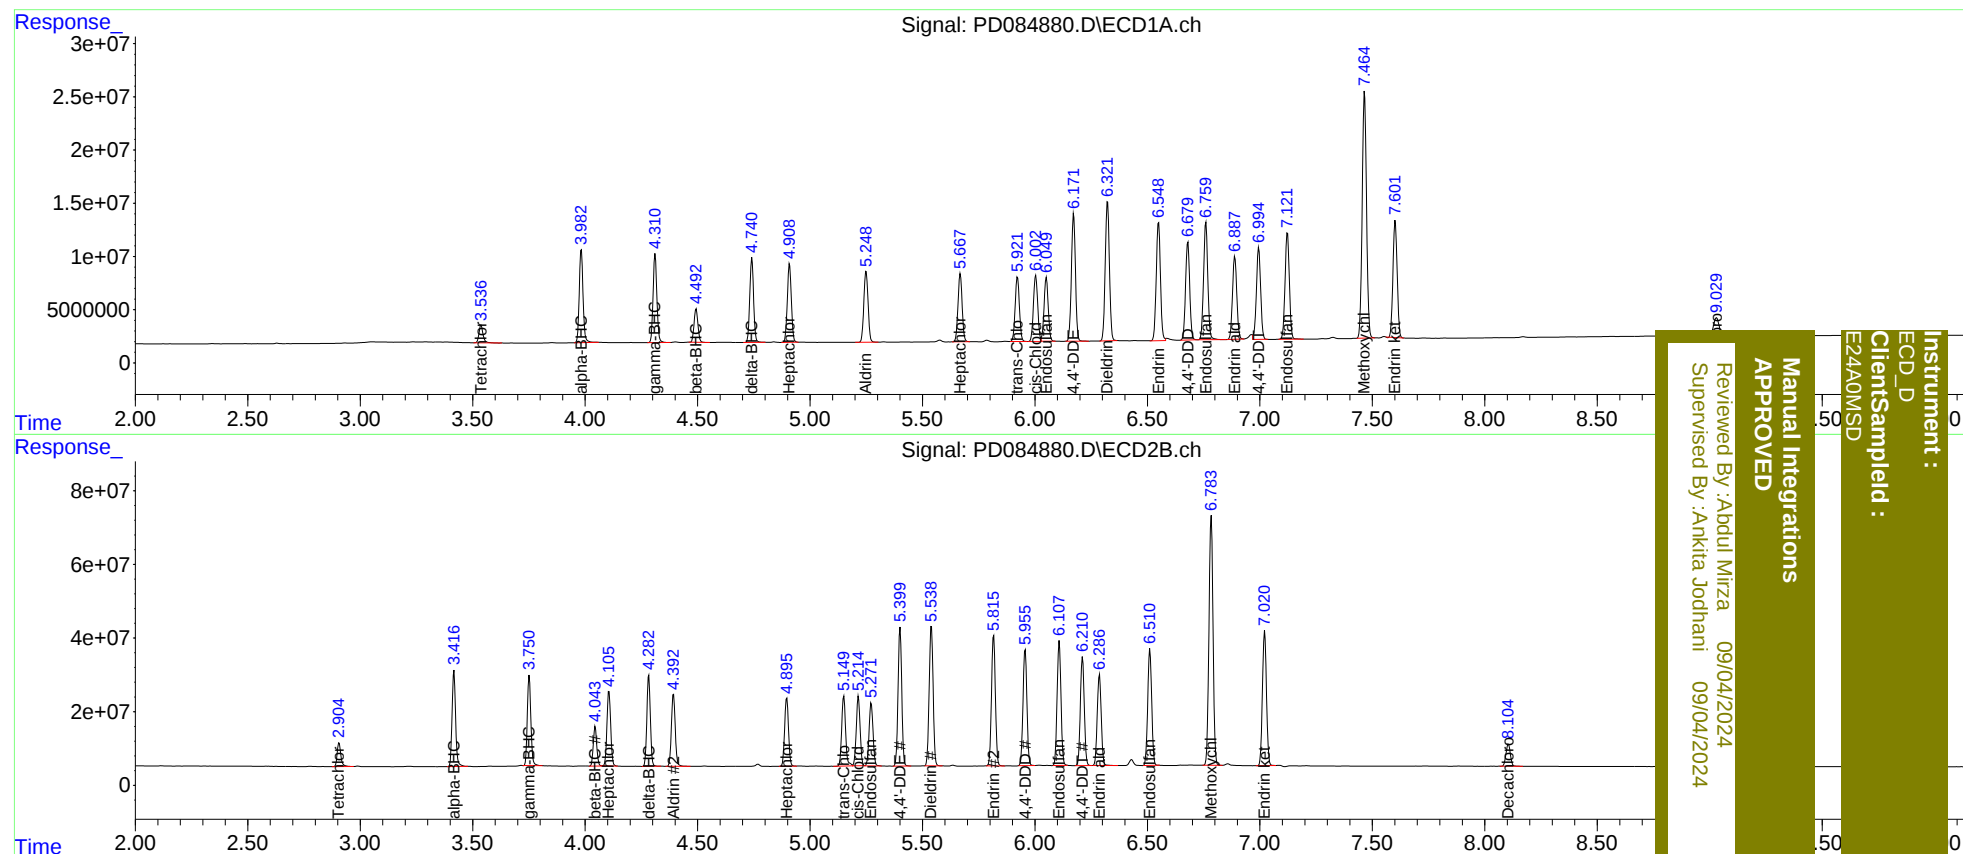

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/04/2024
Supervised By: Ankita Jodhani 09/04/2024

Instrument :
ECD_D
ClientSampleId :
E24A0M5D