

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090420\
 Data File : PD059098.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2020 14:02
 Operator : DD\AJ
 Sample : PIBLK50
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK50

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 14:56:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 04 14:50:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.206	3.865	19969823	33213312	19.811	20.267
27) SA Decachlor...	7.839	8.861	35837782	50233787	36.568	37.351
Target Compounds						
8) B Heptachlo...	0.000	5.708	0	2190547	N.D.	1.091


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090420\
Data File : PD059098.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2020 14:02
Operator : DD\AJ
Sample : PIBLK50
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK50

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 14:56:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 04 14:50:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

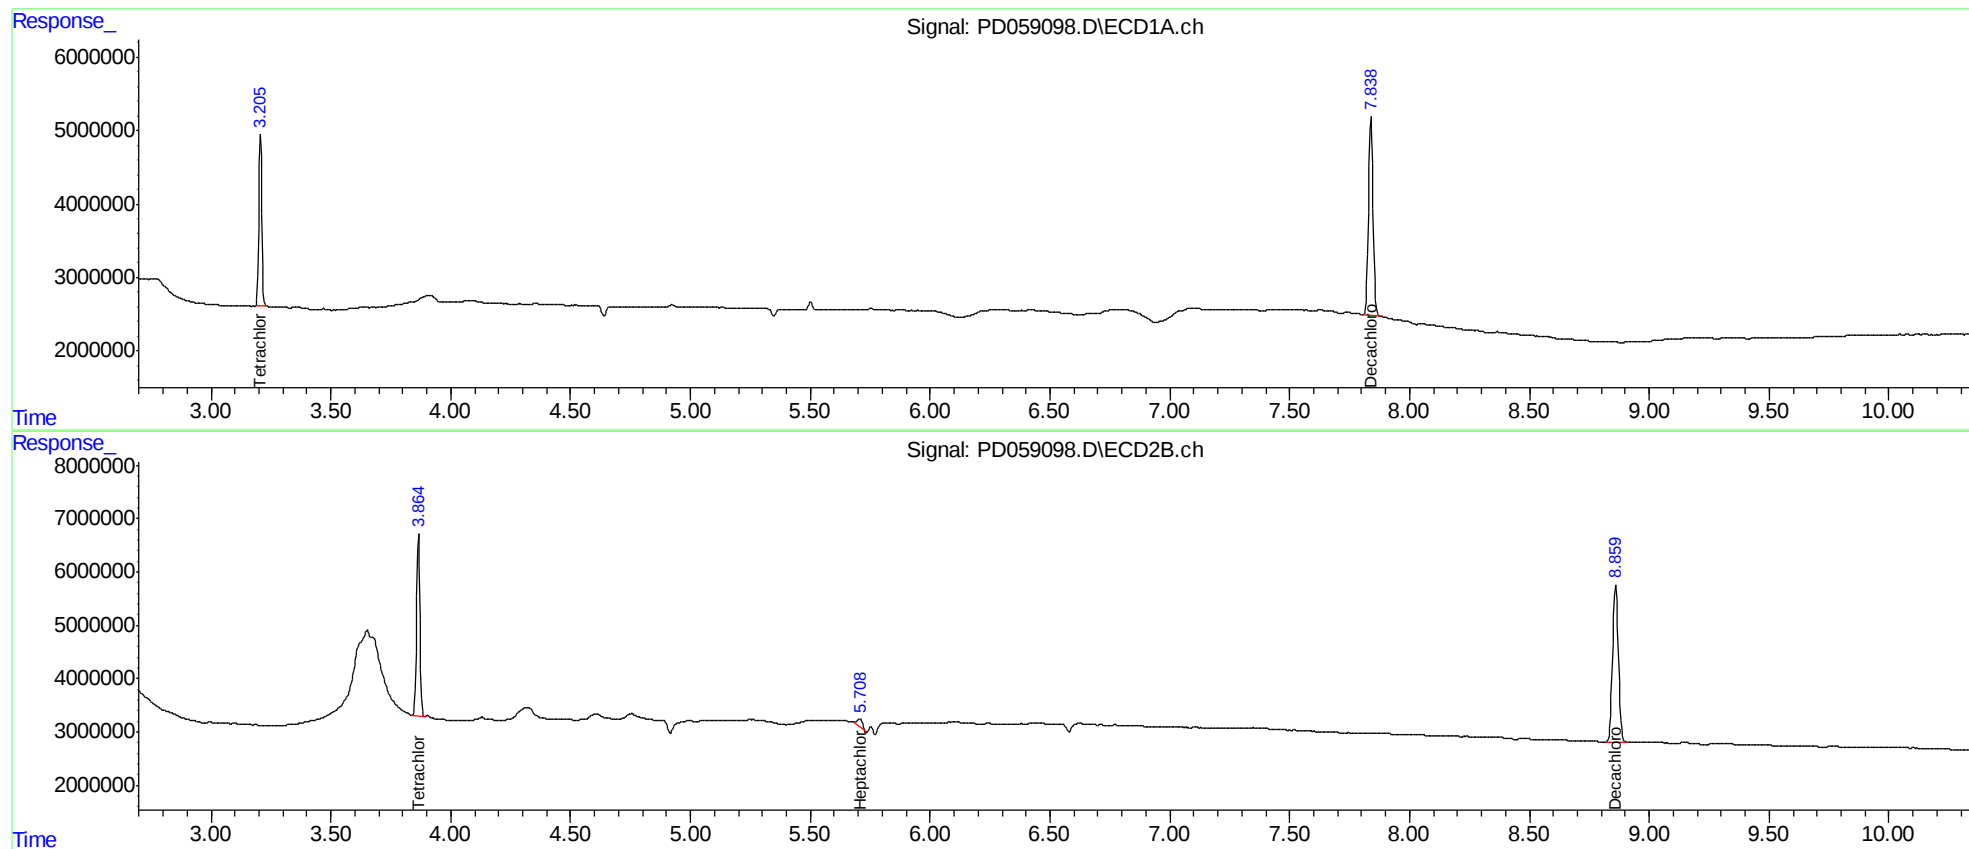


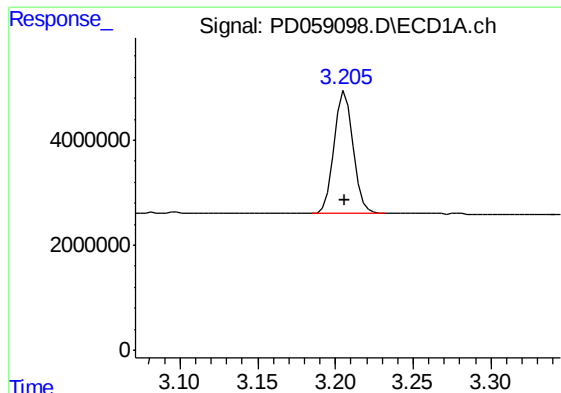

#1 Tetrachloro-m-xylene


R.T.: 3.206 min
Delta R.T.: 0.000 min
Response: 19969823
Conc: 19.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK50

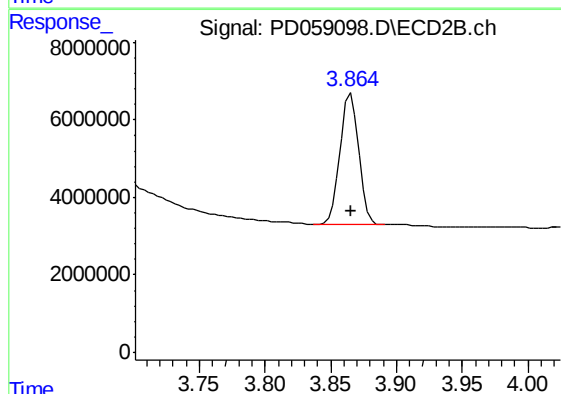


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 33213312
Conc: 20.27 ng/ml

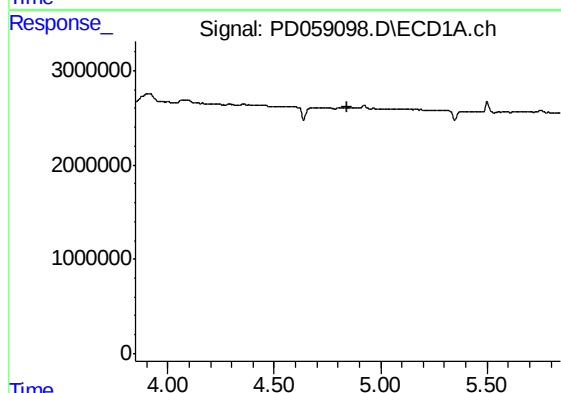


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.845 min
Response: 0
Conc: N.D.

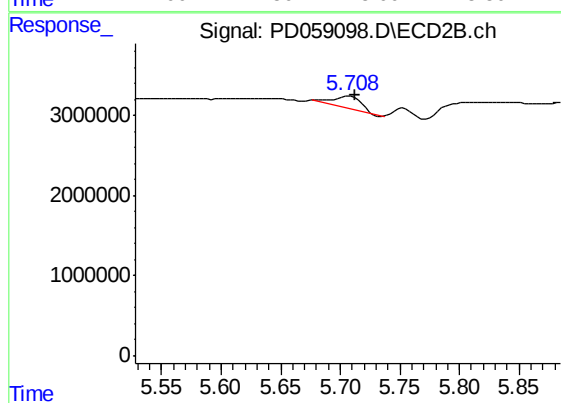

#8 Heptachlor epoxide


R.T.: 5.708 min
Delta R.T.: -0.003 min
Response: 2190547
Conc: 1.09 ng/ml

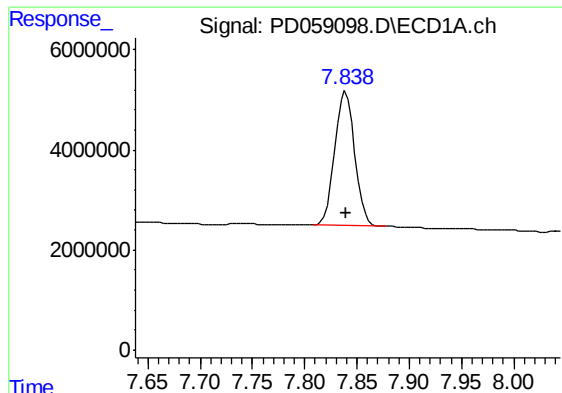

#27 Decachlorobiphenyl

R.T.: 7.839 min
Delta R.T.: 0.000 min
Response: 35837782
Conc: 36.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK50

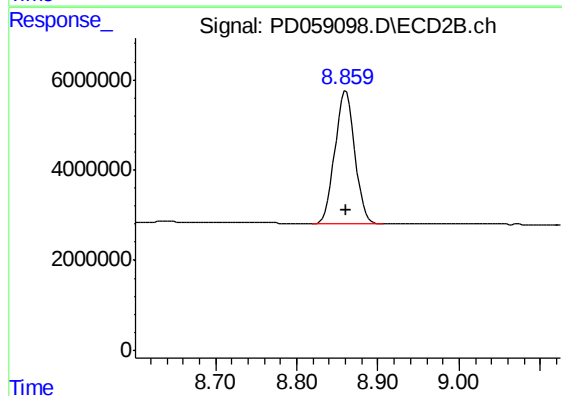

#27 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.000 min
Response: 50233787
Conc: 37.35 ng/ml