

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090421\
 Data File : PD065559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2021 19:34
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:05:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 04 01:04:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.014	63142727	396.7E6	50.000	50.000
28)	SA Decachlor...	8.239	9.085	89591449	279.7E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.365	5.010	21406882	156.6E6	500.000	500.000
24)	Chlordane-2	4.865	5.480	26788025	140.1E6	500.000	500.000
25)	Chlordane-3	5.432	6.128	78193002	528.9E6	500.000	500.000
26)	Chlordane-4	5.490	6.200	63951419	616.0E6	500.000	500.000
27)	Chlordane-5	6.327	7.010	31323724	121.3E6	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090421\
Data File : PD065559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2021 19:34
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:05:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Sat Sep 04 01:04:47 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

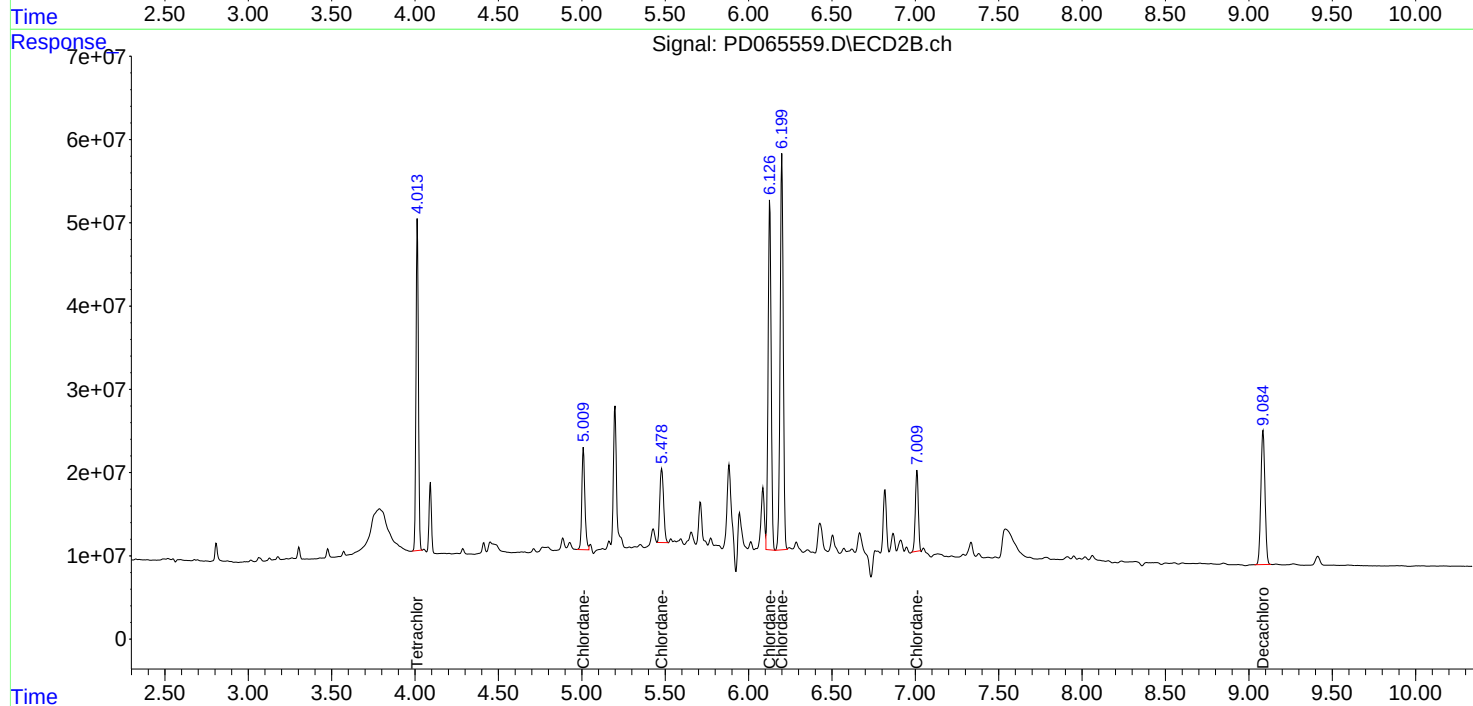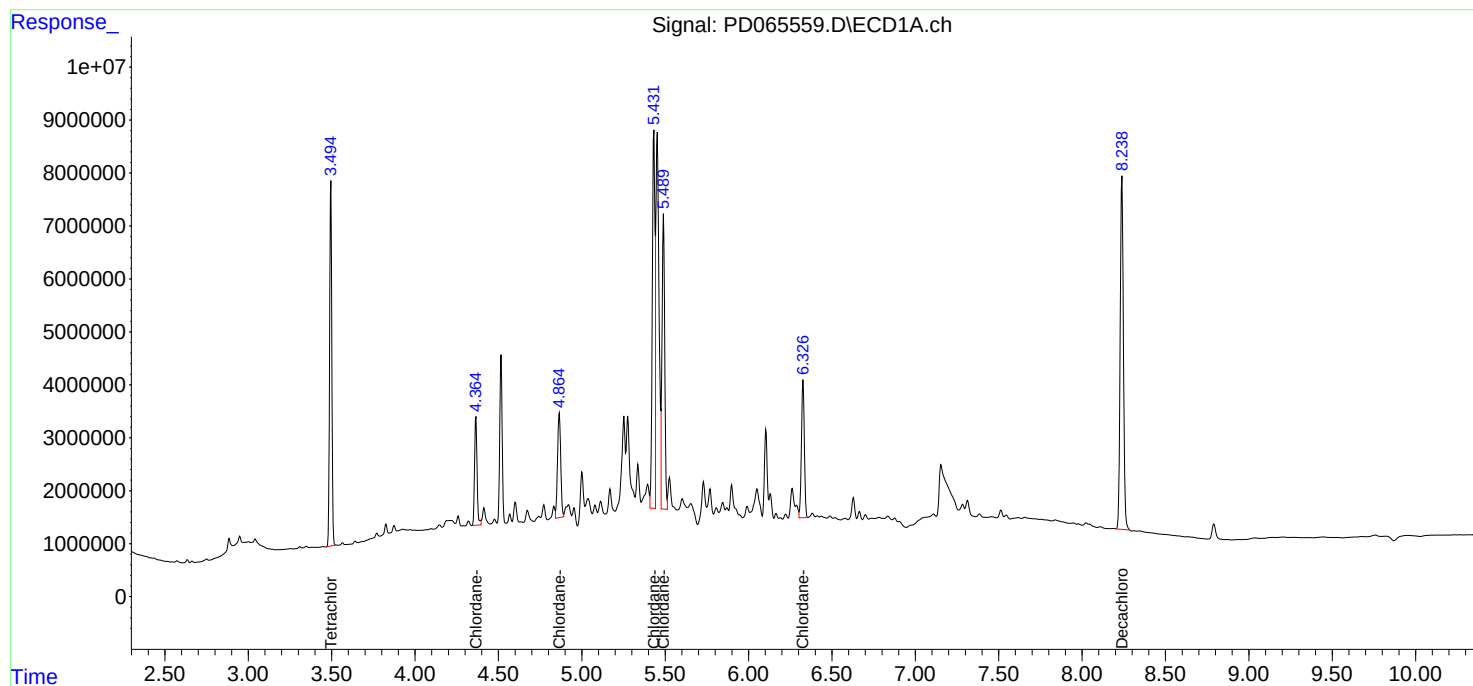

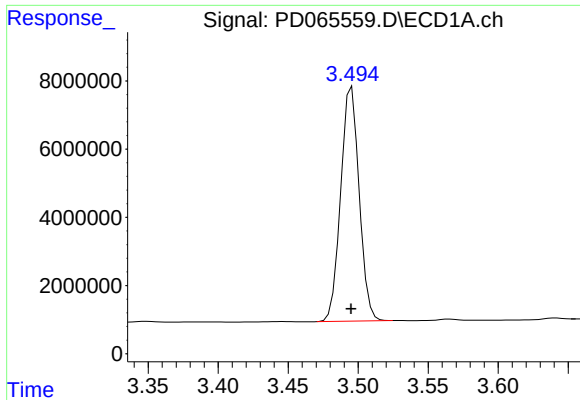


#1 Tetrachloro-m-xylene

R.T.: 3.495 min
Delta R.T.: 0.000 min
Response: 63142727
Conc: 50.00 ng/ml

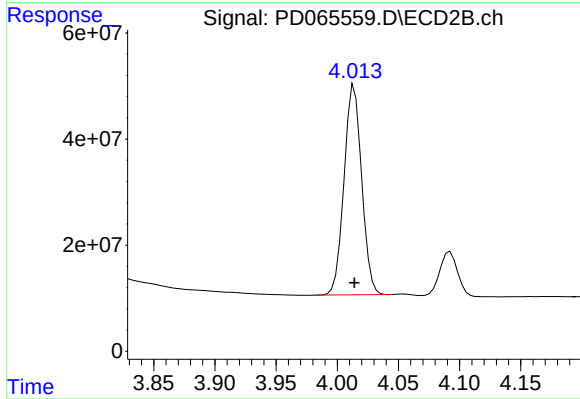


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 396652109
Conc: 50.00 ng/ml

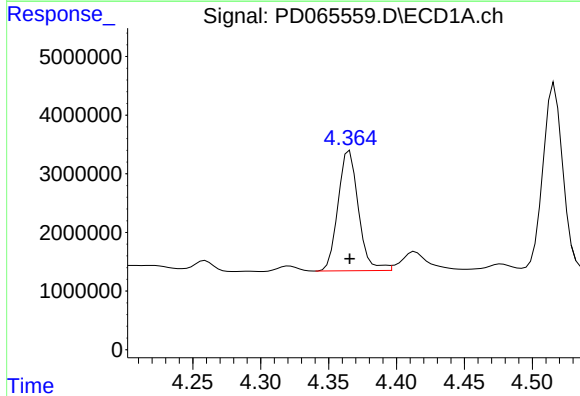


#23 Chlordane-1

R.T.: 4.365 min
Delta R.T.: 0.000 min
Response: 21406882
Conc: 500.00 ng/ml

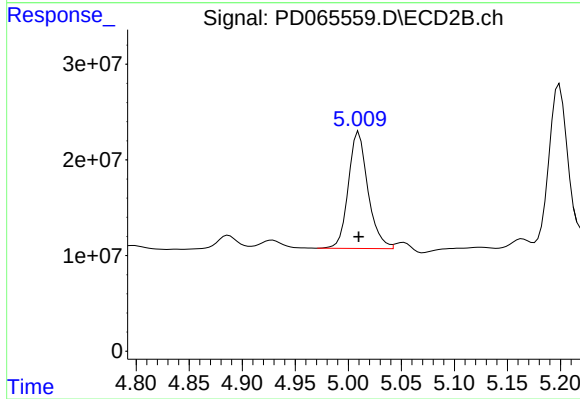


#23 Chlordane-1

R.T.: 5.010 min
Delta R.T.: 0.000 min
Response: 156594540
Conc: 500.00 ng/ml

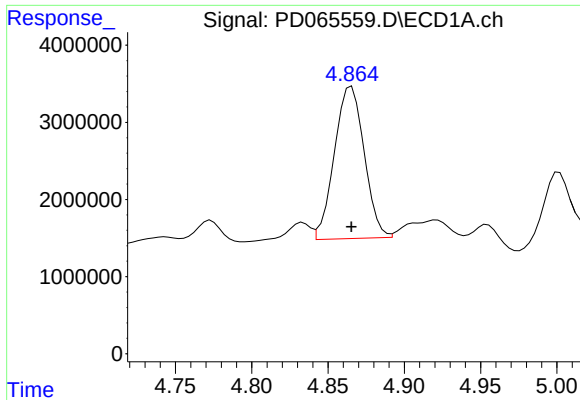


#24 Chlordane-2

R.T.: 4.865 min
Delta R.T.: 0.000 min
Response: 26788025
Conc: 500.00 ng/ml

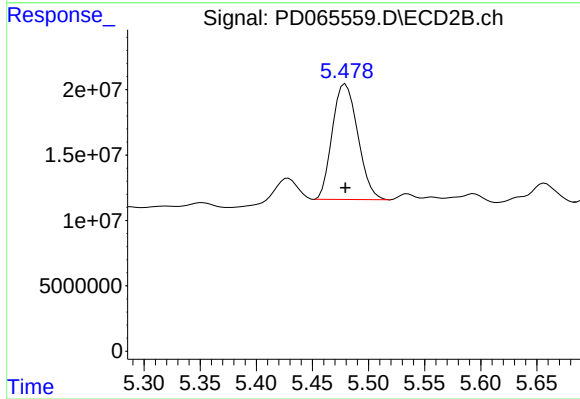


#24 Chlordane-2

R.T.: 5.480 min
Delta R.T.: 0.000 min
Response: 140082236
Conc: 500.00 ng/ml

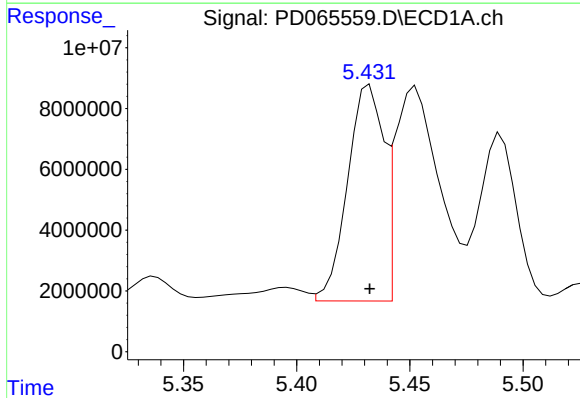


#25 Chlordane-3

R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 78193002
Conc: 500.00 ng/ml

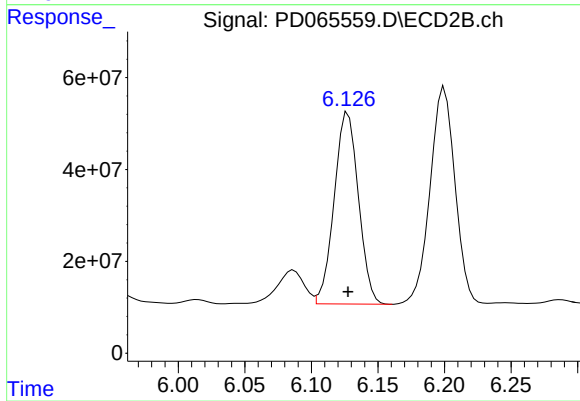


#25 Chlordane-3

R.T.: 6.128 min
Delta R.T.: 0.000 min
Response: 528894851
Conc: 500.00 ng/ml

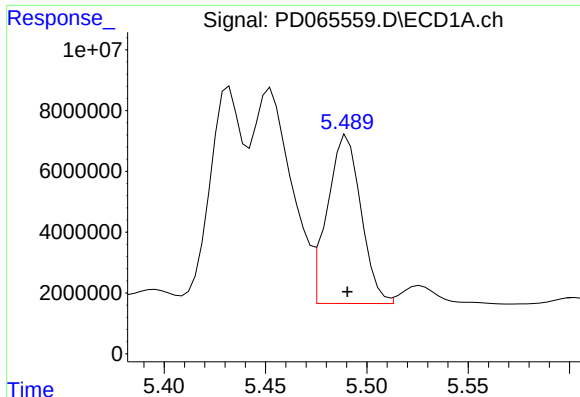


#26 Chlordane-4

R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 63951419
Conc: 500.00 ng/ml

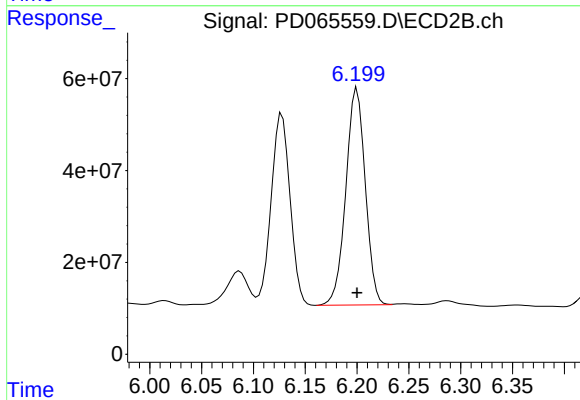


#26 Chlordane-4

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 615980554
Conc: 500.00 ng/ml

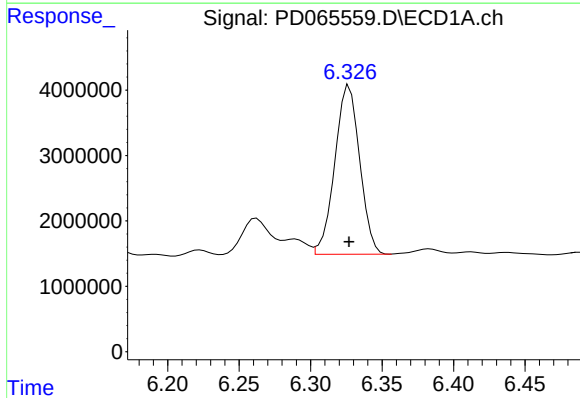


#27 Chlordane-5

R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 31323724
Conc: 500.00 ng/ml

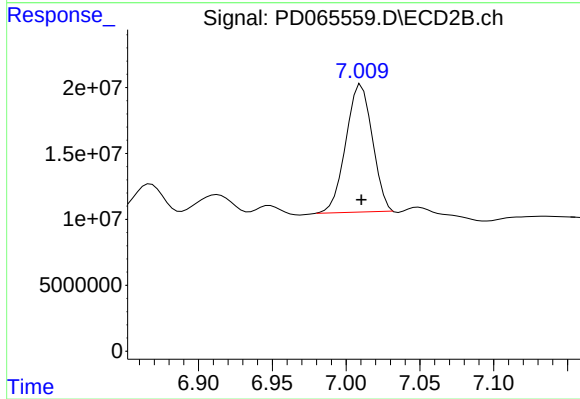


#27 Chlordane-5

R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 121278819
Conc: 500.00 ng/ml

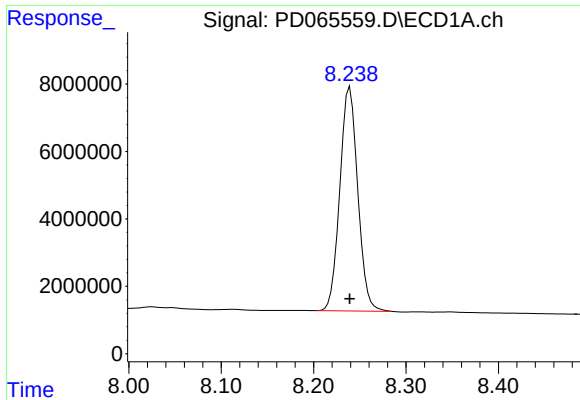

#28 Decachlorobiphenyl

R.T.: 8.239 min
Delta R.T.: 0.000 min
Response: 89591449
Conc: 50.00 ng/ml

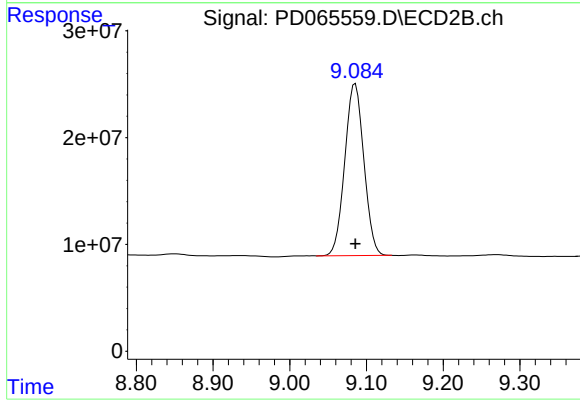

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 279730871
Conc: 50.00 ng/ml