

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090421\
 Data File : PD065563.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2021 20:29
 Operator : AR\AJ
 Sample : PTOXICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:28:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX090421.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 04 01:28:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.014	72903309	538.8E6	74.326	72.430
7)	SA Decachlor...	8.239	9.085	119.4E6	376.2E6	72.043	71.441
Target Compounds							
2)	Toxaphene-1	5.748	6.408	7855582	25509439	718.819	674.984
3)	Toxaphene-2	5.909	6.600	8654243	44962586	723.379	694.386
4)	Toxaphene-3	6.350	7.183	19228558	81236620	713.922	692.102
5)	Toxaphene-4	6.596	7.269	20626705	85180053	699.012	718.713
6)	Toxaphene-5	7.082	7.688	24079375	65000698	709.560	701.804

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090421\
Data File : PD065563.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2021 20:29
Operator : AR\AJ
Sample : PTOXICC750
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:28:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX090421.M
Quant Title : GC Extractables
QLast Update : Sat Sep 04 01:28:02 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

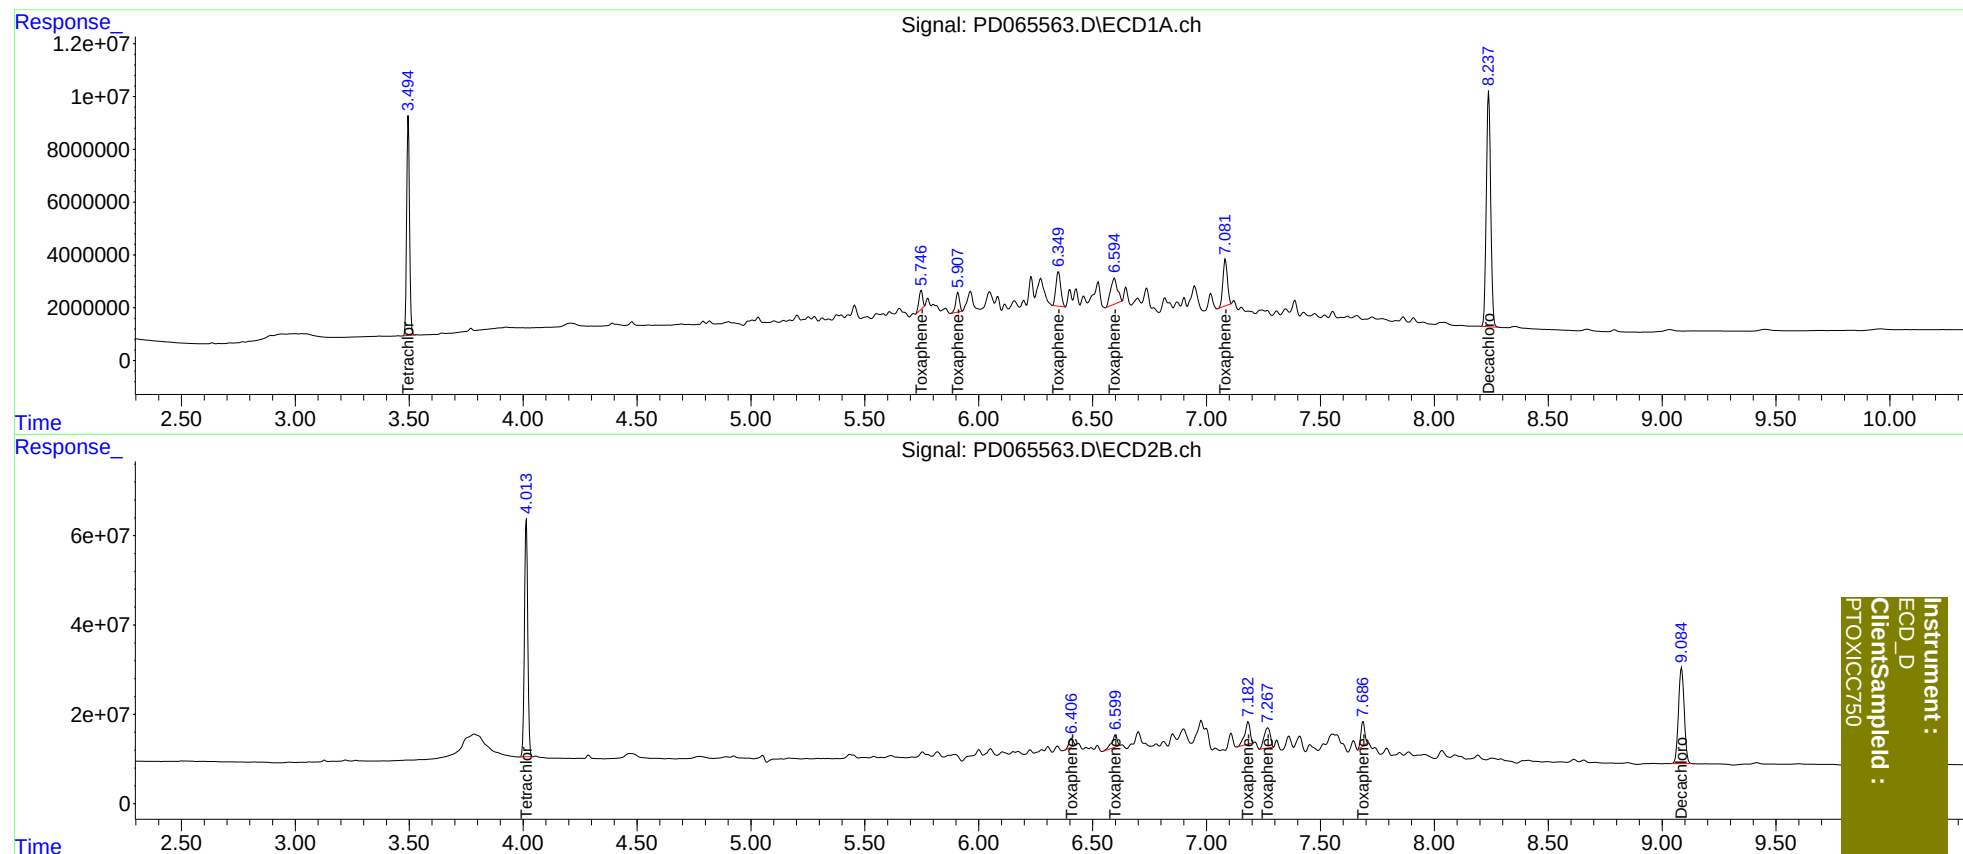

Instrument :
ECD_D
ClientSampled :
PTOXICC750