

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090421\
 Data File : PD065569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2021 21:52
 Operator : AR\AJ
 Sample : PTOXICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD090421TOX

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:38:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX090421.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 04 01:38:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.495	4.013	48767264	366.0E6	50.337	49.990
7) SA Decachlor...	8.238	9.085	81915605	259.7E6	48.950	49.623
Target Compounds						
2) Toxaphene-1	5.747	6.407	5501980	17958767	511.548	546.497
3) Toxaphene-2	5.909	6.598	5851110	32706095	485.861	528.322
4) Toxaphene-3	6.350	7.182	13216864	56599979	503.298	503.097
5) Toxaphene-4	6.595	7.269	14323692	58054399	492.354	503.353
6) Toxaphene-5	7.082	7.687	16850230	44892084	494.449	495.221

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090421\
Data File : PD065569.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2021 21:52
Operator : AR\AJ
Sample : PTOXICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:38:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX090421.M
Quant Title : GC Extractables
QLast Update : Sat Sep 04 01:38:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

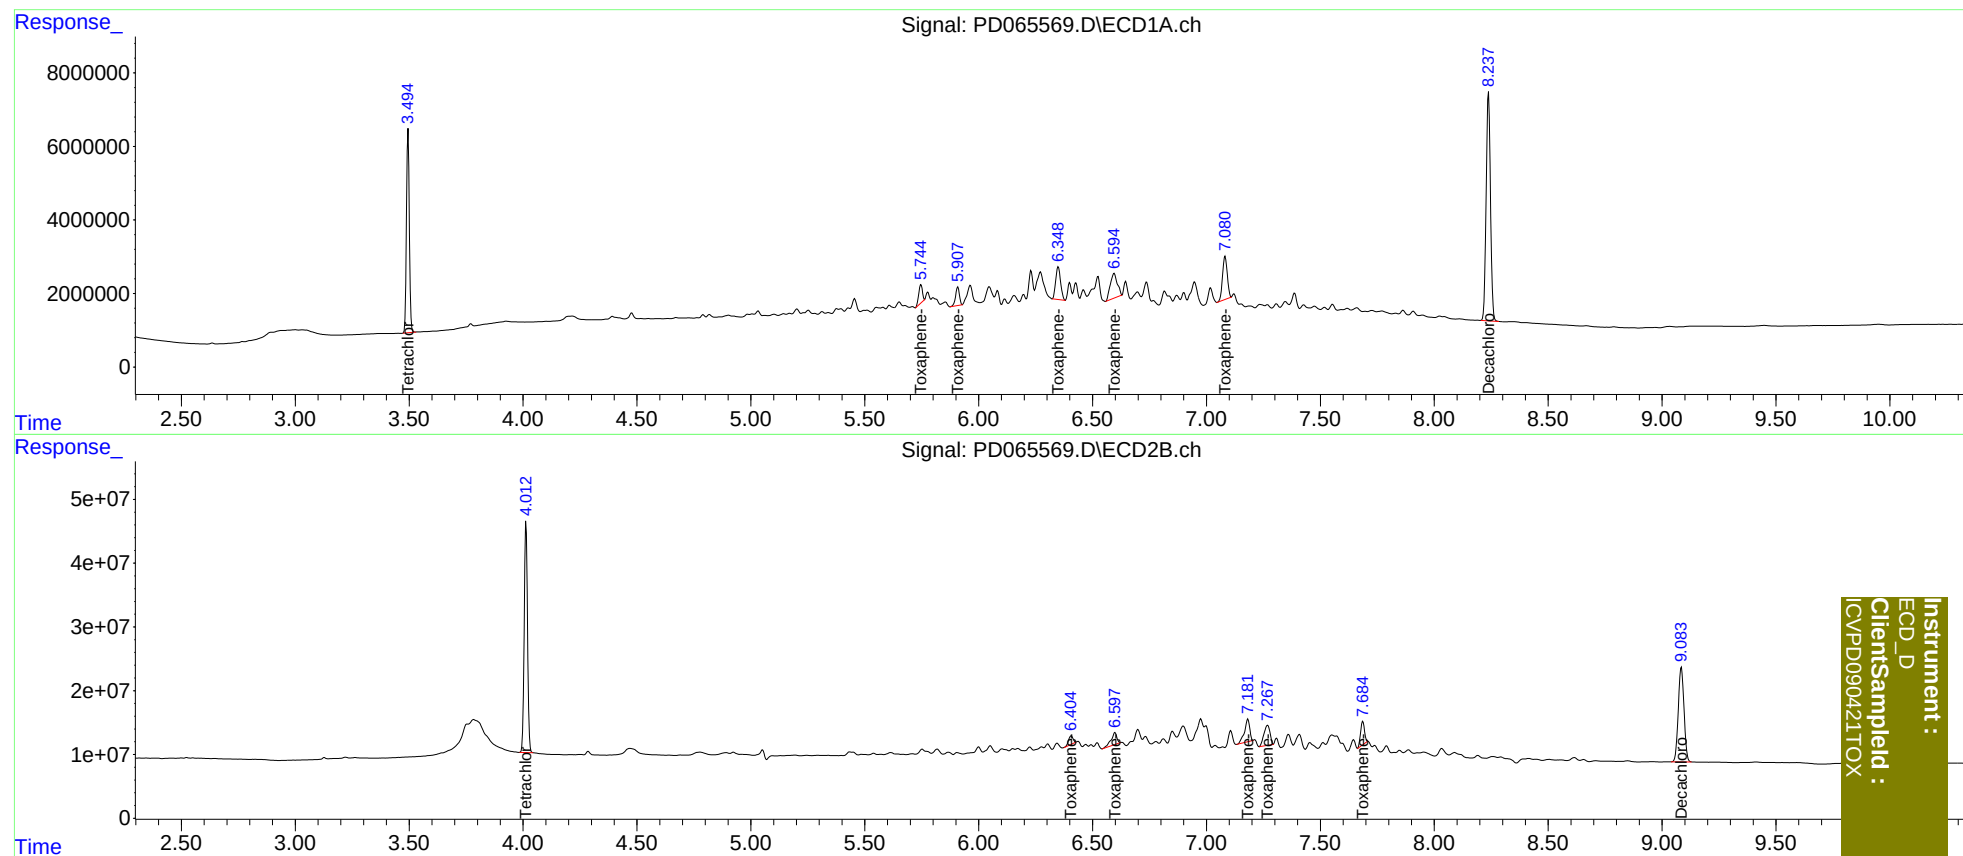

Instrument :
ECD_D
ClientSample :
ICV/PD090421TOX