

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090421\
 Data File : PD065557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2021 19:07
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:05:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 04 01:04:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.014	115.7E6	706.2E6	91.650	89.024
28)	SA Decachlor...	8.239	9.086	158.5E6	491.4E6	88.464	87.829
Target Compounds							
23)	Chlordane-1	4.365	5.009	38082671	281.3E6	889.496	898.137
24)	Chlordane-2	4.865	5.479	46864323	246.3E6	874.725	879.040
25)	Chlordane-3	5.432	6.127	145.7E6	954.7E6	931.516	902.545
26)	Chlordane-4	5.490	6.200	120.2E6	1101.5E6	939.935	894.074
27)	Chlordane-5	6.327	7.011	56333956	218.2E6	899.222	899.543



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090421\
Data File : PD065557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2021 19:07
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:05:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Sat Sep 04 01:04:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

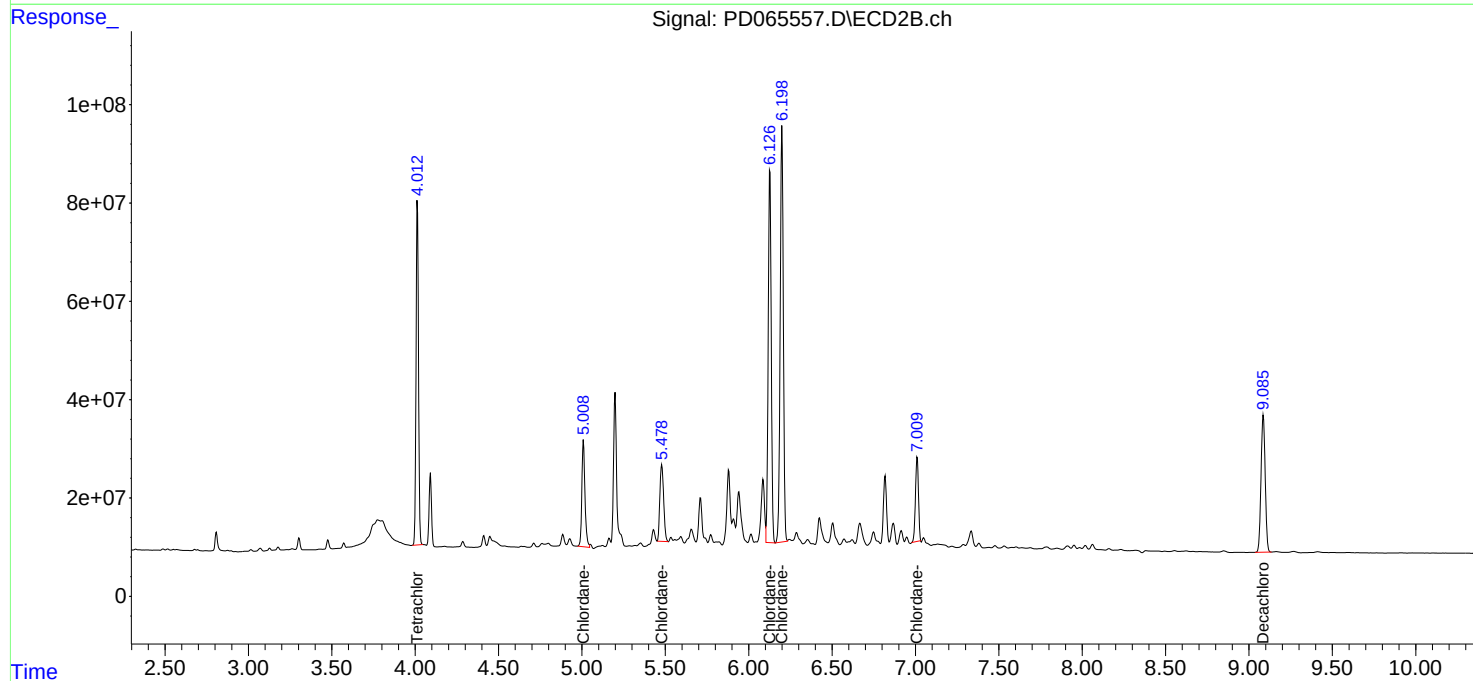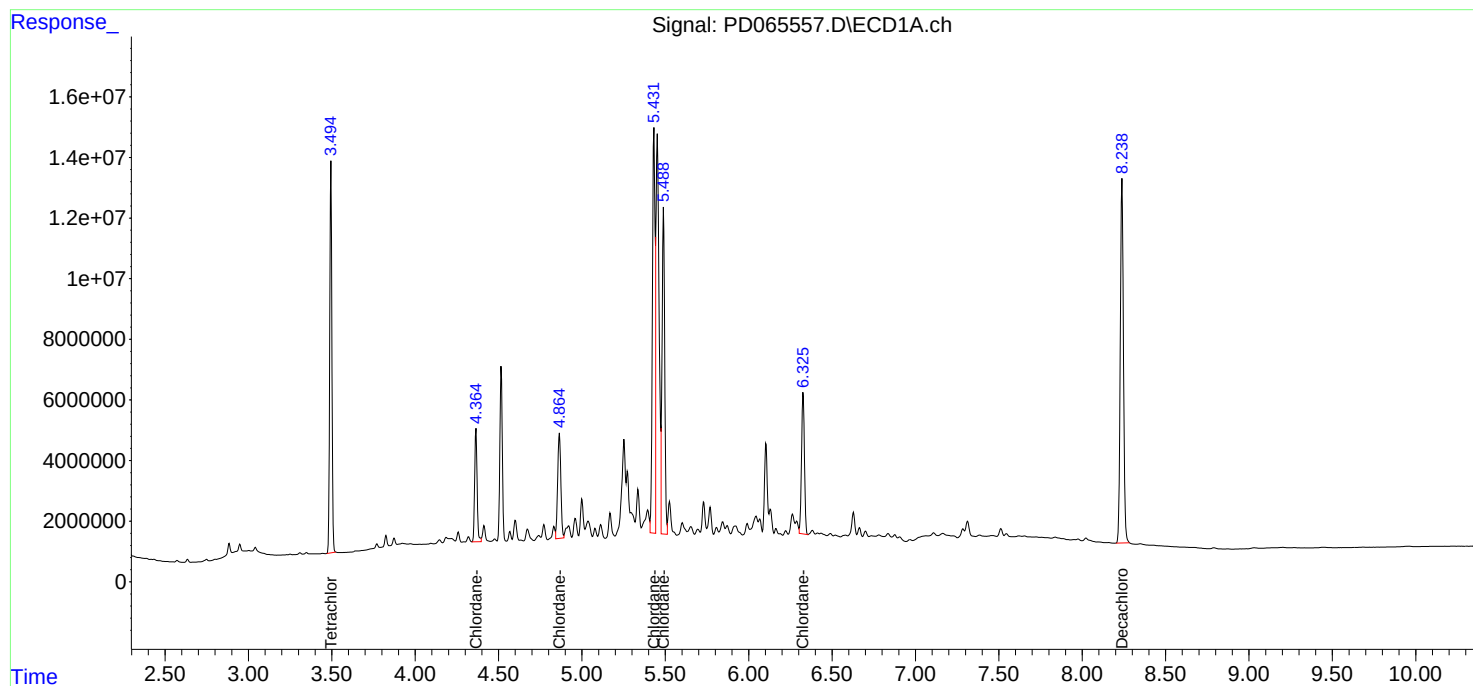


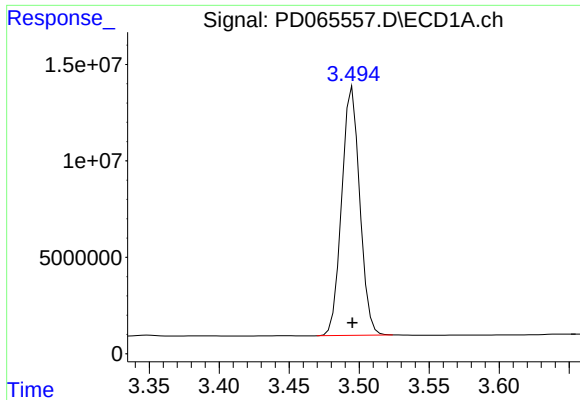

#1 Tetrachloro-m-xylene


R.T.: 3.495 min
Delta R.T.: 0.000 min
Response: 115740223
Conc: 91.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

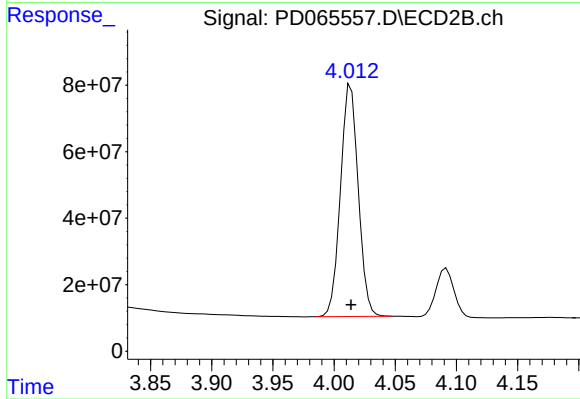


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 706229152
Conc: 89.02 ng/ml

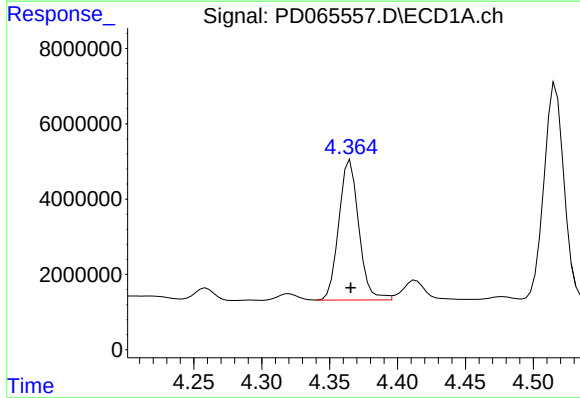


#23 Chlordane-1

R.T.: 4.365 min
Delta R.T.: 0.000 min
Response: 38082671
Conc: 889.50 ng/ml

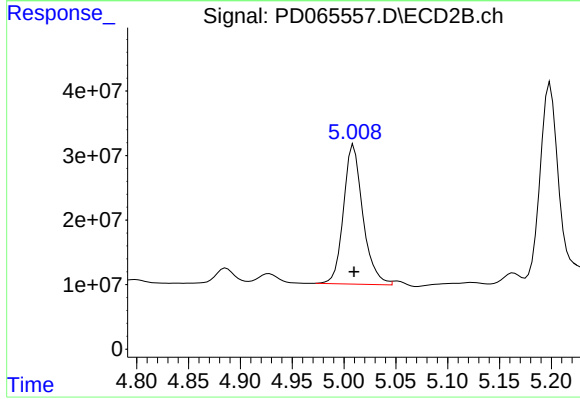

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 281286714
Conc: 898.14 ng/ml

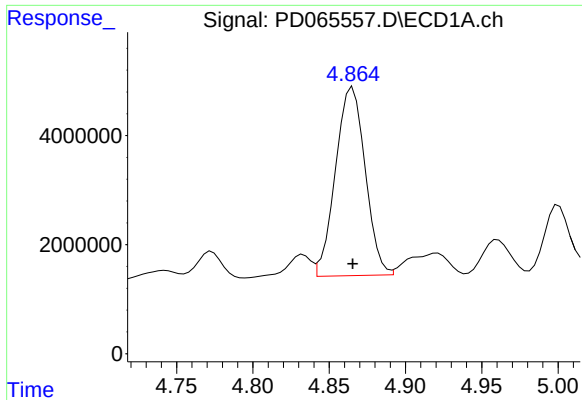

#24 Chlordane-2


R.T.: 4.865 min
Delta R.T.: 0.000 min
Response: 46864323
Conc: 874.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

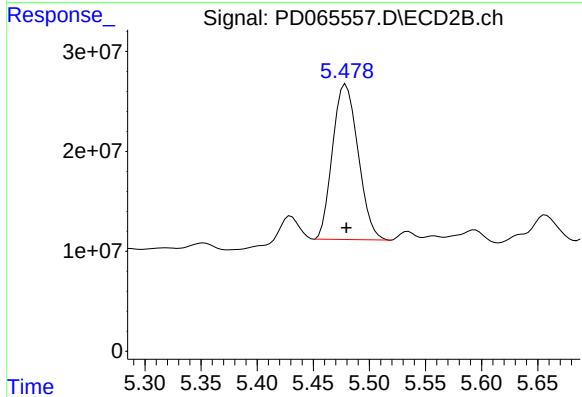


#24 Chlordane-2

R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 246275750
Conc: 879.04 ng/ml

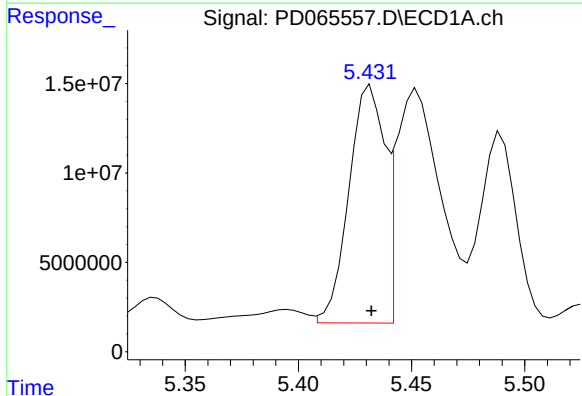


#25 Chlordane-3

R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 145676070
Conc: 931.52 ng/ml

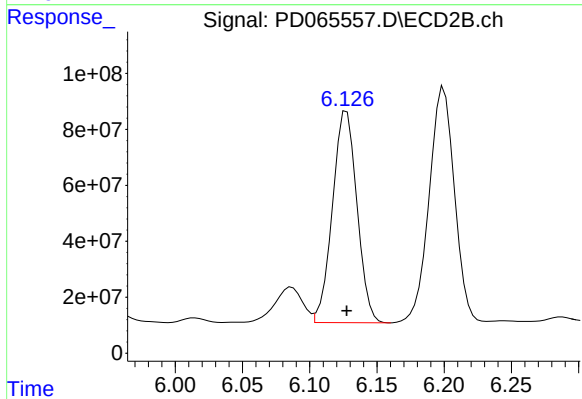

#25 Chlordane-3


R.T.: 6.127 min
Delta R.T.: 0.000 min
Response: 954703204
Conc: 902.55 ng/ml

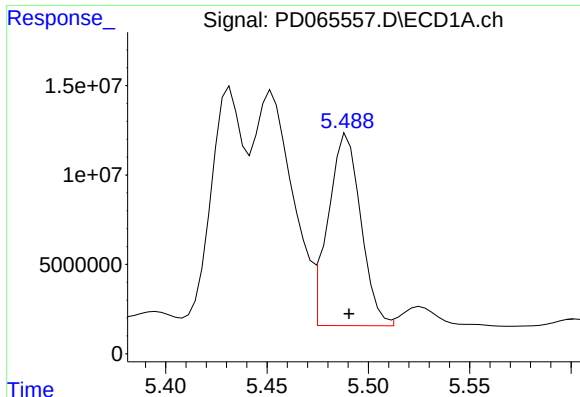

#26 Chlordane-4


R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 120220311
Conc: 939.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

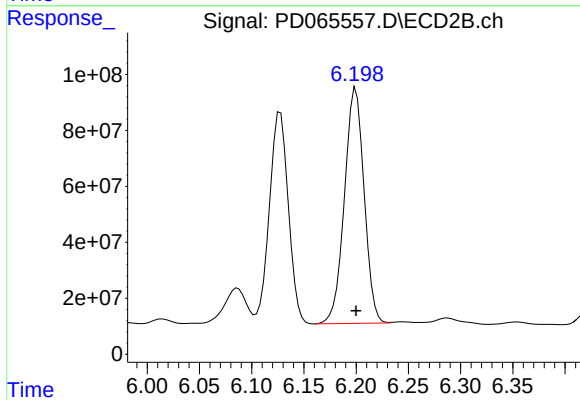


#26 Chlordane-4

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 1101464553
Conc: 894.07 ng/ml

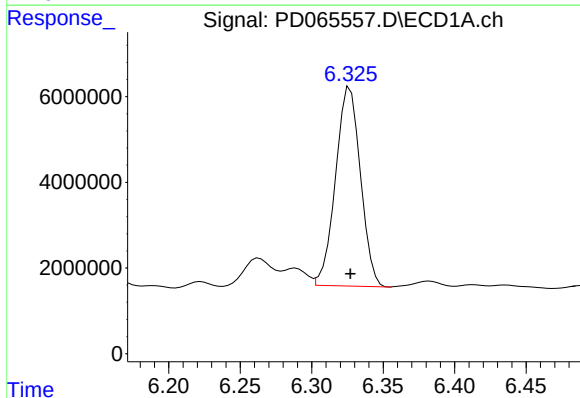


#27 Chlordane-5

R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 56333956
Conc: 899.22 ng/ml

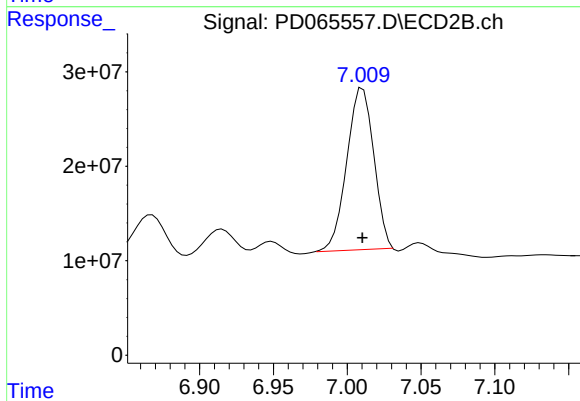

#27 Chlordane-5


R.T.: 7.011 min
Delta R.T.: 0.000 min
Response: 218190936
Conc: 899.54 ng/ml

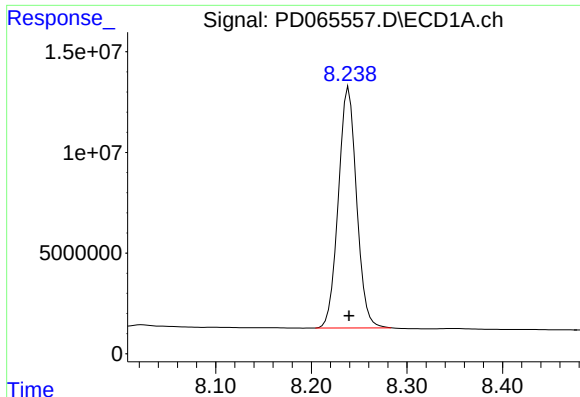

#28 Decachlorobiphenyl

R.T.: 8.239 min
Delta R.T.: 0.000 min
Response: 158512961
Conc: 88.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

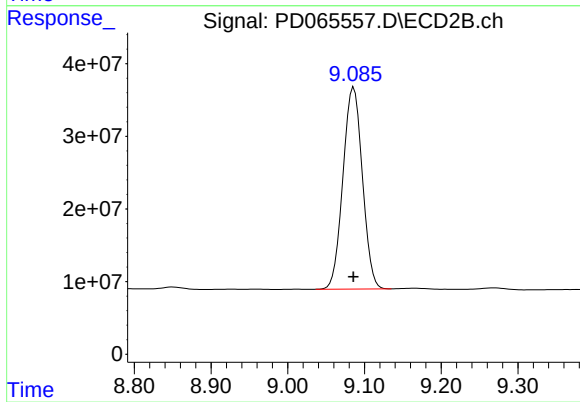

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 491367384
Conc: 87.83 ng/ml