

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090421\
 Data File : PD065560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2021 19:48
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:05:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 04 01:04:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.014	30161958	201.4E6	23.884	25.388
28)	SA Decachlor...	8.239	9.085	46051105	143.6E6	25.701	25.675
Target Compounds							
23)	Chlordane-1	4.365	5.009	10559851	81223958	246.646	259.345
24)	Chlordane-2	4.865	5.479	13960223	73715555	260.568	263.115
25)	Chlordane-3	5.431	6.127	37174054	264.2E6	237.707	249.766
26)	Chlordane-4	5.490	6.200	31211907	310.3E6	244.028	251.890
27)	Chlordane-5	6.326	7.010	15415639	60165959	246.070	248.048



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090421\
Data File : PD065560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2021 19:48
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleID :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:05:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Sat Sep 04 01:04:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

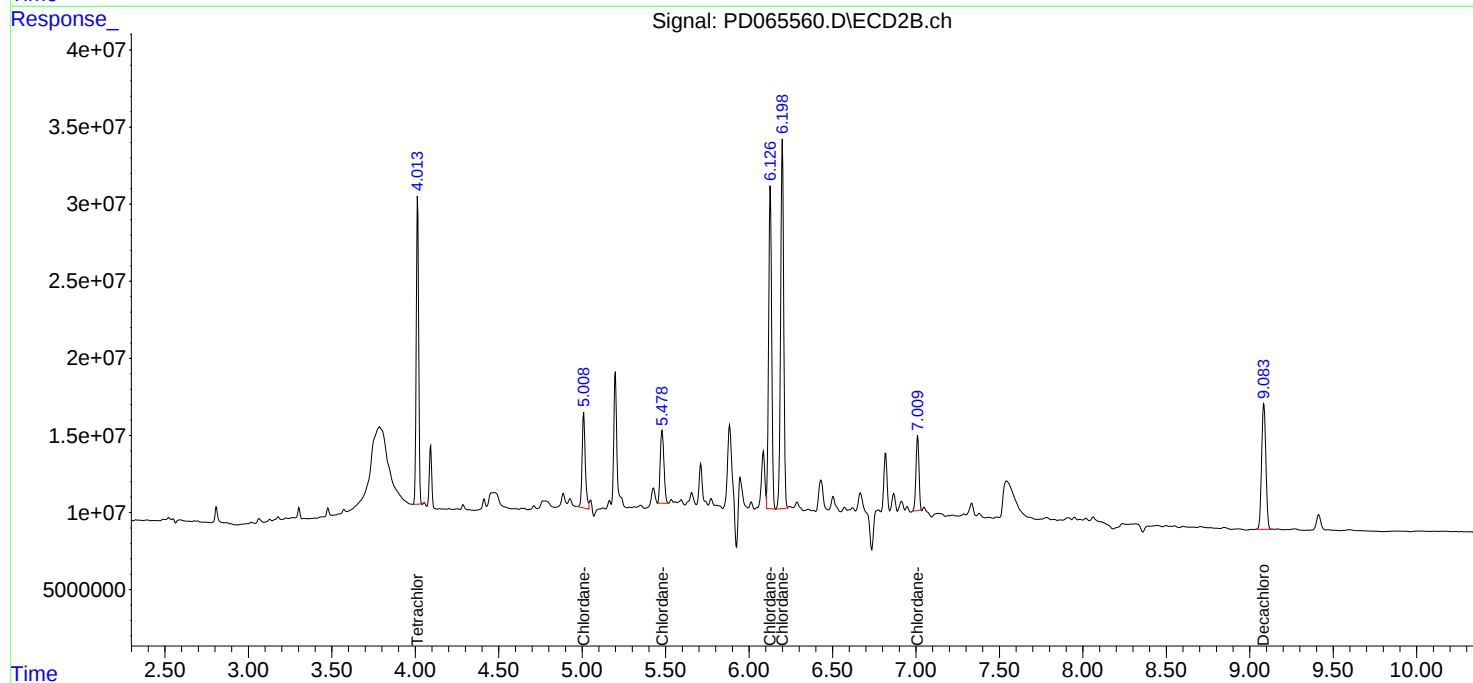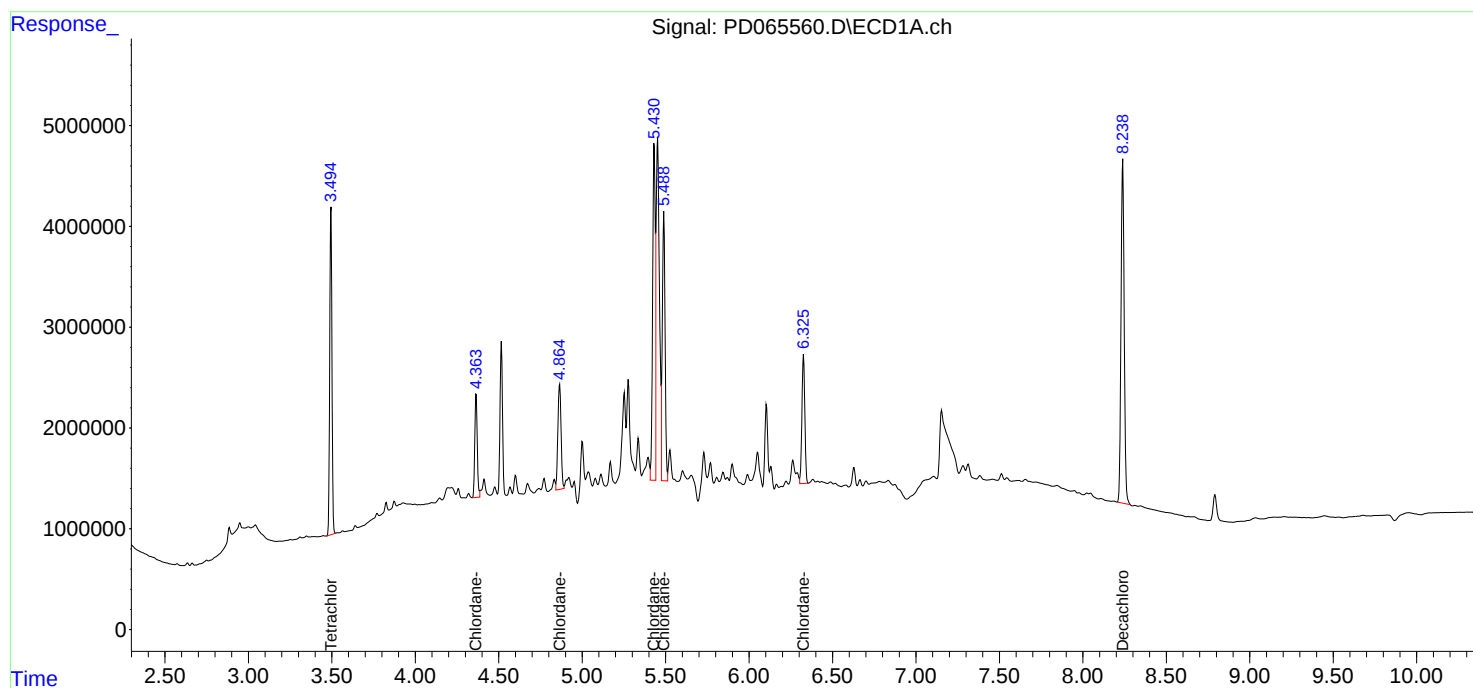


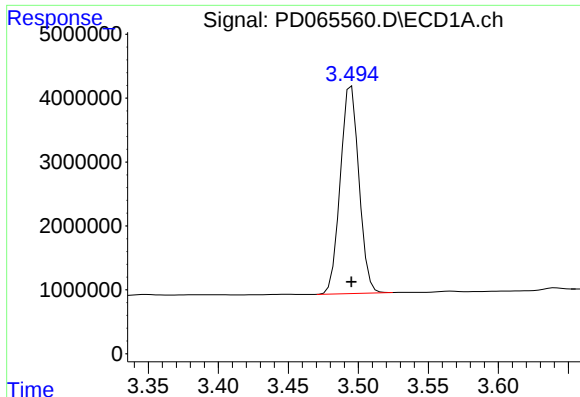

#1 Tetrachloro-m-xylene


R.T.: 3.495 min
Delta R.T.: 0.000 min
Response: 30161958
Conc: 23.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

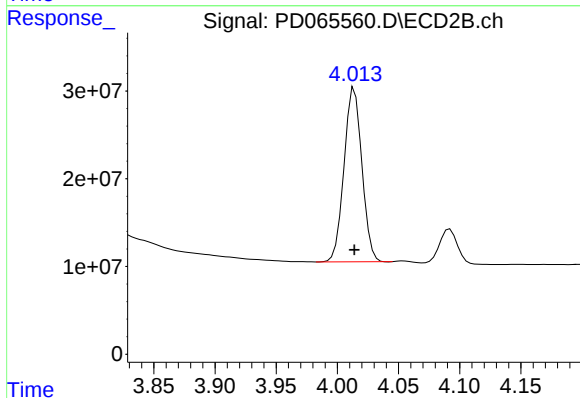


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 201402841
Conc: 25.39 ng/ml

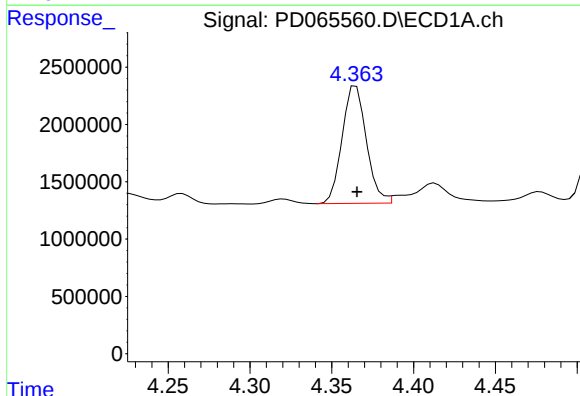


#23 Chlordane-1

R.T.: 4.365 min
Delta R.T.: 0.000 min
Response: 10559851
Conc: 246.65 ng/ml

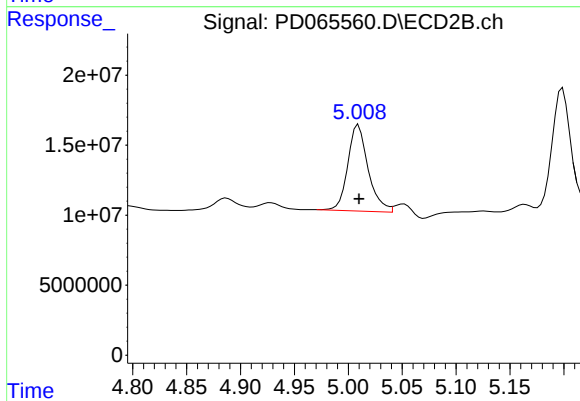

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 81223958
Conc: 259.34 ng/ml

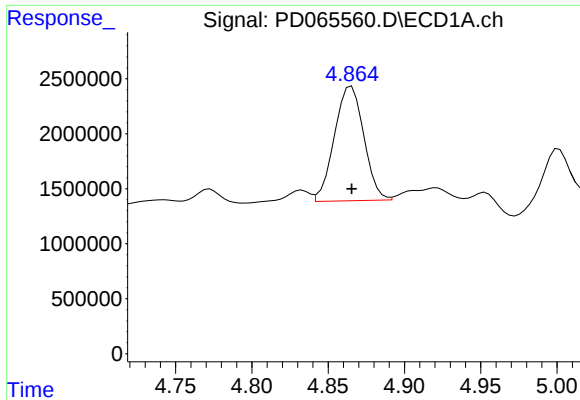

#24 Chlordane-2


R.T.: 4.865 min
Delta R.T.: 0.000 min
Response: 13960223
Conc: 260.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

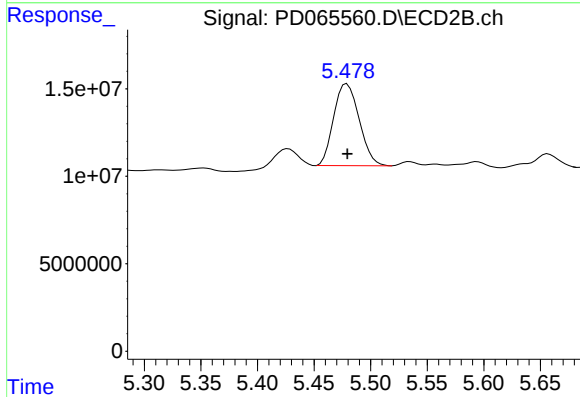


#24 Chlordane-2

R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 73715555
Conc: 263.12 ng/ml

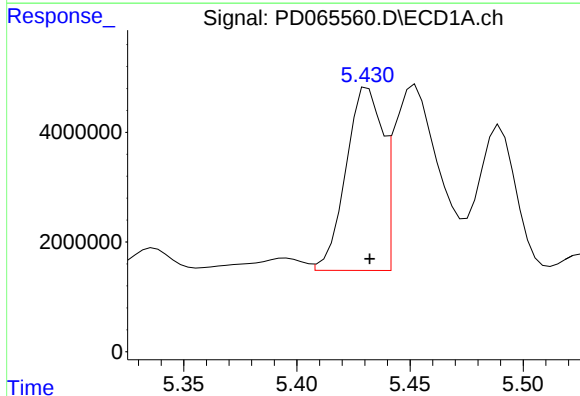


#25 Chlordane-3

R.T.: 5.431 min
Delta R.T.: 0.000 min
Response: 37174054
Conc: 237.71 ng/ml

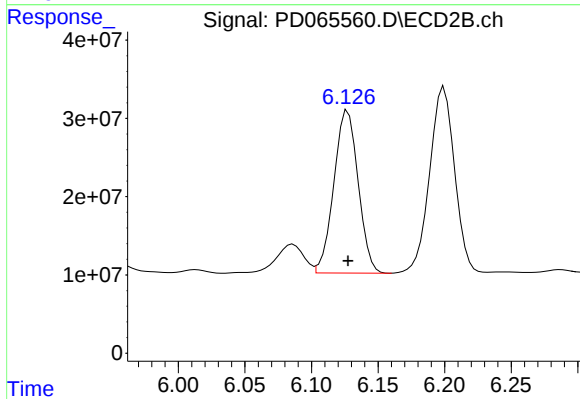

#25 Chlordane-3


R.T.: 6.127 min
Delta R.T.: 0.000 min
Response: 264199645
Conc: 249.77 ng/ml

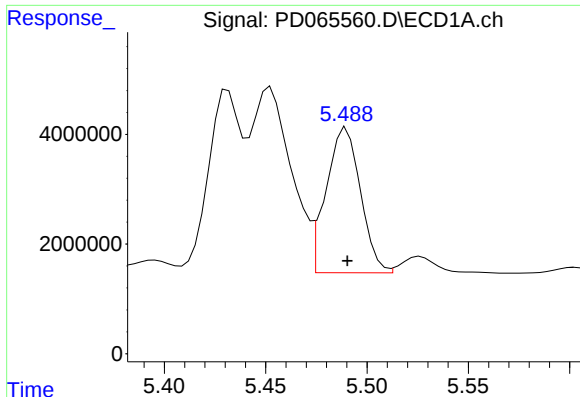

#26 Chlordane-4


R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 31211907
Conc: 244.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

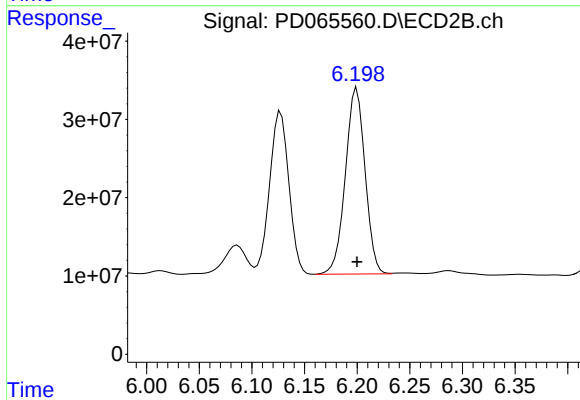


#26 Chlordane-4

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 310319208
Conc: 251.89 ng/ml

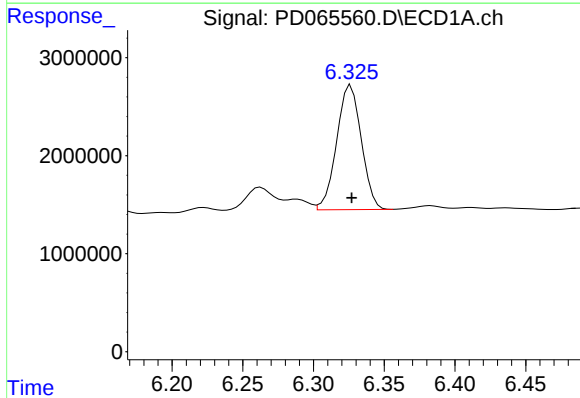


#27 Chlordane-5

R.T.: 6.326 min
Delta R.T.: 0.000 min
Response: 15415639
Conc: 246.07 ng/ml

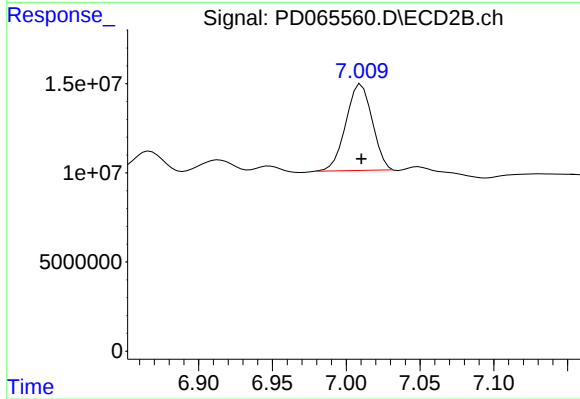

#27 Chlordane-5


R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 60165959
Conc: 248.05 ng/ml

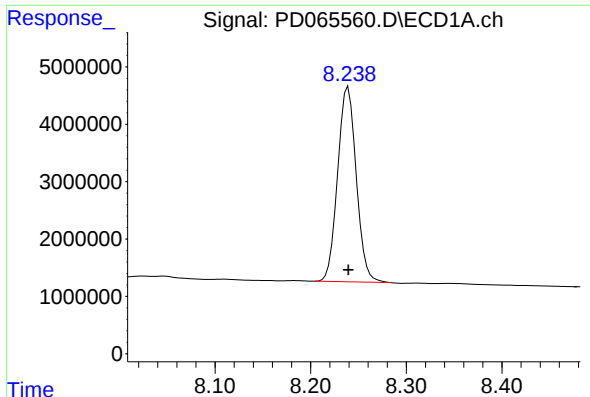

#28 Decachlorobiphenyl

R.T.: 8.239 min
Delta R.T.: 0.000 min
Response: 46051105
Conc: 25.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

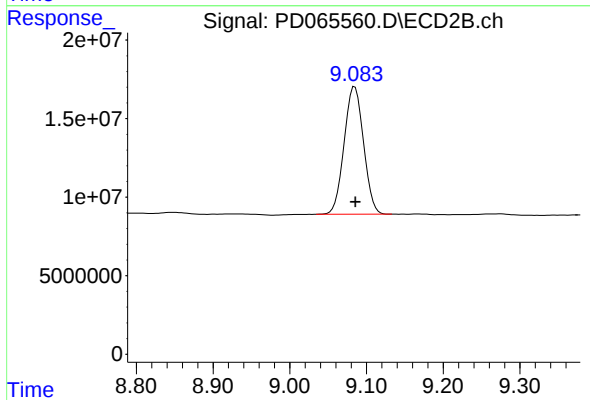

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 143641196
Conc: 25.67 ng/ml