

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090421\
 Data File : PD065568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Sep 2021 21:38
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD090421CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 04 01:21:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 04 01:20:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.014	62292521	387.9E6	51.800	49.874
28)	SA Decachlor...	8.238	9.084	89226925	280.0E6	49.809	51.002
Target Compounds							
23)	Chlordane-1	4.365	5.009	21126202	159.9E6	510.917	548.121
24)	Chlordane-2	4.865	5.479	26617121	138.0E6	512.376	490.288
25)	Chlordane-3	5.432	6.126	77274154	519.6E6	516.033	503.388
26)	Chlordane-4	5.489	6.200	63269444	608.1E6	510.683	503.876
27)	Chlordane-5	6.326	7.010	30852359	120.2E6	511.314	512.773



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090421\
Data File : PD065568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Sep 2021 21:38
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD090421CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 01:21:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Sat Sep 04 01:20:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

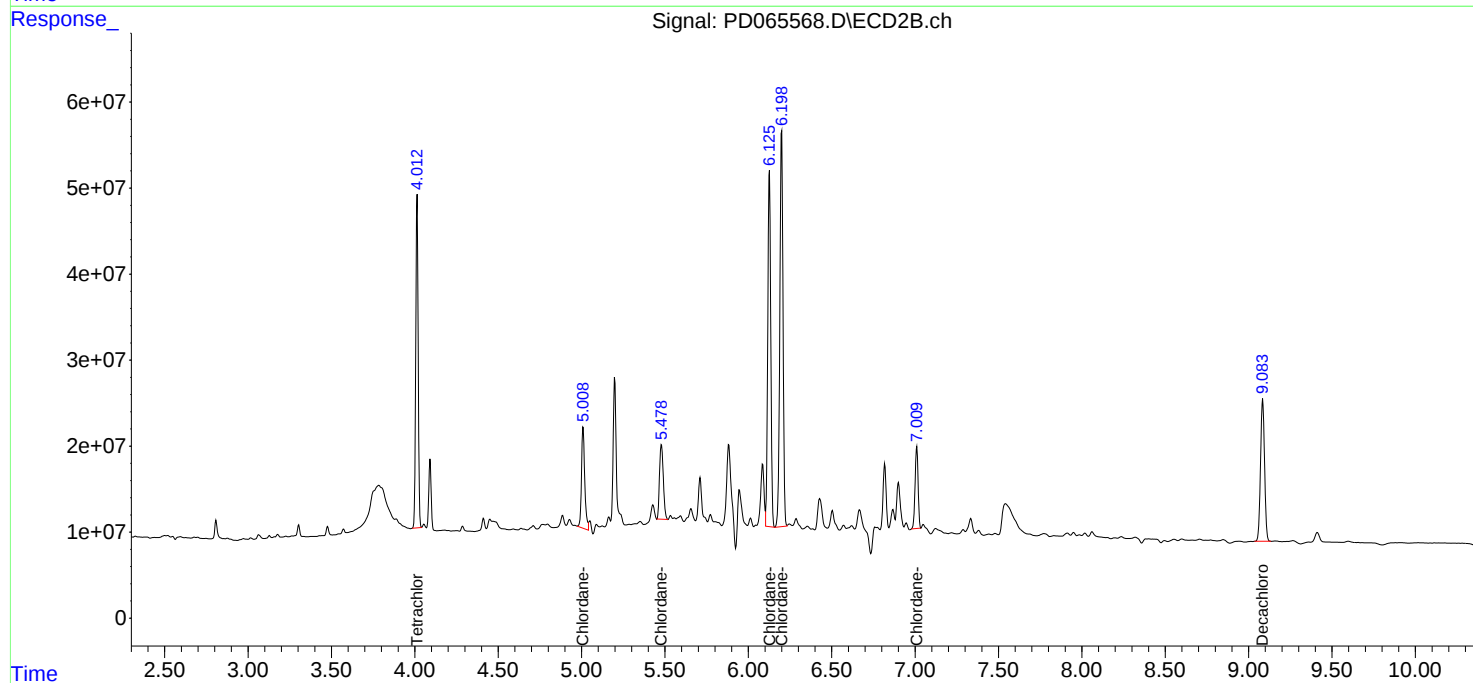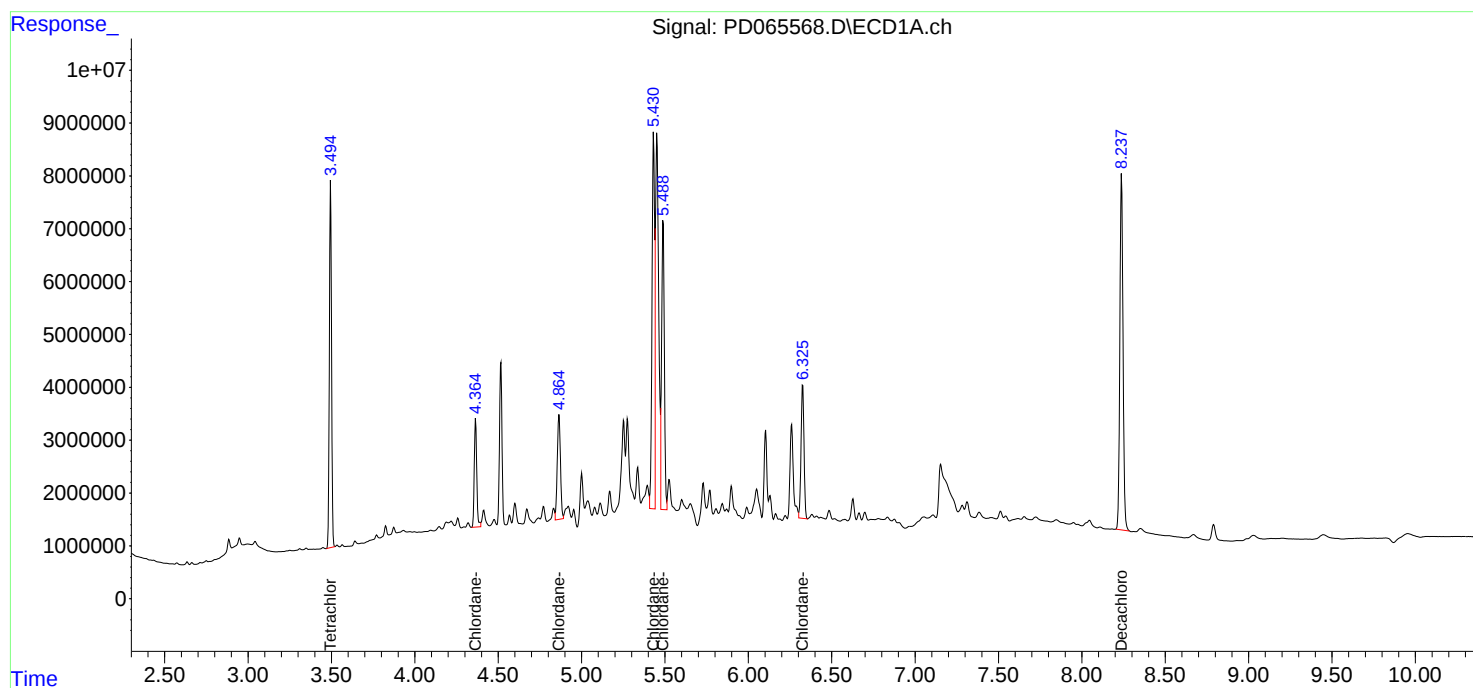


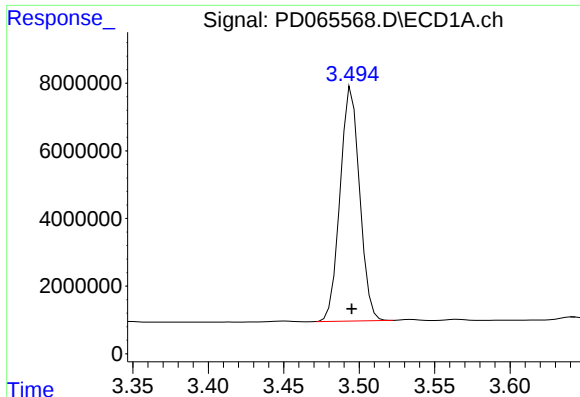

#1 Tetrachloro-m-xylene


R.T.: 3.495 min
Delta R.T.: 0.000 min
Response: 62292521
Conc: 51.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD090421CHLOR

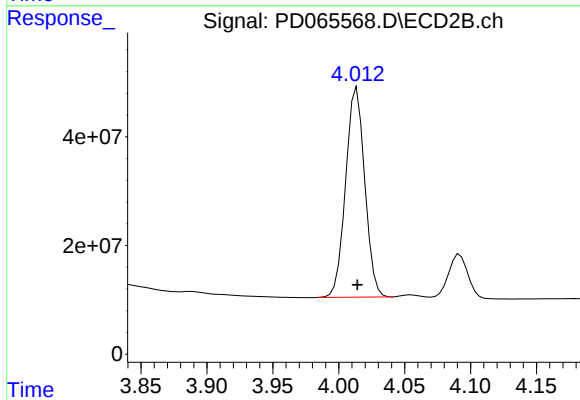


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 387916565
Conc: 49.87 ng/ml

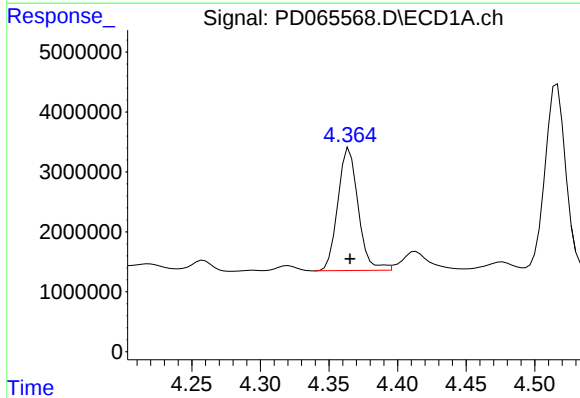


#23 Chlordane-1

R.T.: 4.365 min
Delta R.T.: 0.000 min
Response: 21126202
Conc: 510.92 ng/ml

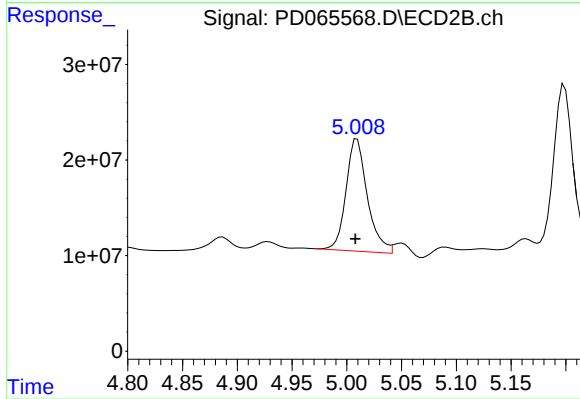

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.001 min
Response: 159859551
Conc: 548.12 ng/ml

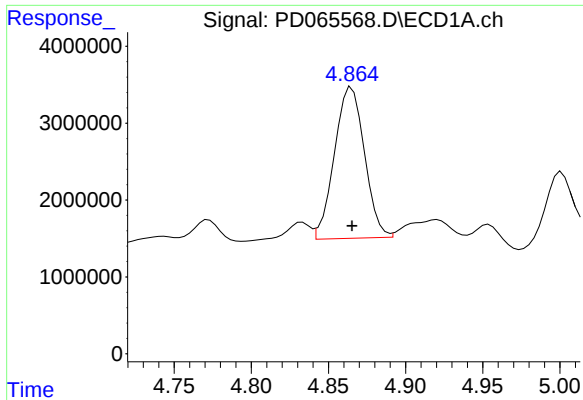

#24 Chlordane-2


R.T.: 4.865 min
Delta R.T.: 0.000 min
Response: 26617121
Conc: 512.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD090421CHLOR

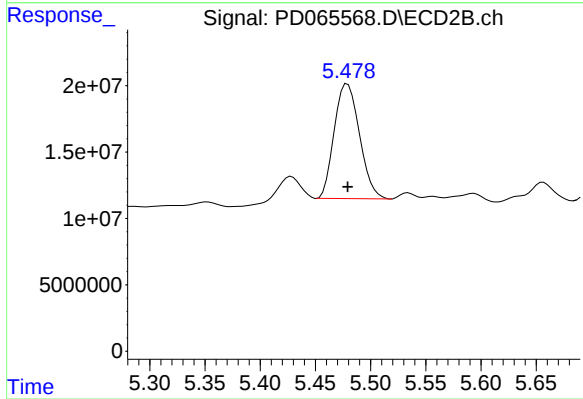


#24 Chlordane-2

R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 137994507
Conc: 490.29 ng/ml

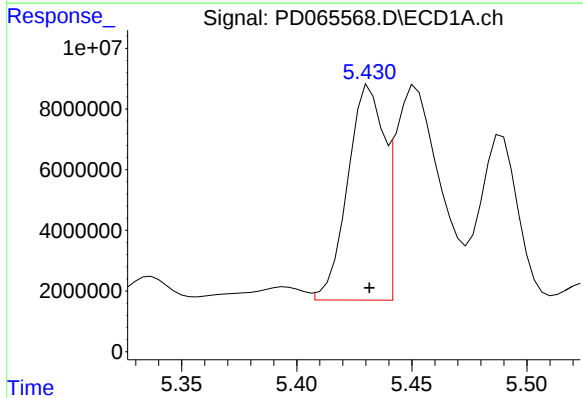


#25 Chlordane-3

R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 77274154
Conc: 516.03 ng/ml

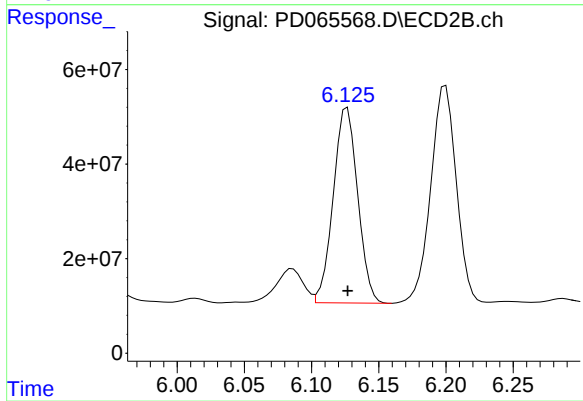

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 519626809
Conc: 503.39 ng/ml

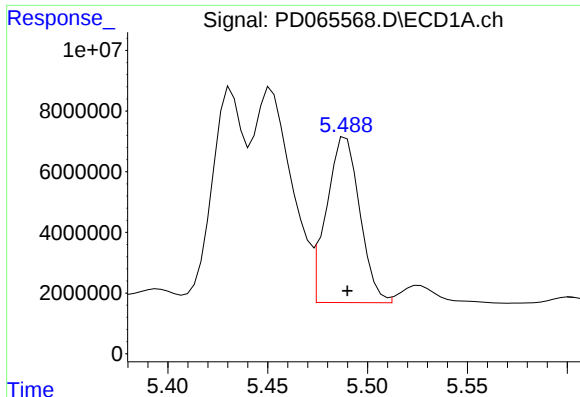

#26 Chlordane-4


R.T.: 5.489 min
Delta R.T.: 0.000 min
Response: 63269444
Conc: 510.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD090421CHLOR

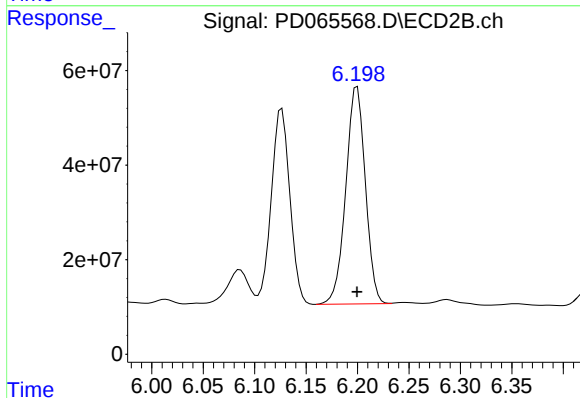


#26 Chlordane-4

R.T.: 6.200 min
Delta R.T.: 0.000 min
Response: 608109227
Conc: 503.88 ng/ml

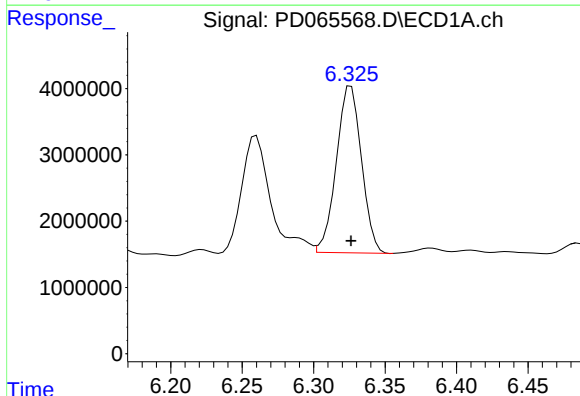


#27 Chlordane-5

R.T.: 6.326 min
Delta R.T.: 0.000 min
Response: 30852359
Conc: 511.31 ng/ml

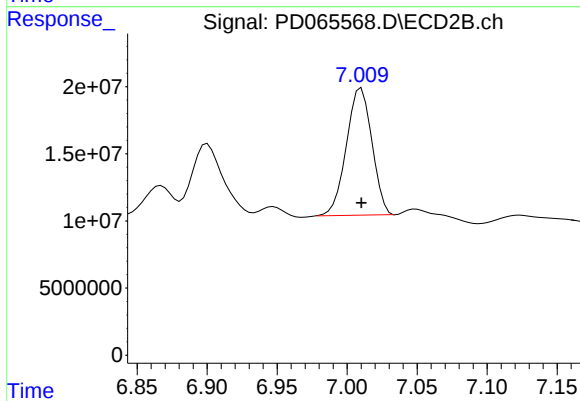

#27 Chlordane-5


R.T.: 7.010 min
Delta R.T.: 0.000 min
Response: 120248774
Conc: 512.77 ng/ml

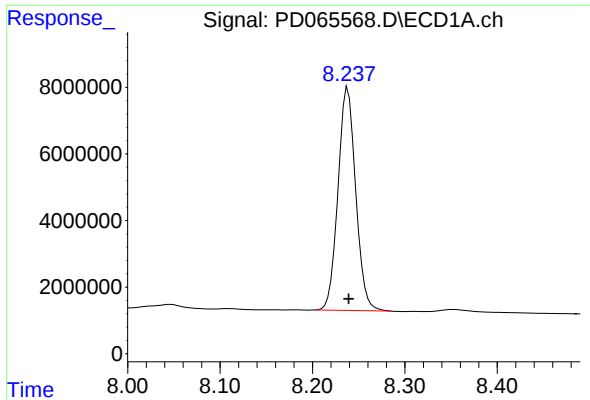

#28 Decachlorobiphenyl

R.T.: 8.238 min
Delta R.T.: 0.000 min
Response: 89226925
Conc: 49.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD090421CHLOR

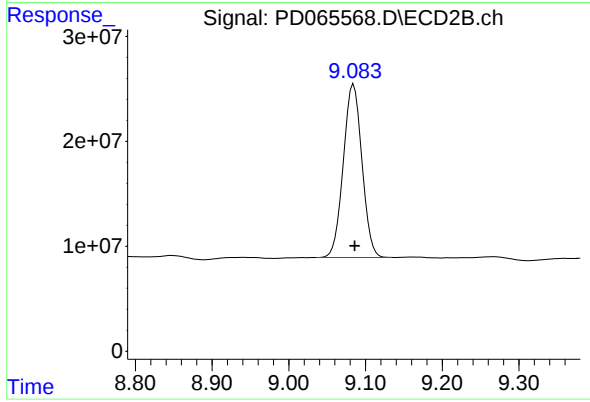

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.002 min
Response: 280010953
Conc: 51.00 ng/ml