

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED



Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

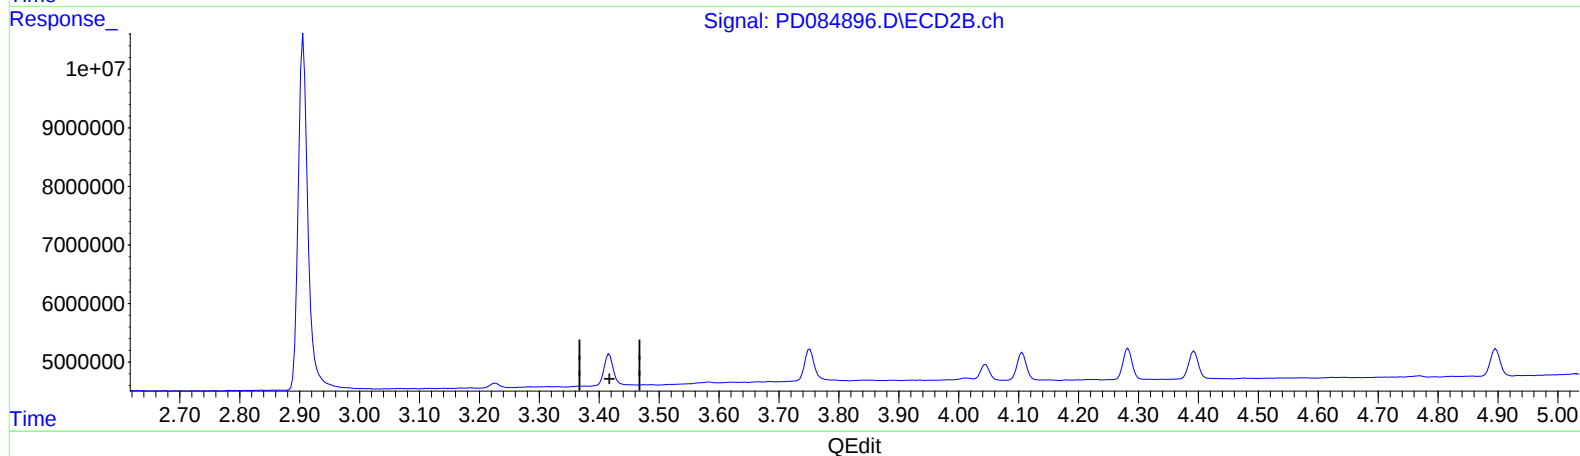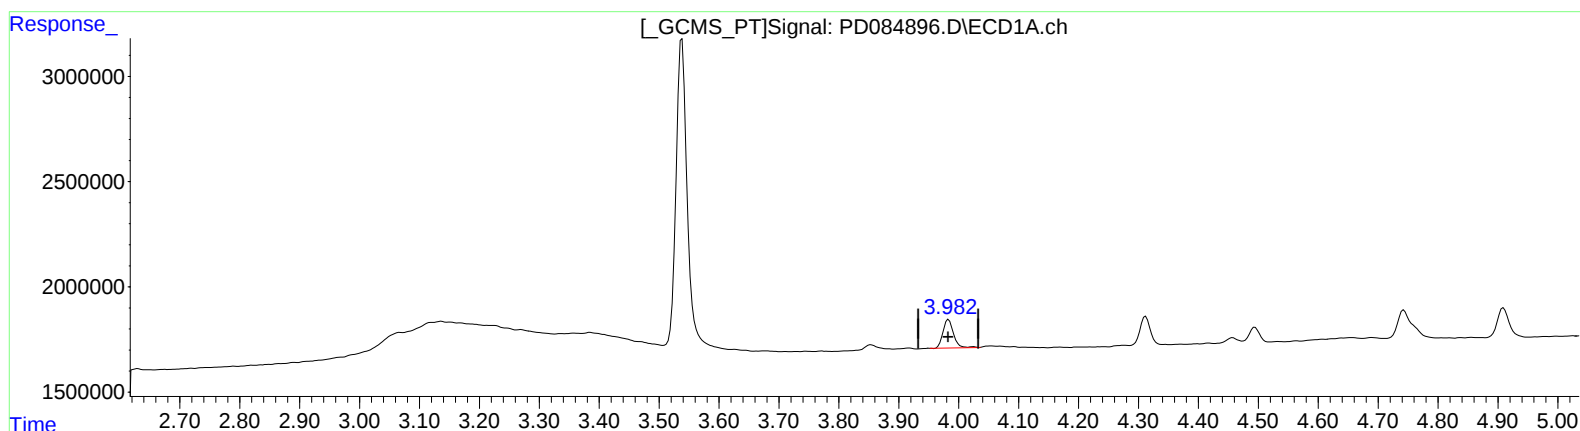

(2) alpha-BHC (A)  
3.983min 0.972 ng/ml  
response 1653057

(2) alpha-BHC #2 (A)  
0.000min 0.000 ng/ml  
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

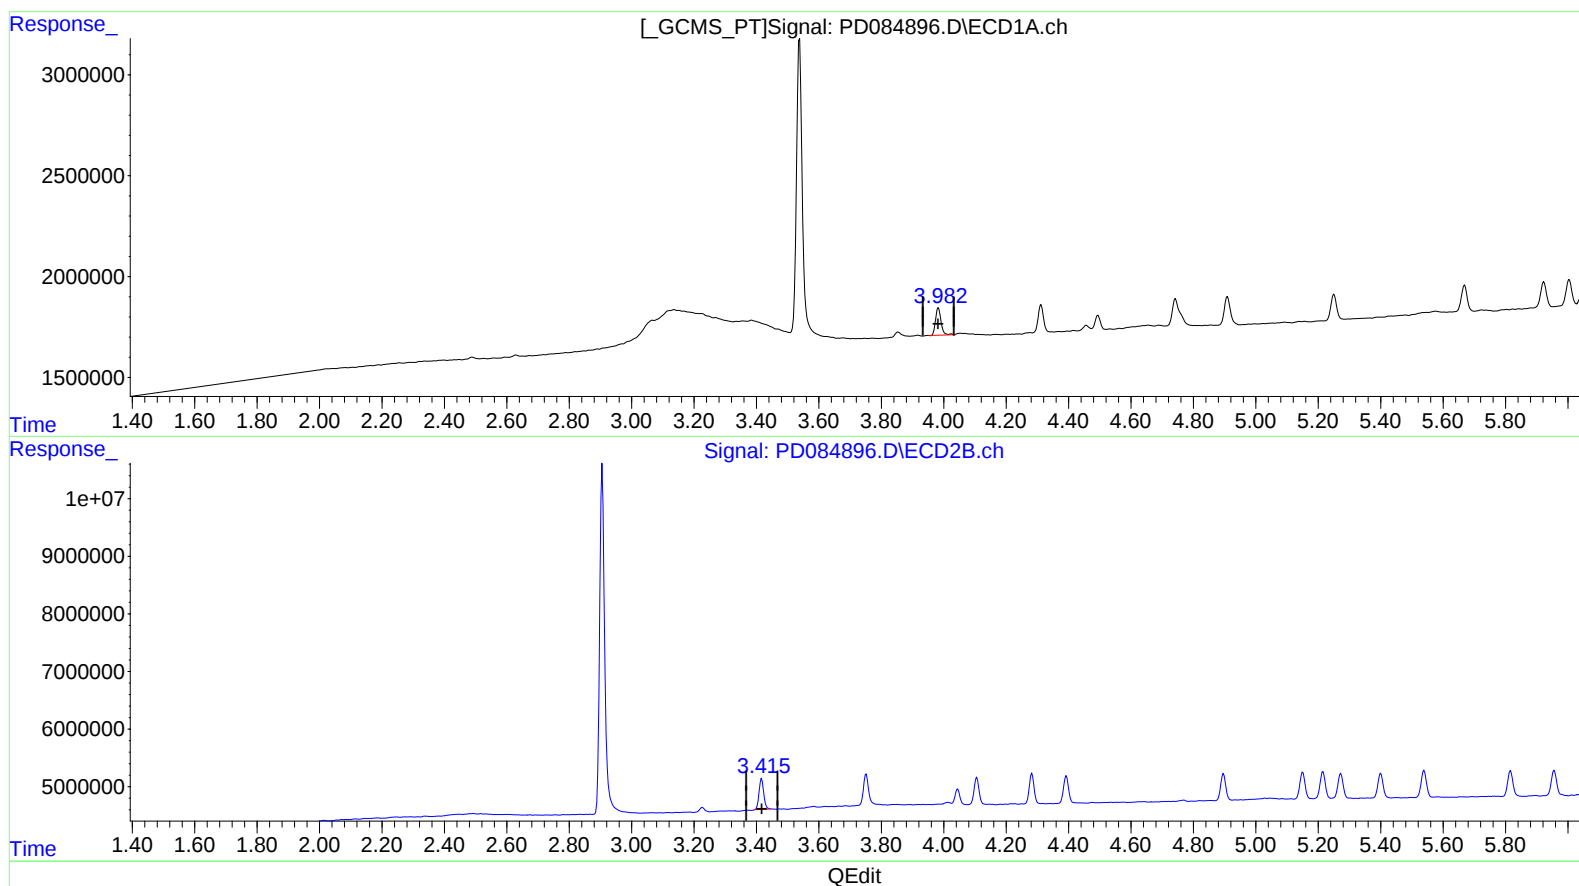

(2) alpha-BHC (A)  
3.983min 0.972 ng/ml  
response 1653057

(2) alpha-BHC #2 (A)  
3.415min 1.091 ng/ml m  
response 5530693

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

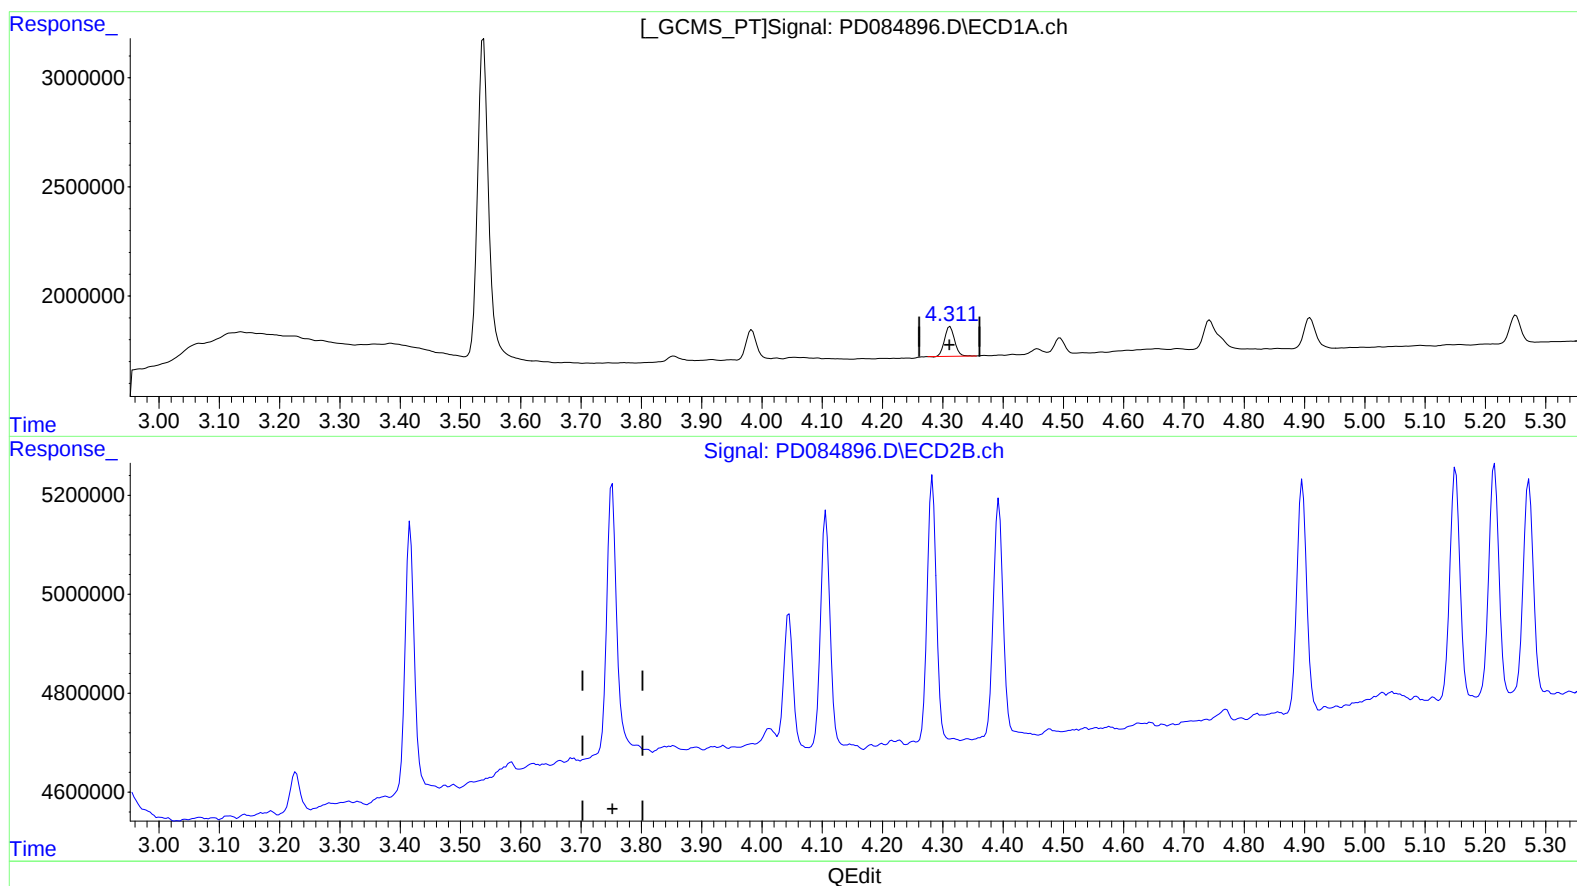

(3) gamma-BHC (Lindane) (MA)

4.312min 0.984 ng/ml

response 1591912

(3) gamma-BHC (Lindane) #2 (MA)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

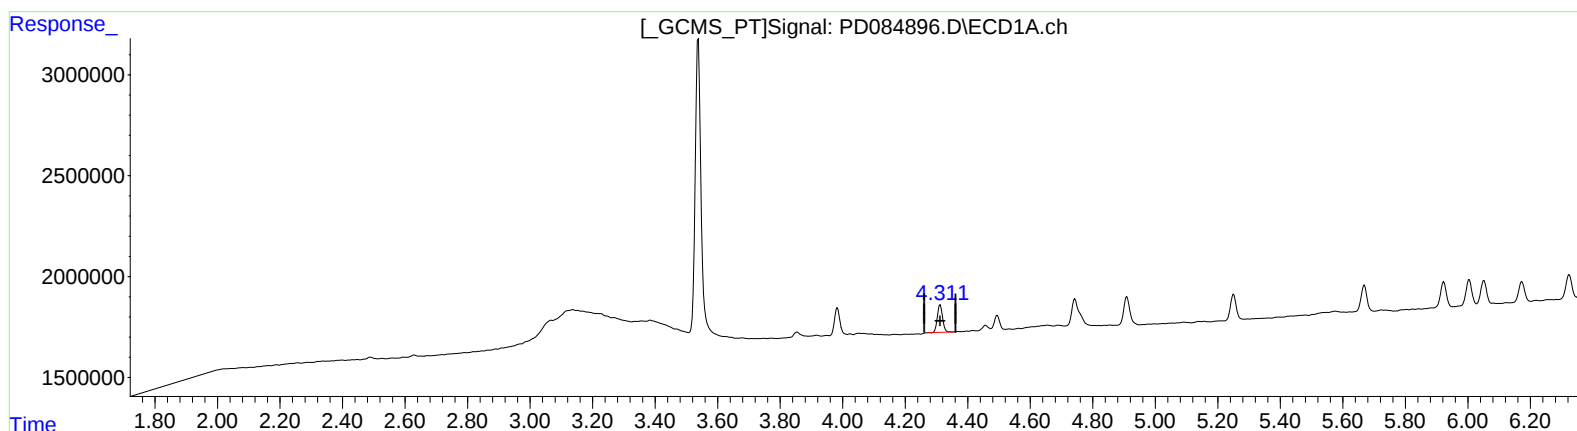

(3) gamma-BHC (Lindane) (MA)

4.312min 0.984 ng/ml

response 1591912

(3) gamma-BHC (Lindane) #2 (MA)

3.750min 1.288 ng/ml m

response 6240197

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

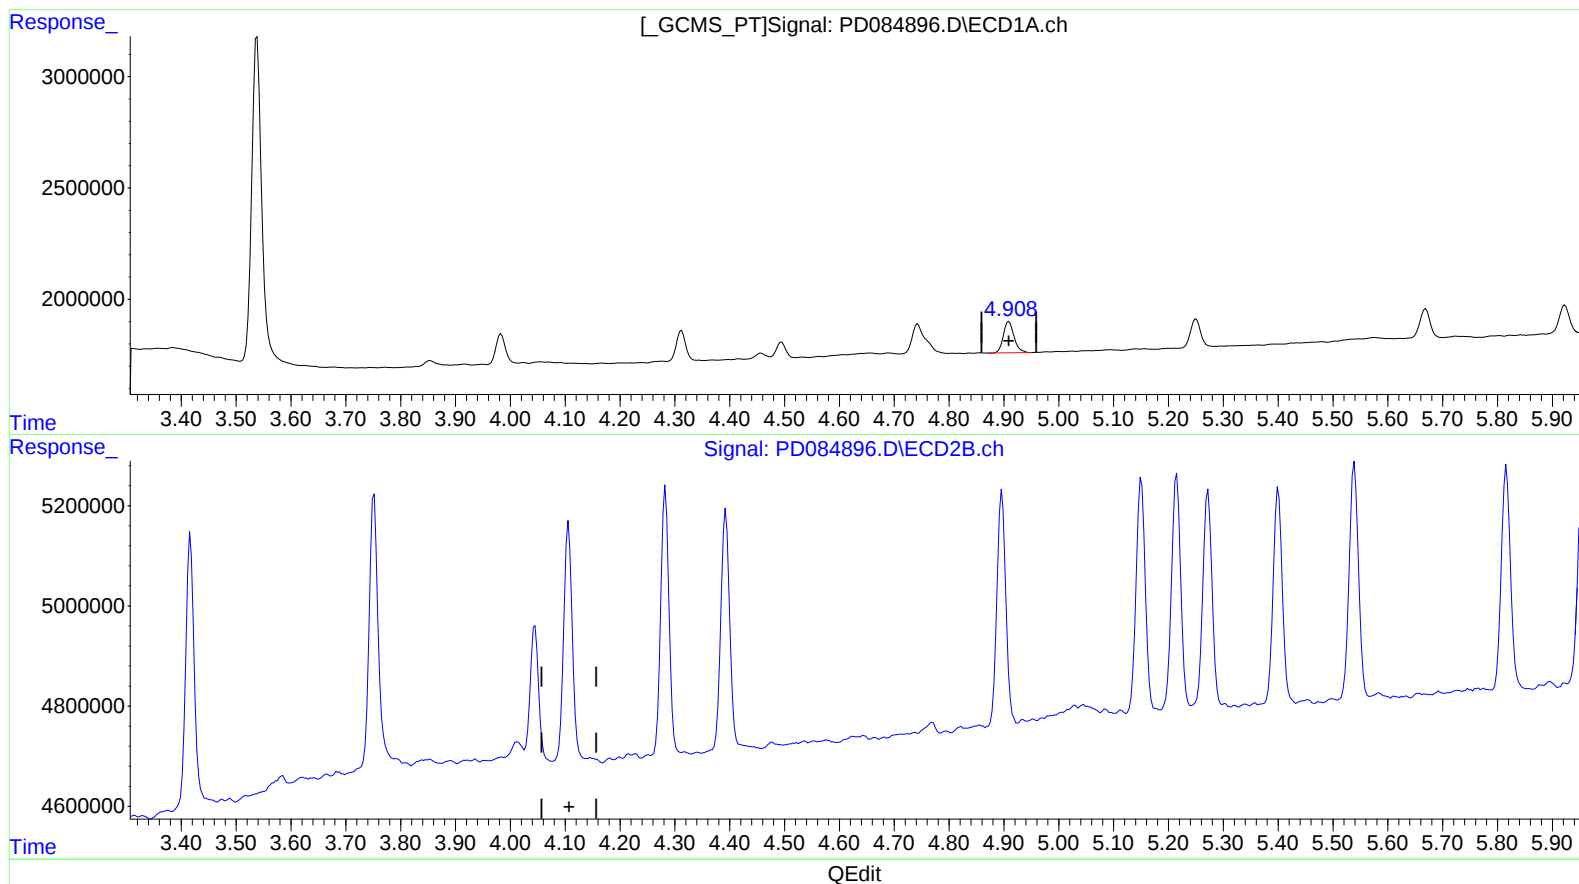

(4) Heptachlor (MA)  
4.909min 1.239 ng/ml  
response 1905797

(4) Heptachlor #2 (MA)  
0.000min 0.000 ng/ml  
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED



Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

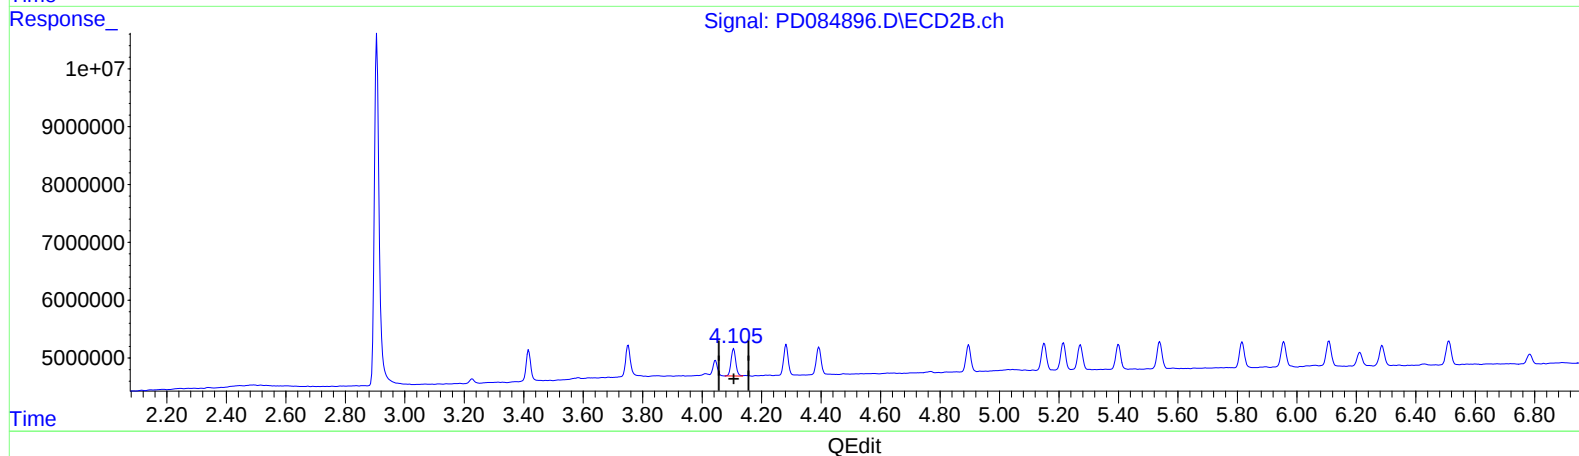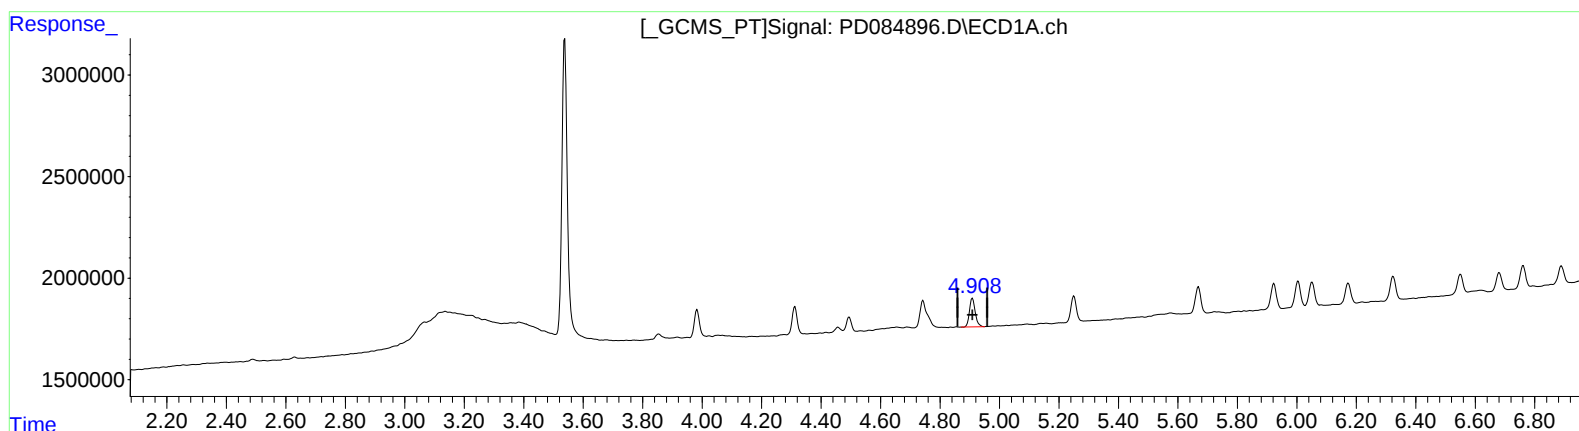

(4) Heptachlor (MA)

4.909min 1.239 ng/ml

response 1905797

(4) Heptachlor #2 (MA)

4.105min 1.229 ng/ml m

response 5233105

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

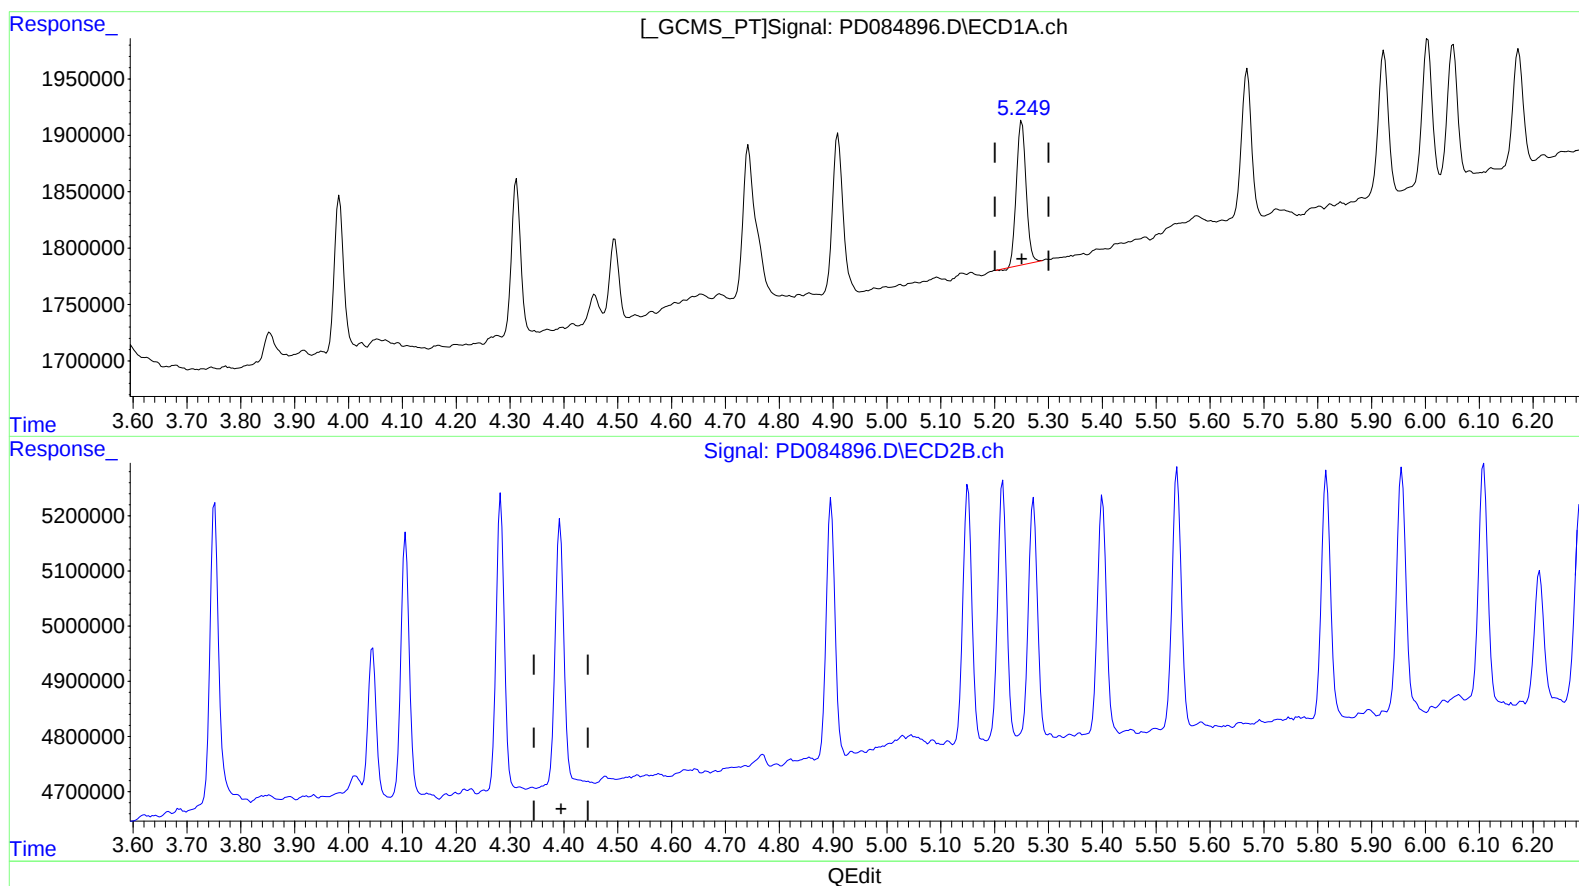

(5) Aldrin (MB)

5.251min 0.995 ng/ml

response 1591792

(5) Aldrin #2 (MB)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

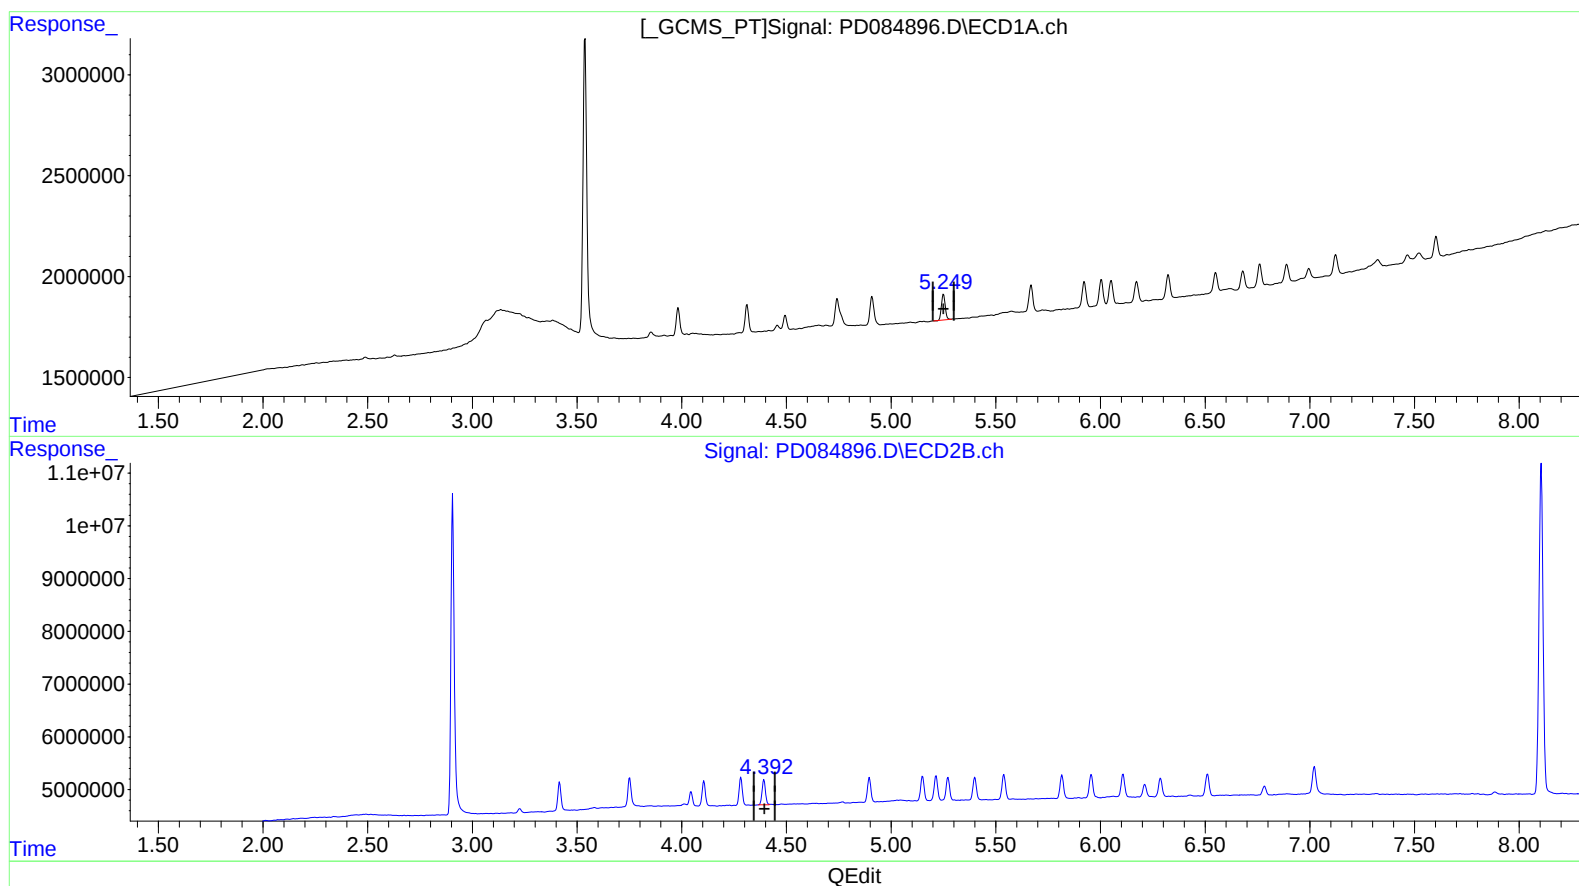

(5) Aldrin (MB)

5.251min 0.995 ng/ml

response 1591792

(5) Aldrin #2 (MB)

4.392min 1.205 ng/ml m

response 5350680

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

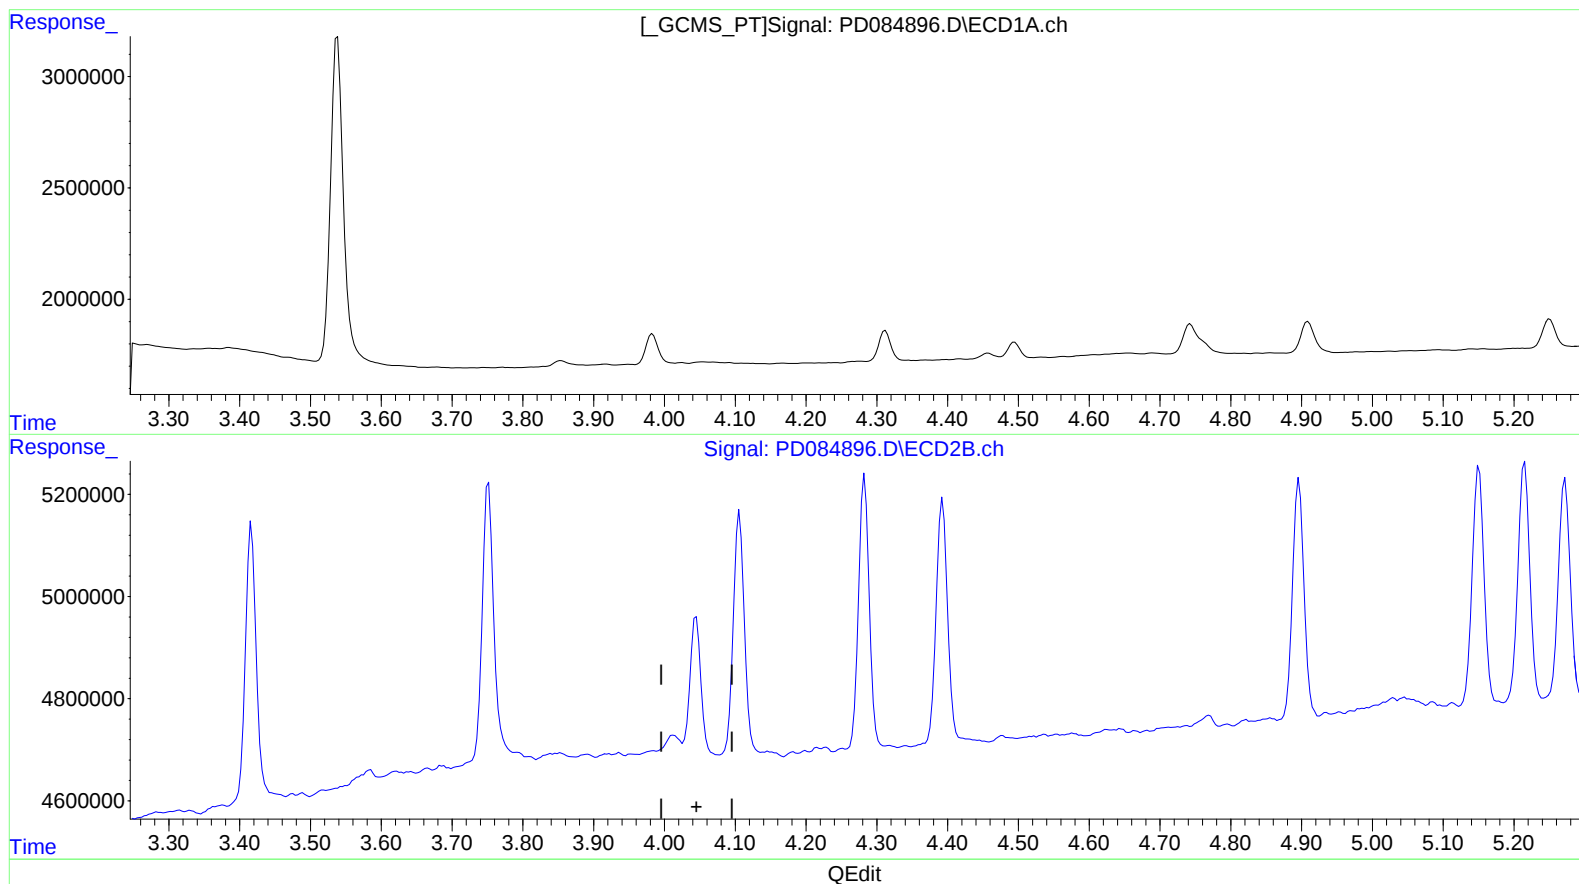

(6) beta-BHC (B)

0.000min 0.000 ng/ml

response 0

(6) beta-BHC #2 (B)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED



Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

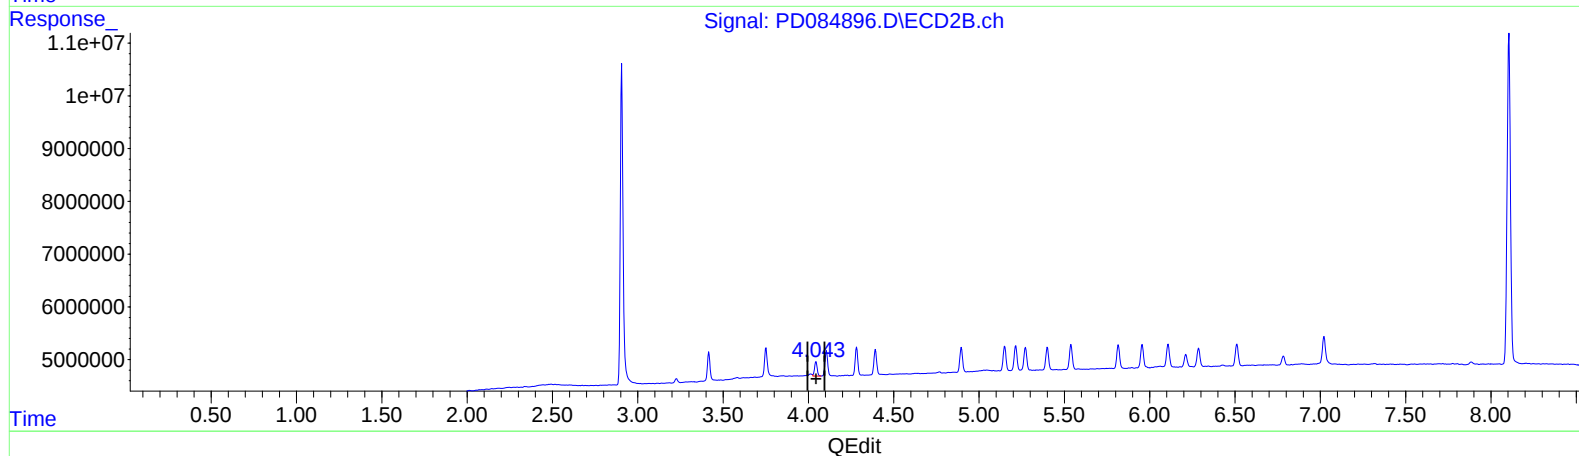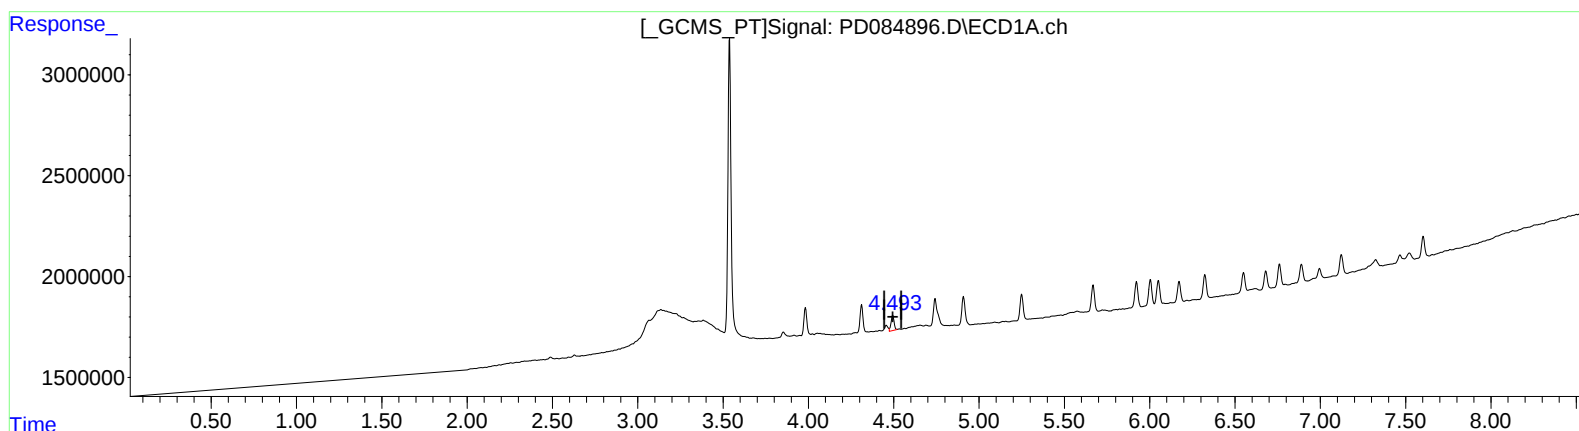

(6) beta-BHC (B)

4.493min 1.287 ng/ml m  
response 935081

(6) beta-BHC #2 (B)

4.043min 1.348 ng/ml m  
response 2921310

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

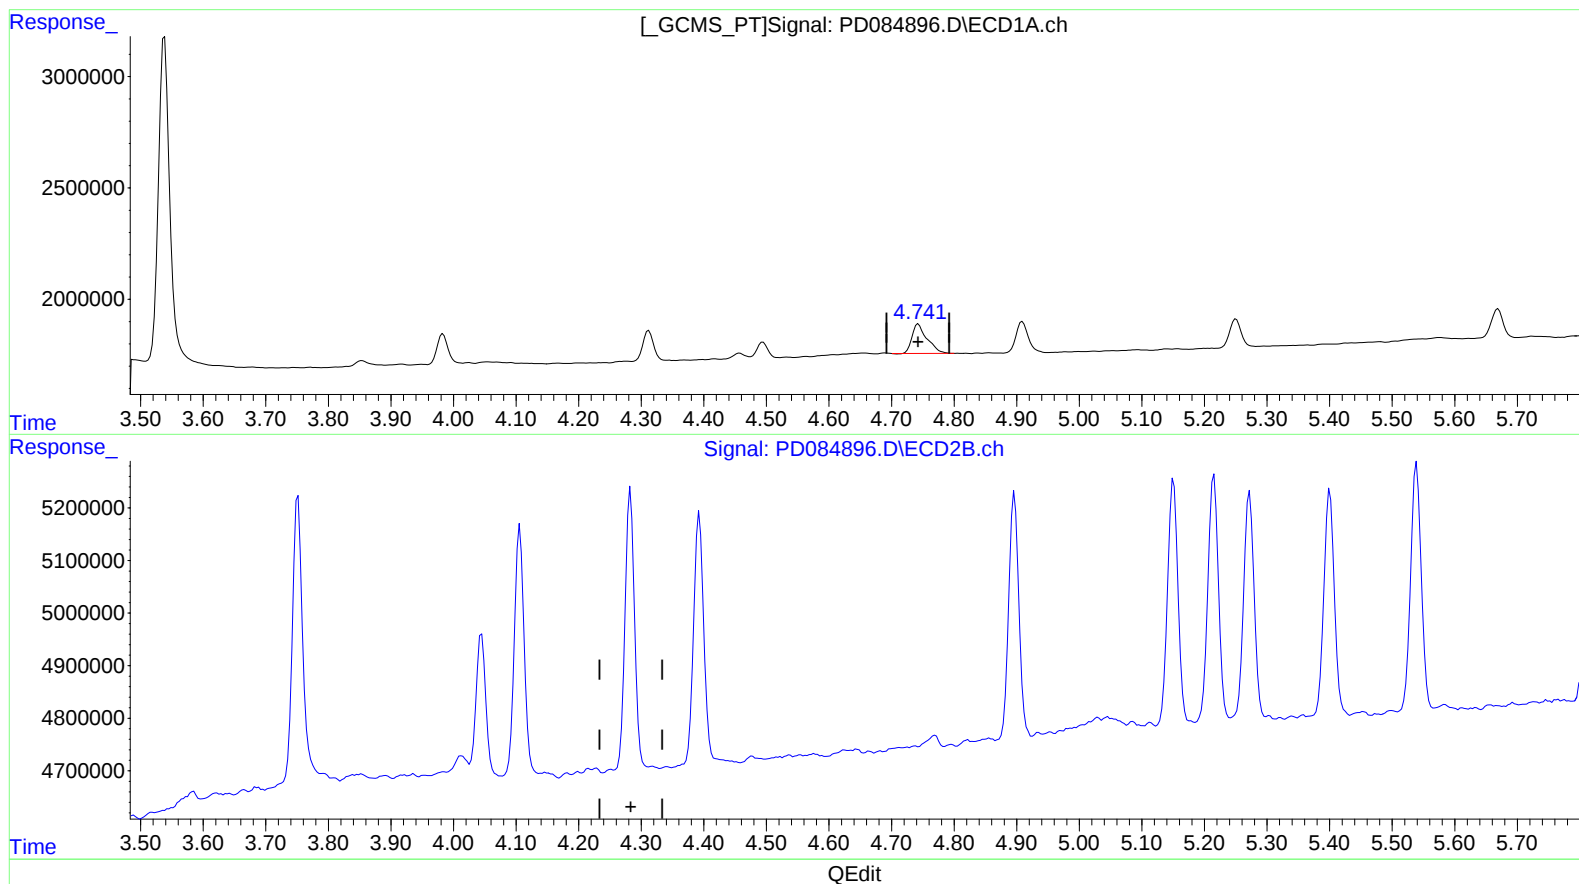

(7) delta-BHC (B)  
4.743min 1.338 ng/ml  
response 2193934

(7) delta-BHC #2 (B)  
0.000min 0.000 ng/ml  
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

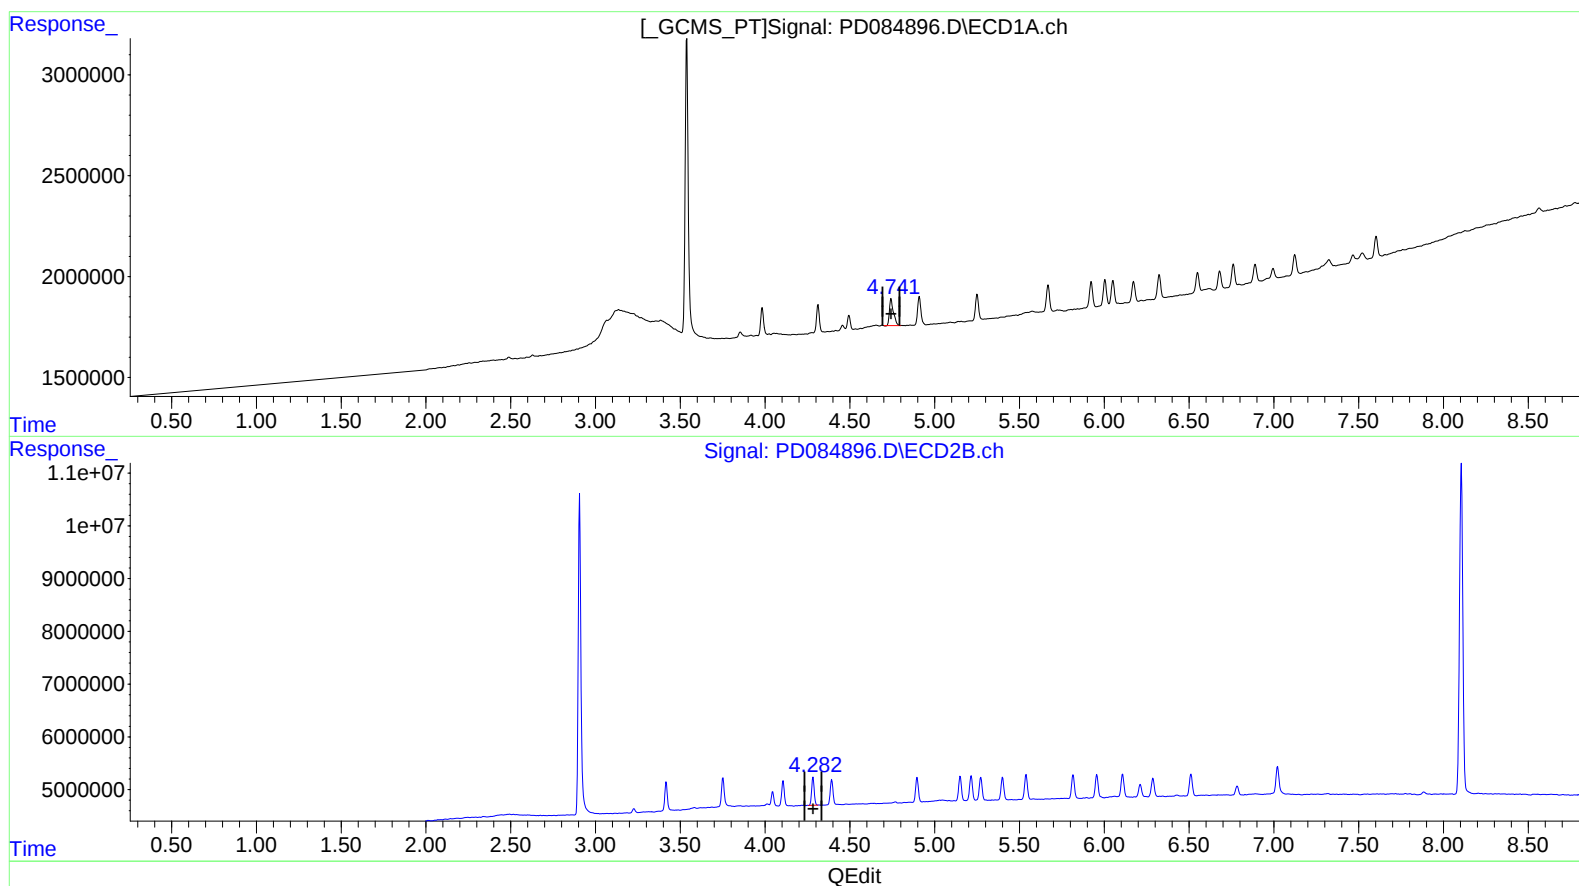

(7) delta-BHC (B)

4.743min 1.338 ng/ml  
response 2193934

(7) delta-BHC #2 (B)

4.282min 1.123 ng/ml m  
response 5574597

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

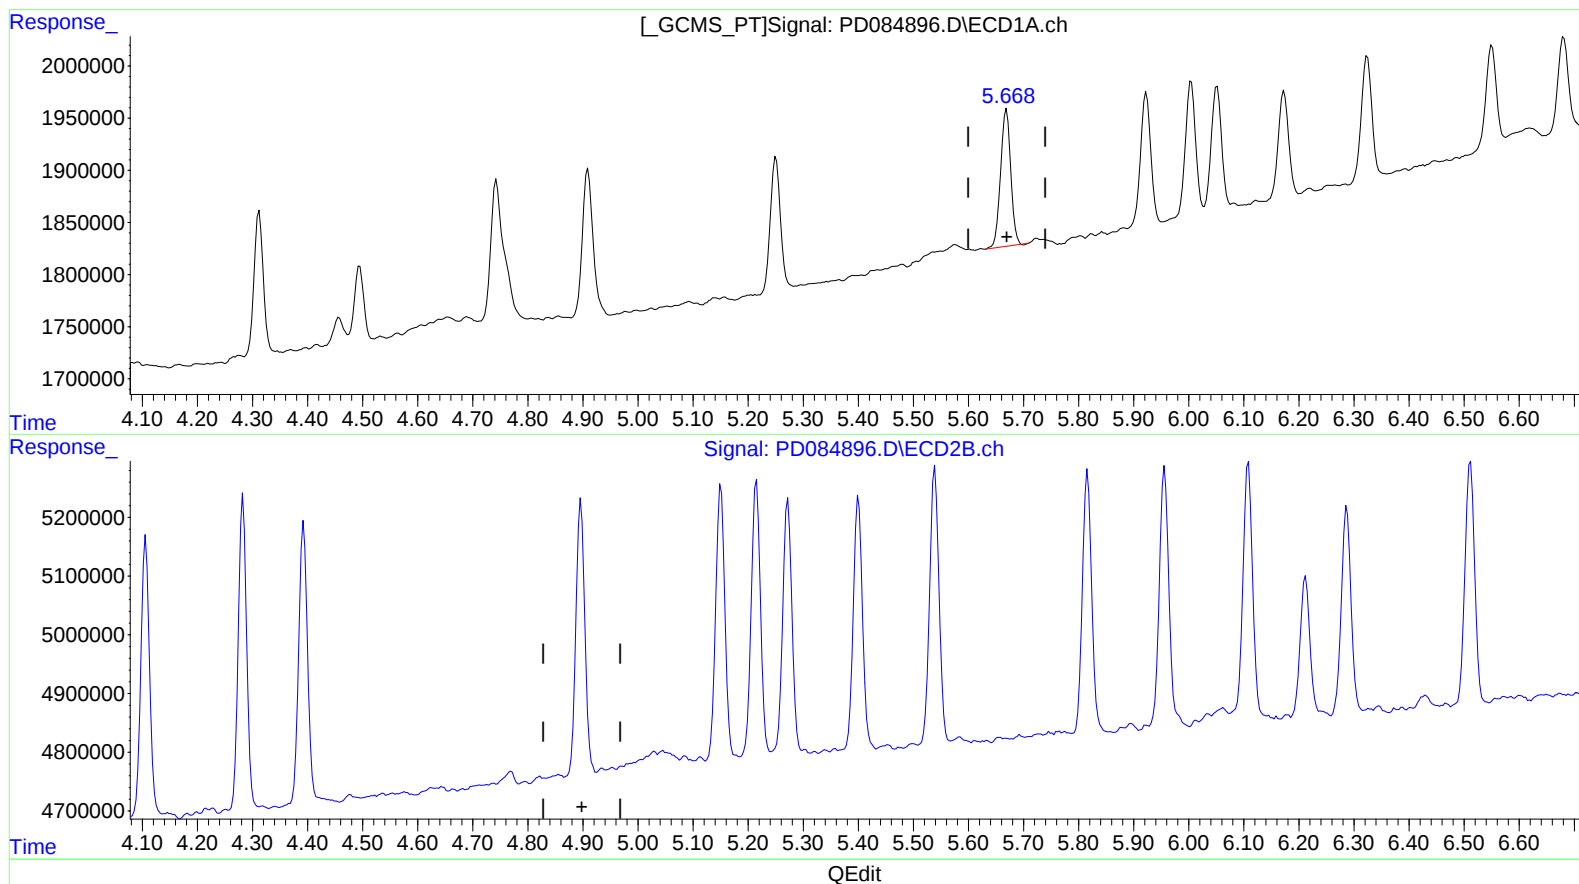

(8) Heptachlor epoxide (B)

5.669min 1.130 ng/ml

response 1685497

(8) Heptachlor epoxide #2 (B)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED



Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

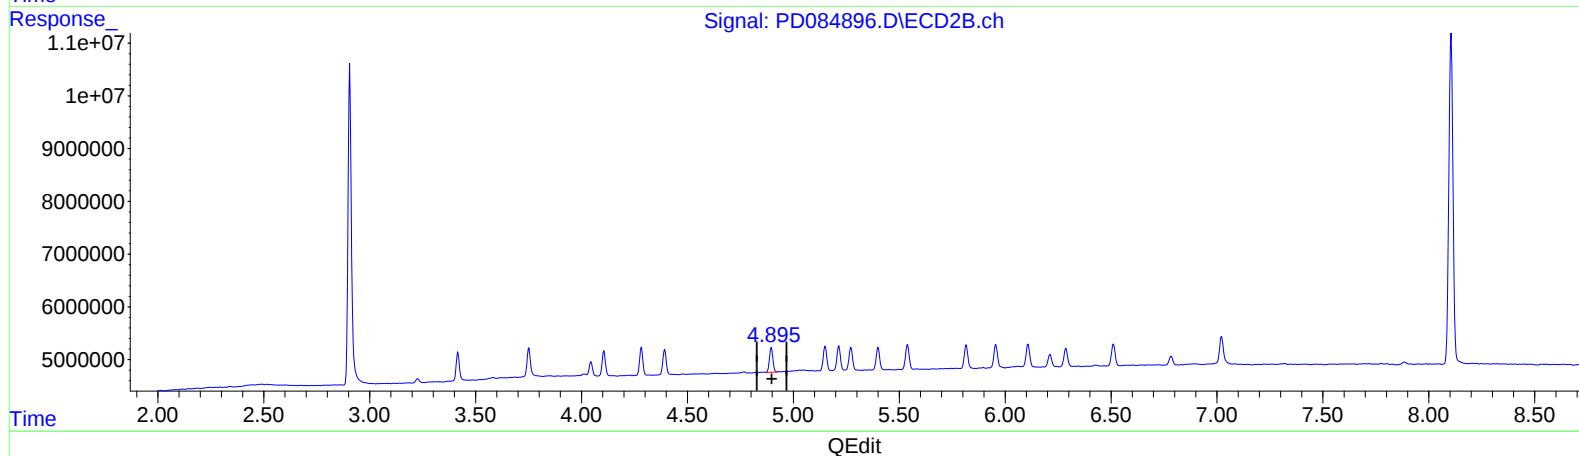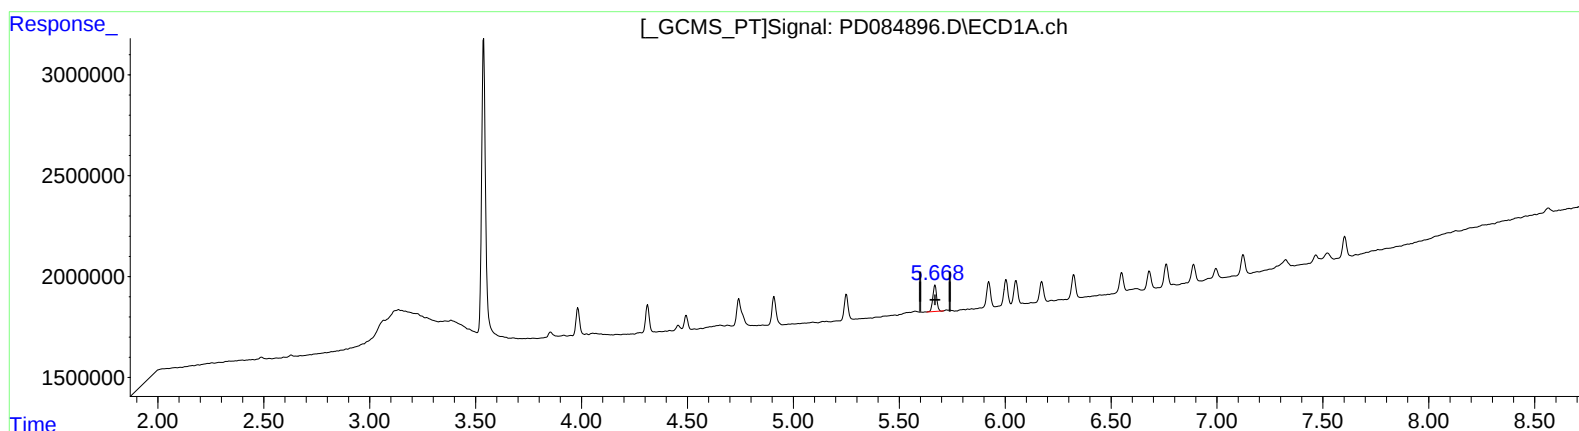

(8) Heptachlor epoxide (B)

5.669min 1.130 ng/ml

response 1685497

(8) Heptachlor epoxide #2 (B)

4.895min 1.247 ng/ml m

response 5280068

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

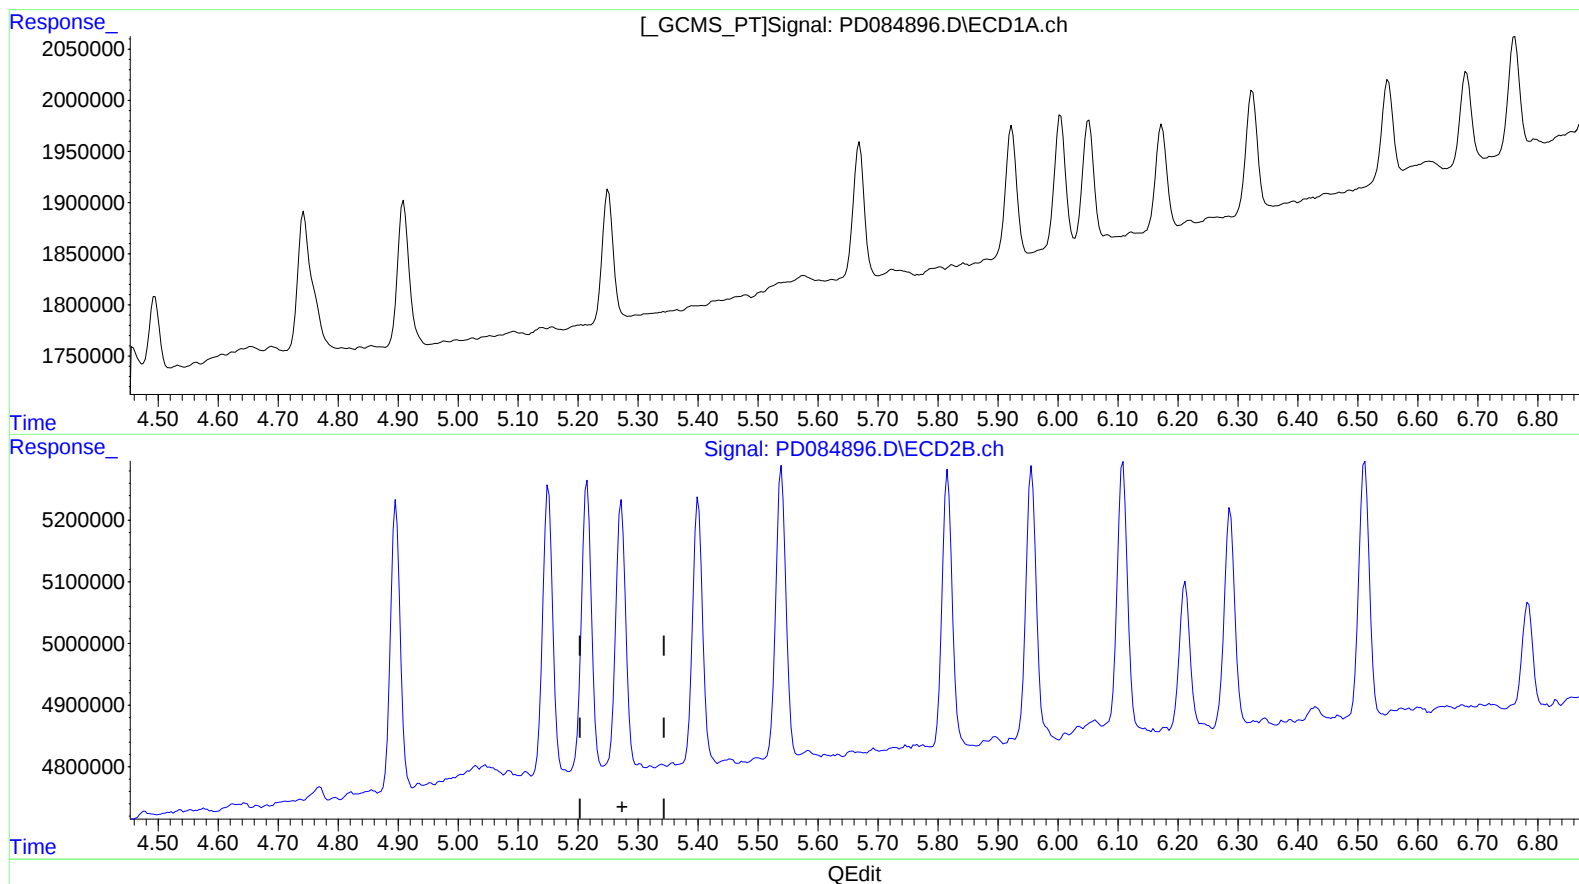

(9) Endosulfan I (A)

0.000min 0.000 ng/ml

response 0

(9) Endosulfan I #2 (A)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED



Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

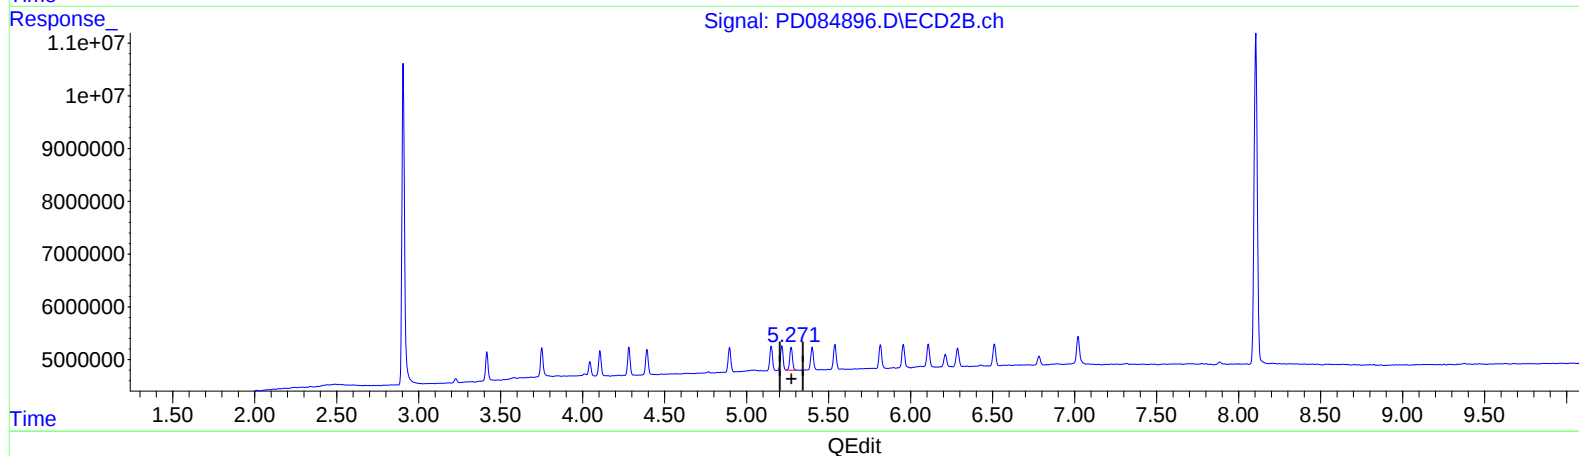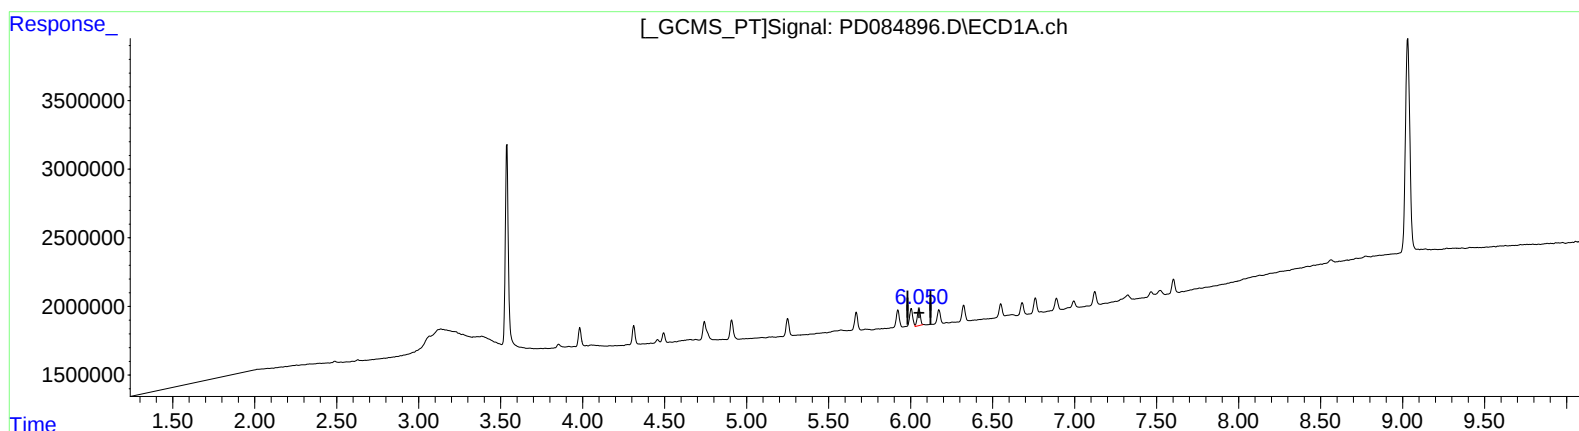

(9) Endosulfan I (A)

6.050min 1.174 ng/ml m

response 1614561

(9) Endosulfan I #2 (A)

5.271min 1.303 ng/ml m

response 4995294

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

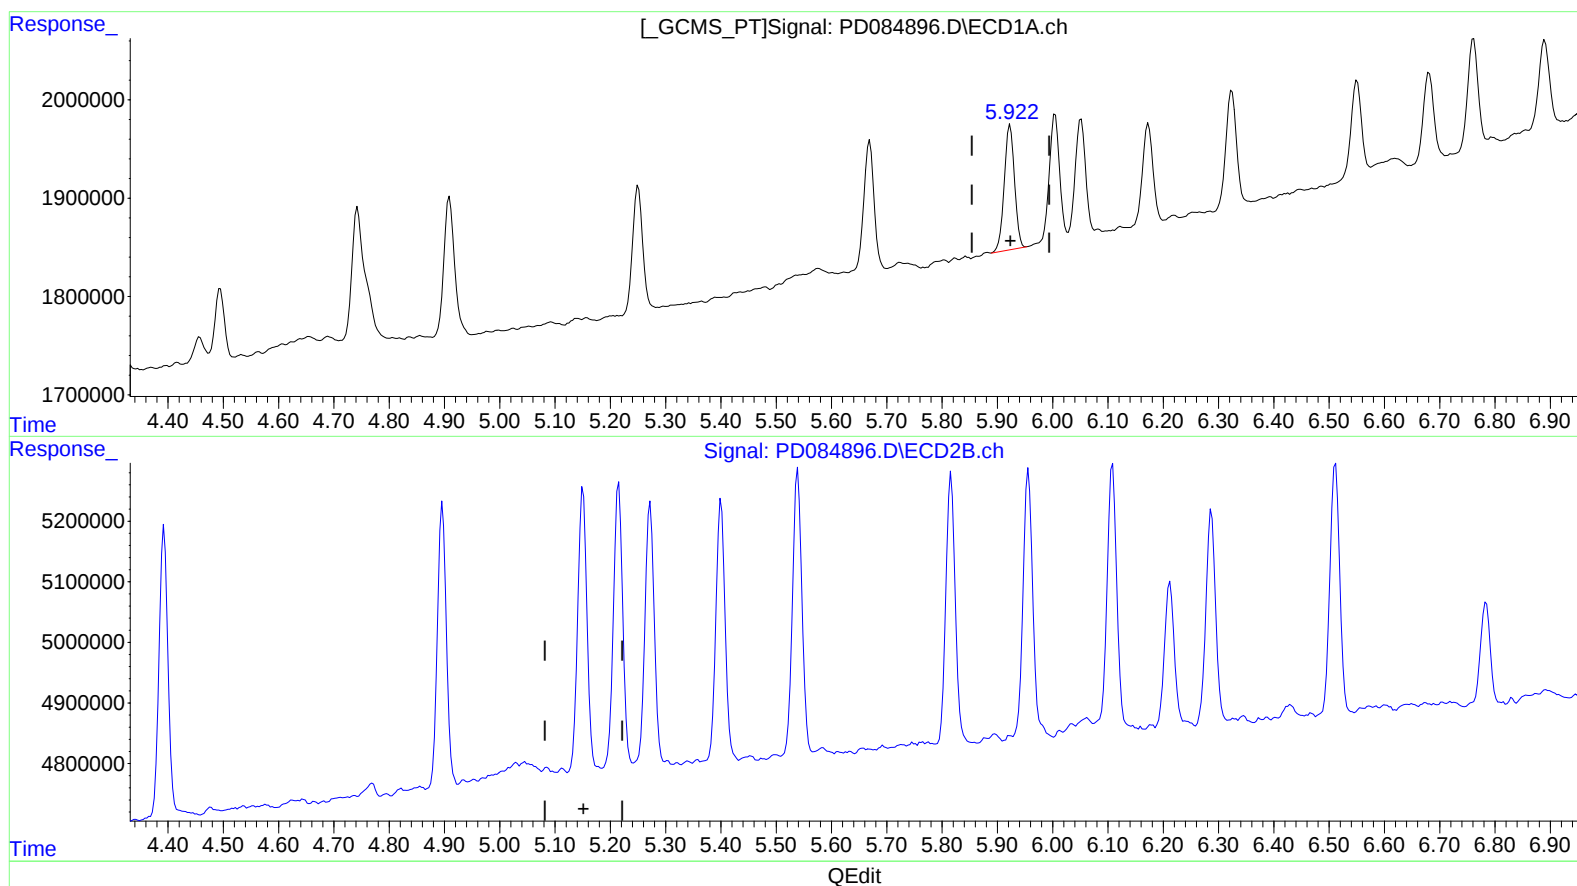

(10) trans-Chlordane (B)

5.923min 1.163 ng/ml

response 1639816

(10) trans-Chlordane #2 (B)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

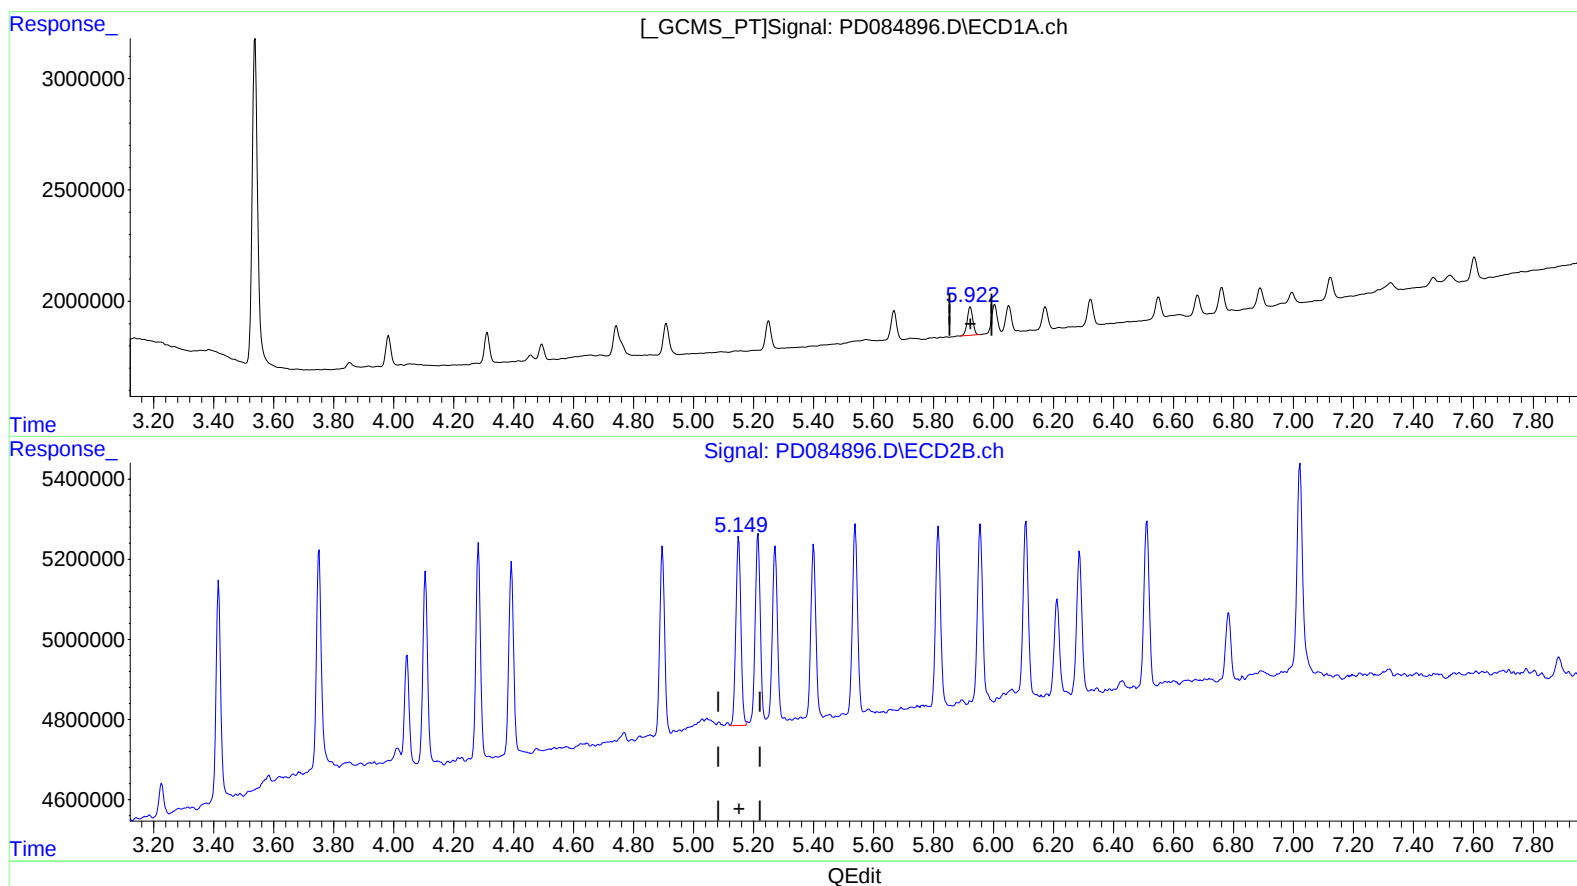

(10) trans-Chlordane (B)

5.923min 1.163 ng/ml  
response 1639816

(10) trans-Chlordane #2 (B)

5.149min 1.343 ng/ml m  
response 5525464

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

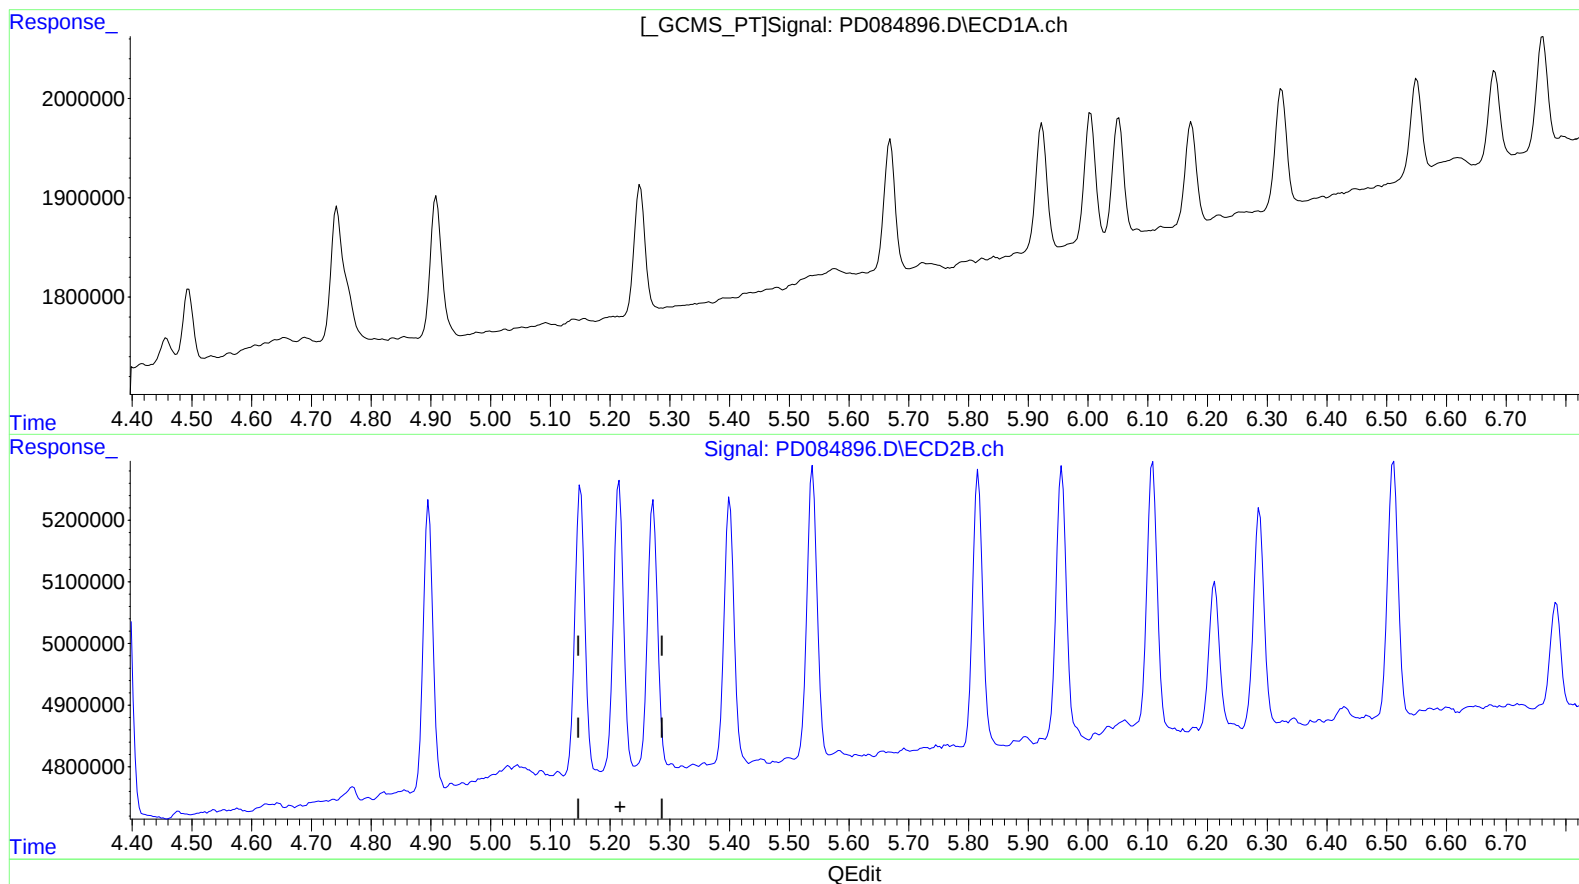

(11) cis-Chlordane (B)

0.000min 0.000 ng/ml

response 0

(11) cis-Chlordane #2 (B)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

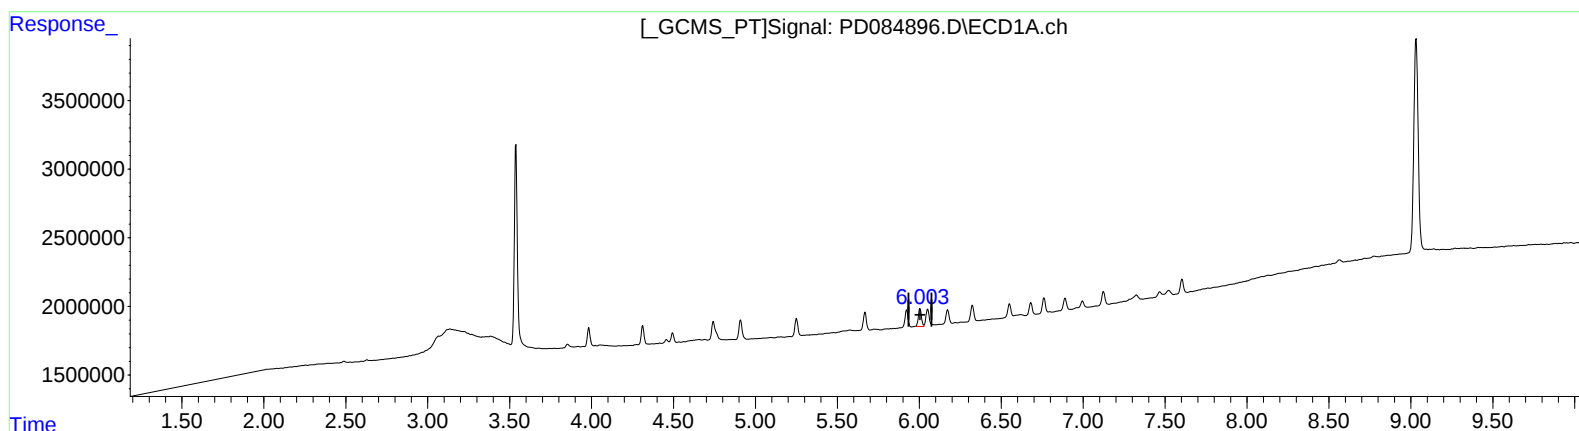

(11) cis-Chlordane (B)

6.003min 1.165 ng/ml m

response 1722573

(11) cis-Chlordane #2 (B)

5.214min 1.323 ng/ml m

response 5549177

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

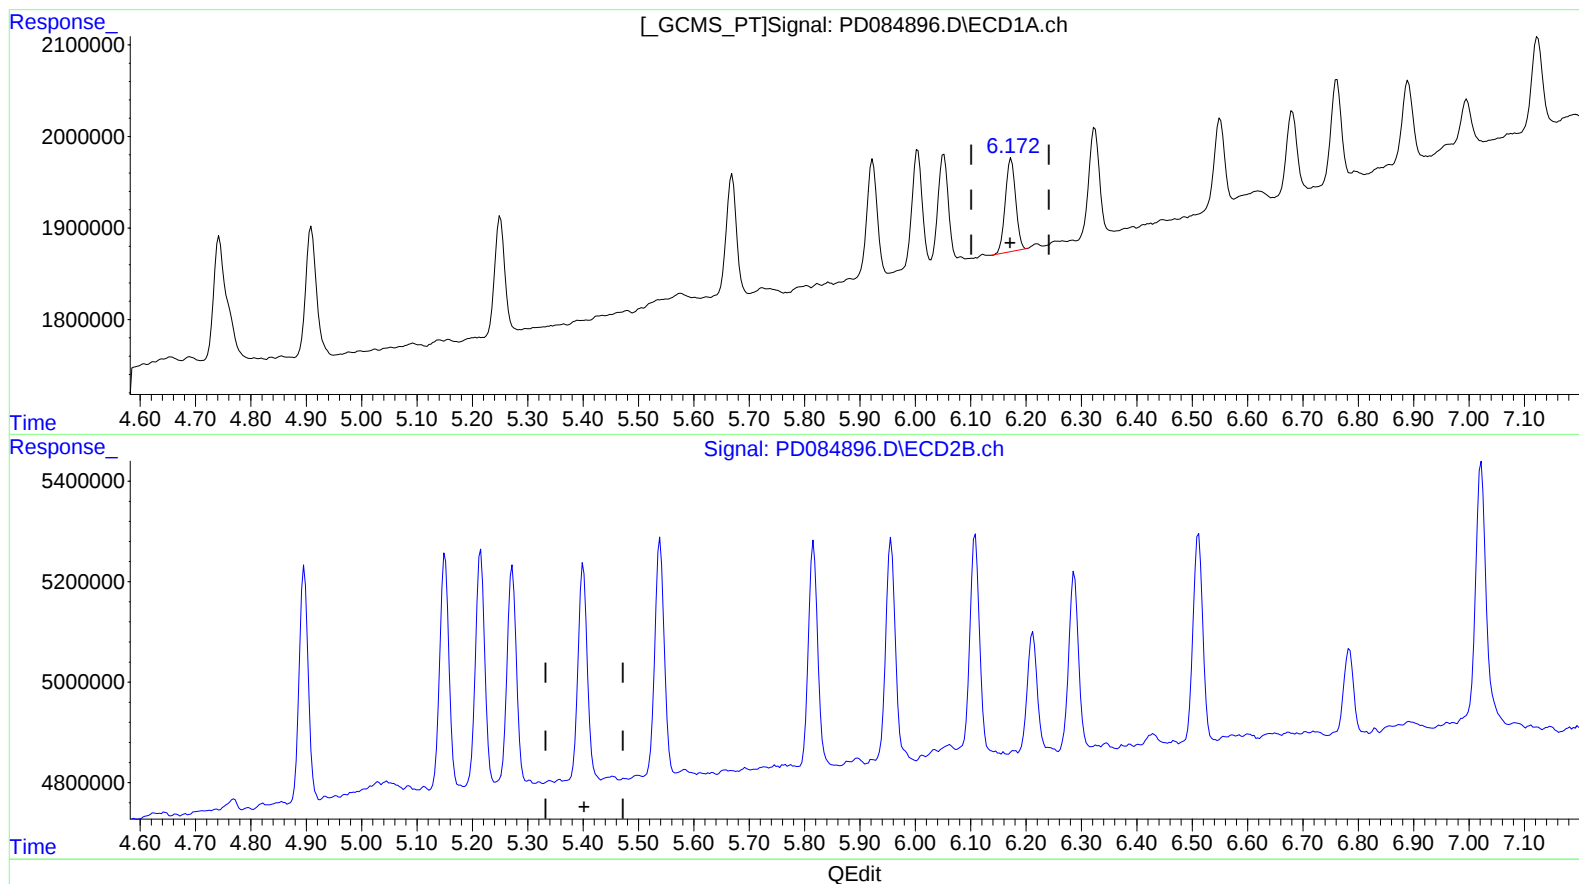

(12) 4,4'-DDE (B)  
6.173min 1.055 ng/ml  
response 1316118

(12) 4,4'-DDE #2 (B)  
0.000min 0.000 ng/ml  
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

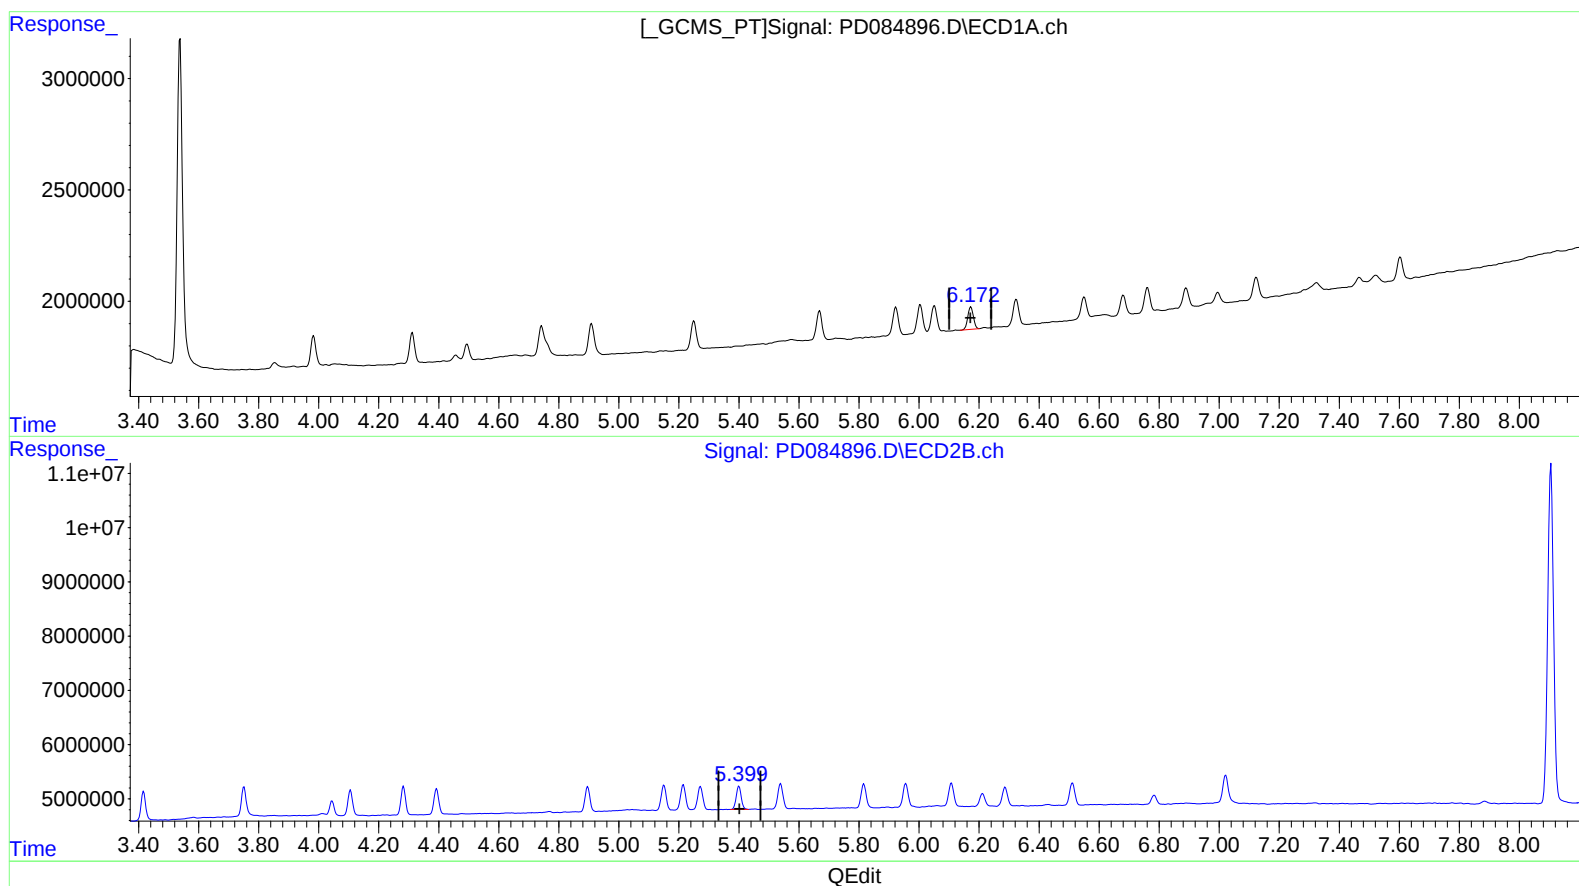

(12) 4,4'-DDE (B)

6.173min 1.055 ng/ml

response 1316118

(12) 4,4'-DDE #2 (B)

5.399min 1.271 ng/ml m

response 4985349

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

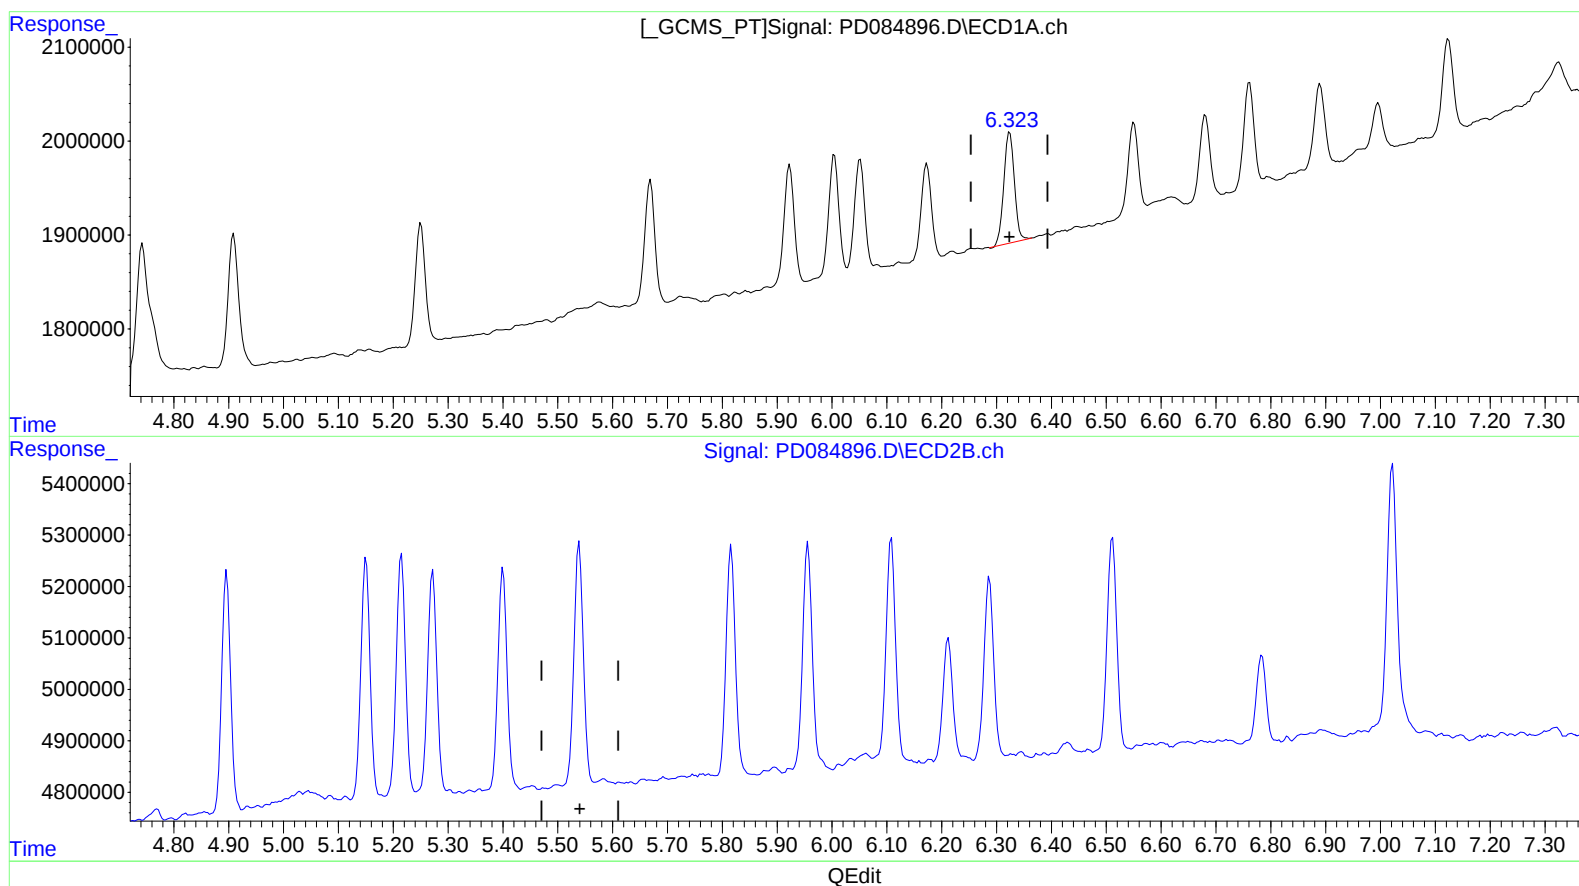

(13) Dieldrin (MA)  
6.324min 1.078 ng/ml  
response 1590204

(13) Dieldrin #2 (MA)  
0.000min 0.000 ng/ml  
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

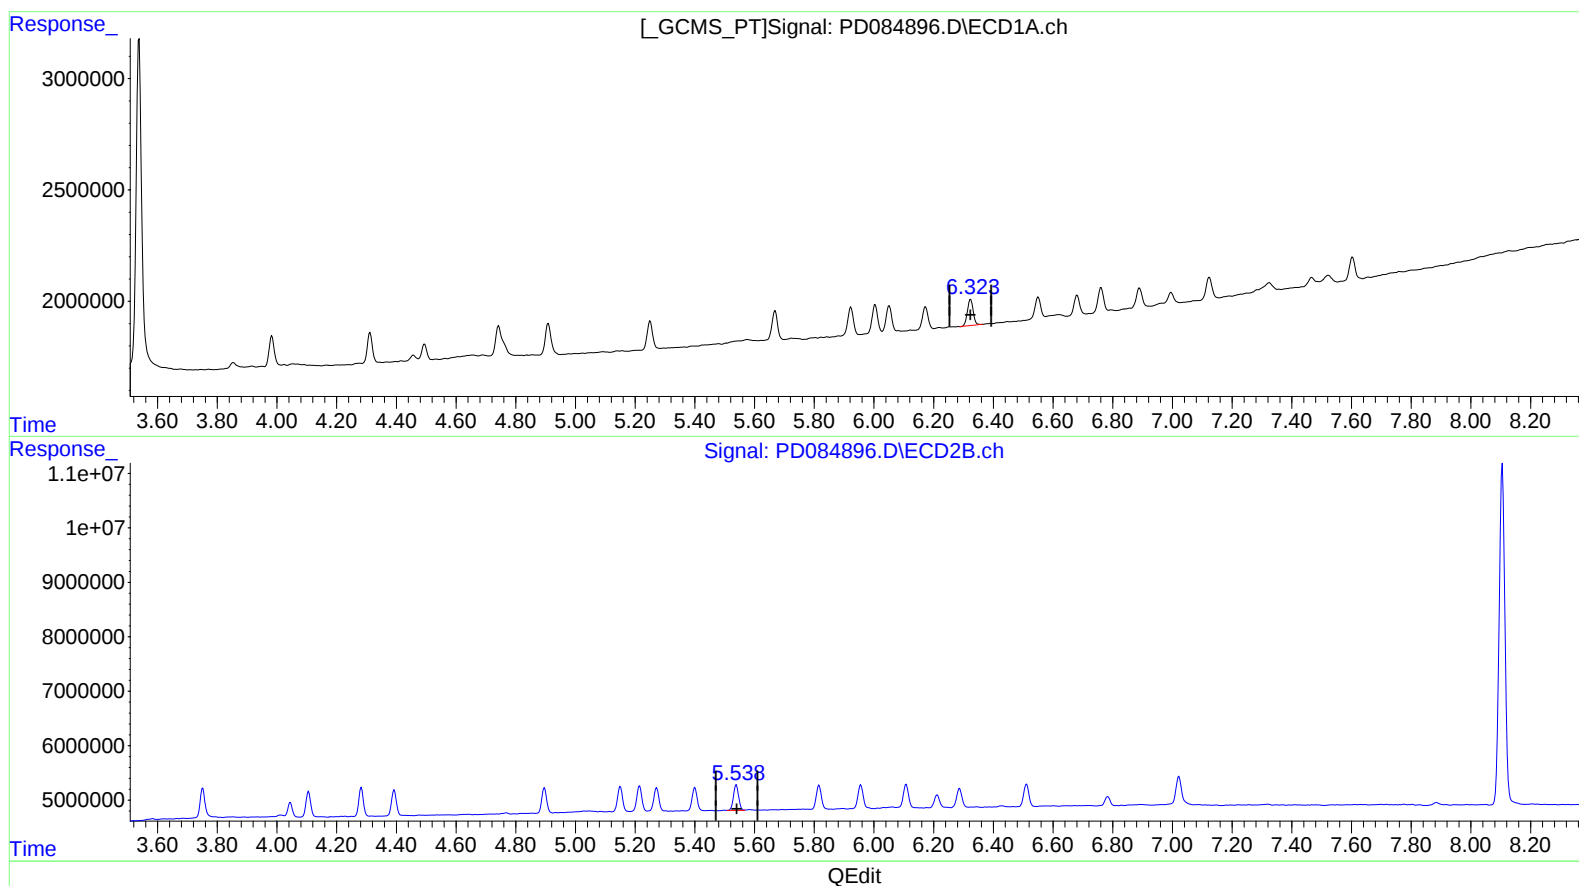

(13) Dieldrin (MA)

6.324min 1.078 ng/ml  
response 1590204

(13) Dieldrin #2 (MA)

5.538min 1.321 ng/ml m  
response 5676034

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

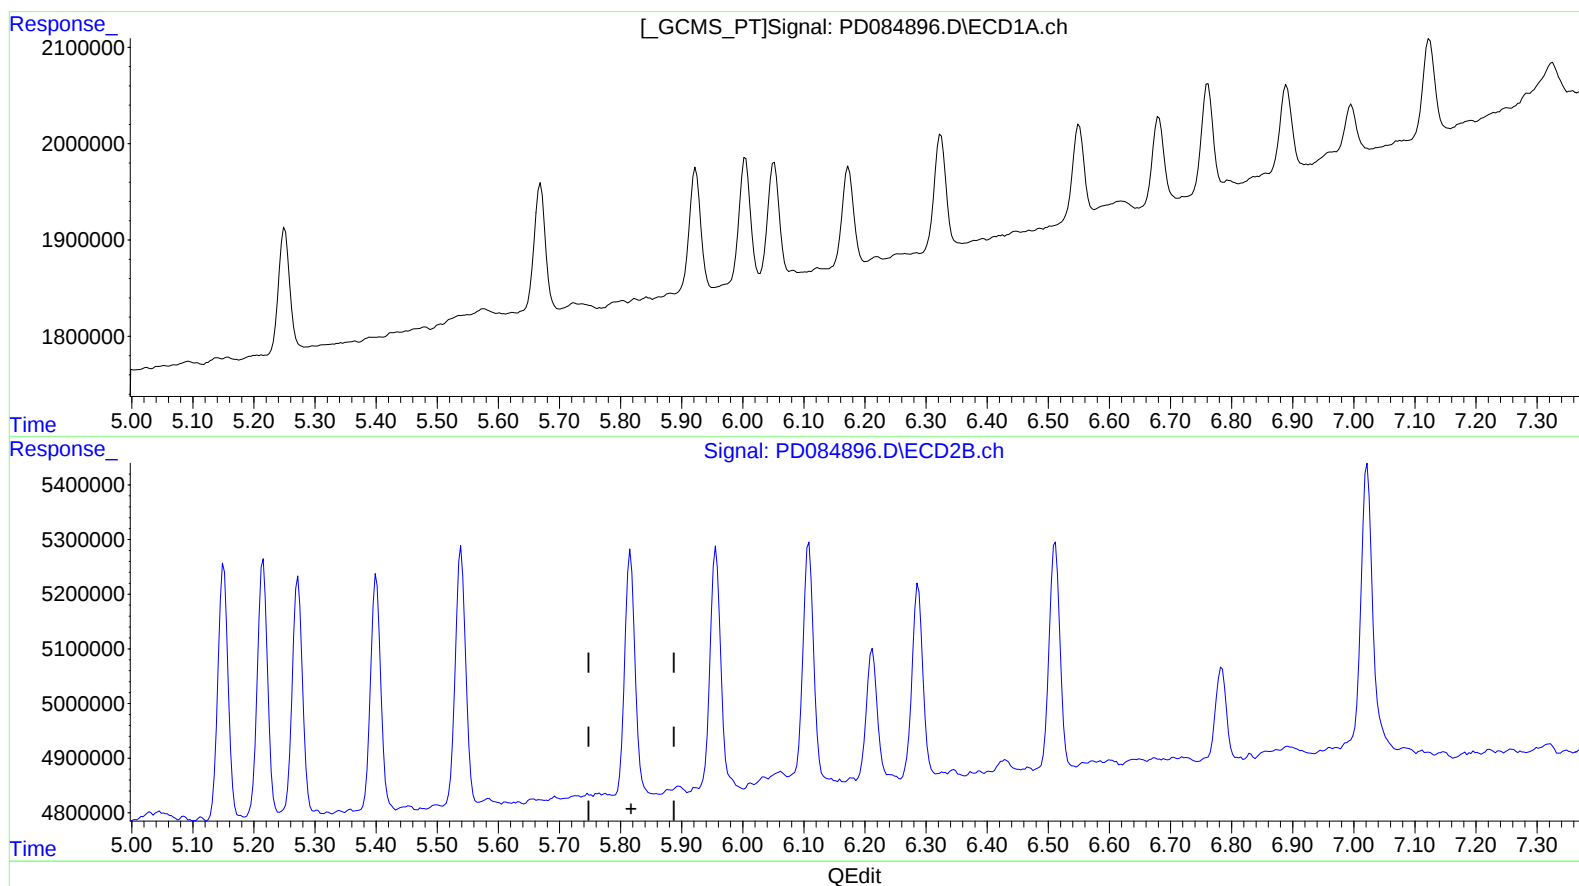

(14) Endrin (MA)

0.000min 0.000 ng/ml  
response 0

(14) Endrin #2 (MA)

0.000min 0.000 ng/ml  
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

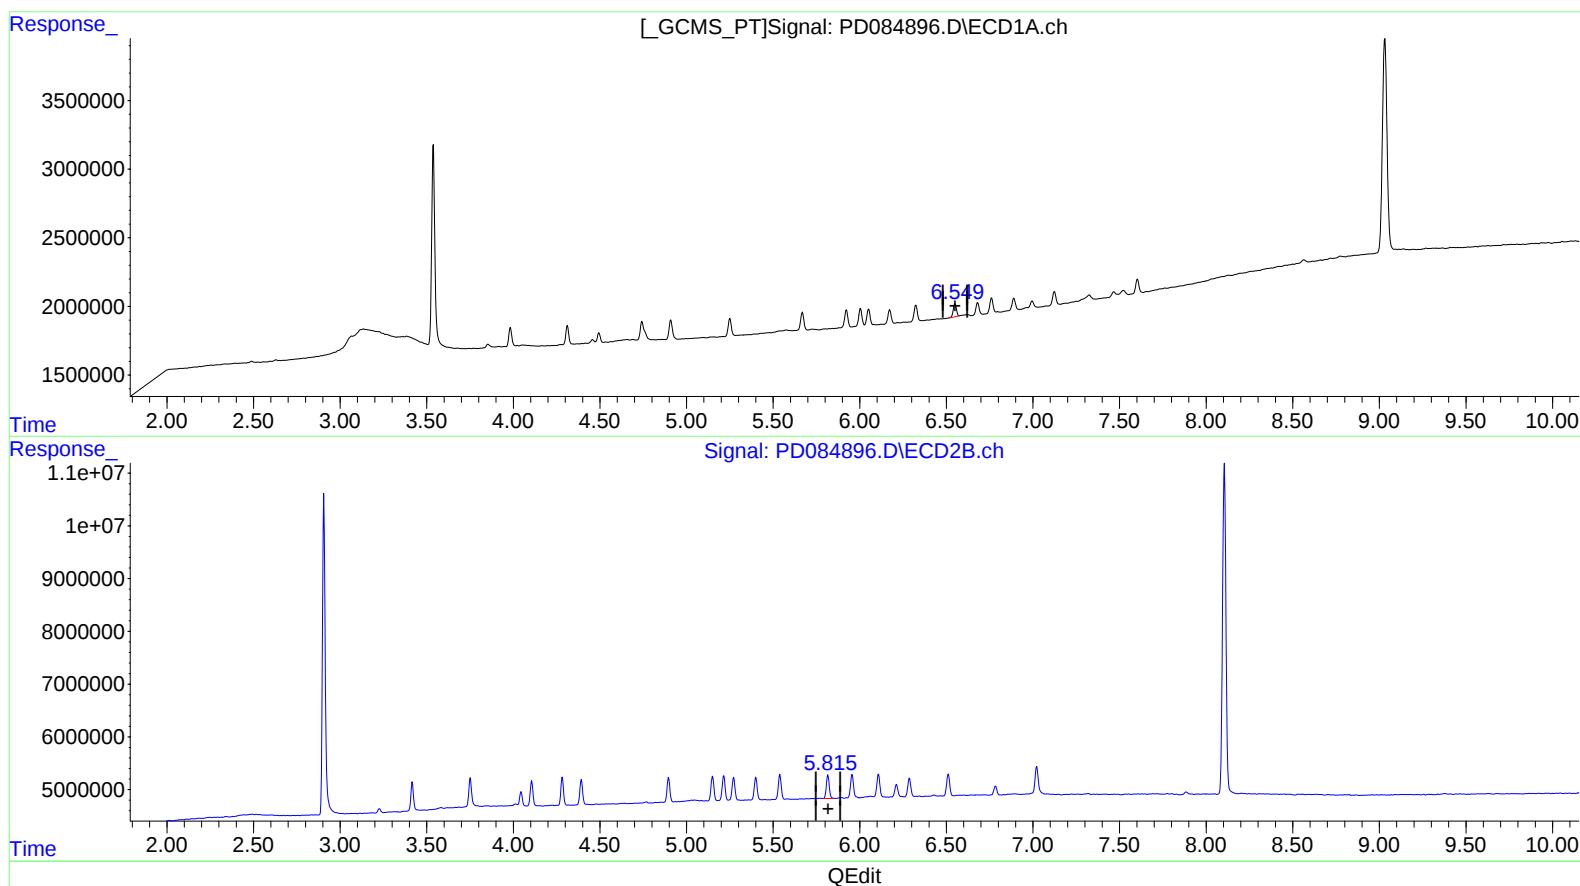

(14) Endrin (MA)

6.549min 1.089 ng/ml m  
response 1228352

(14) Endrin #2 (MA)

5.815min 1.414 ng/ml m  
response 5234427

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

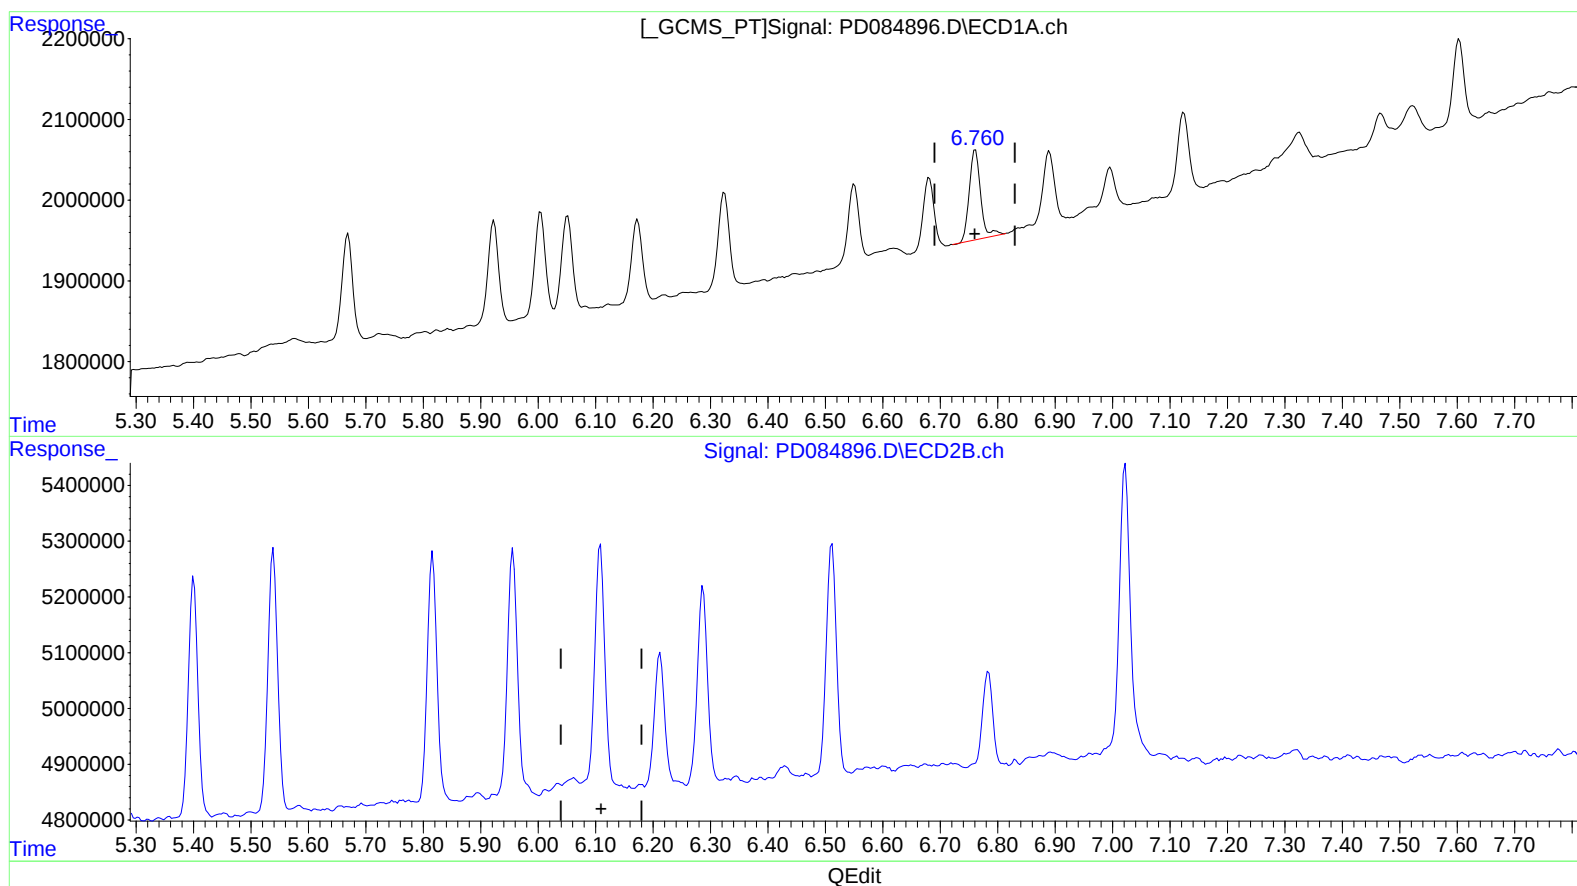

(15) Endosulfan II (B)  
6.761min 1.153 ng/ml  
response 1521783

(15) Endosulfan II #2 (B)  
0.000min 0.000 ng/ml  
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED



Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

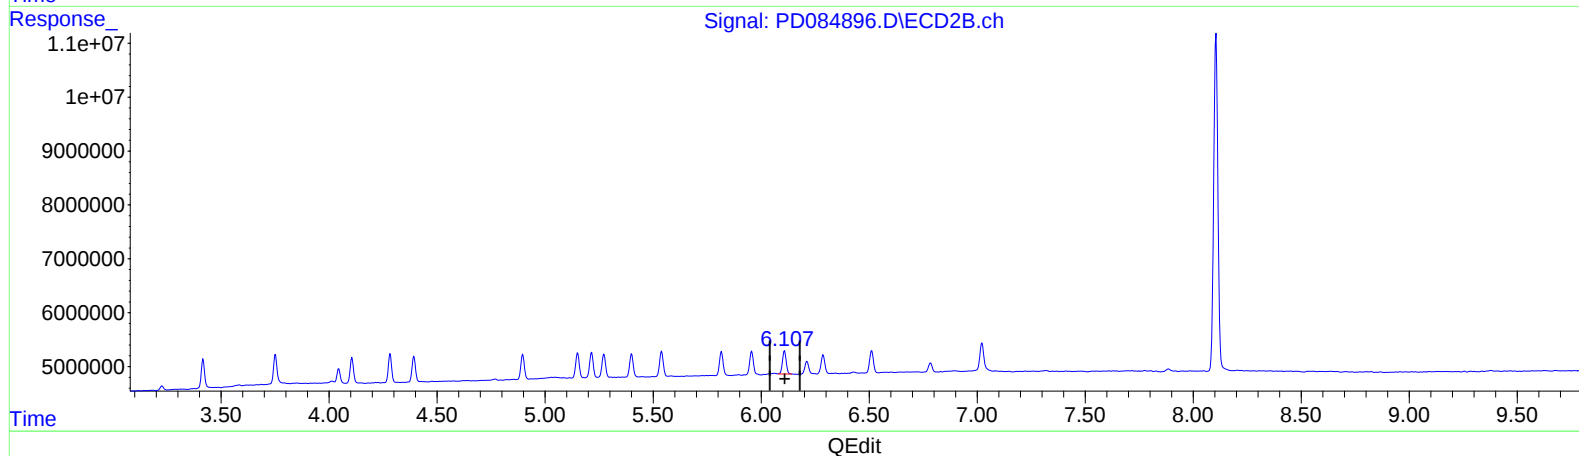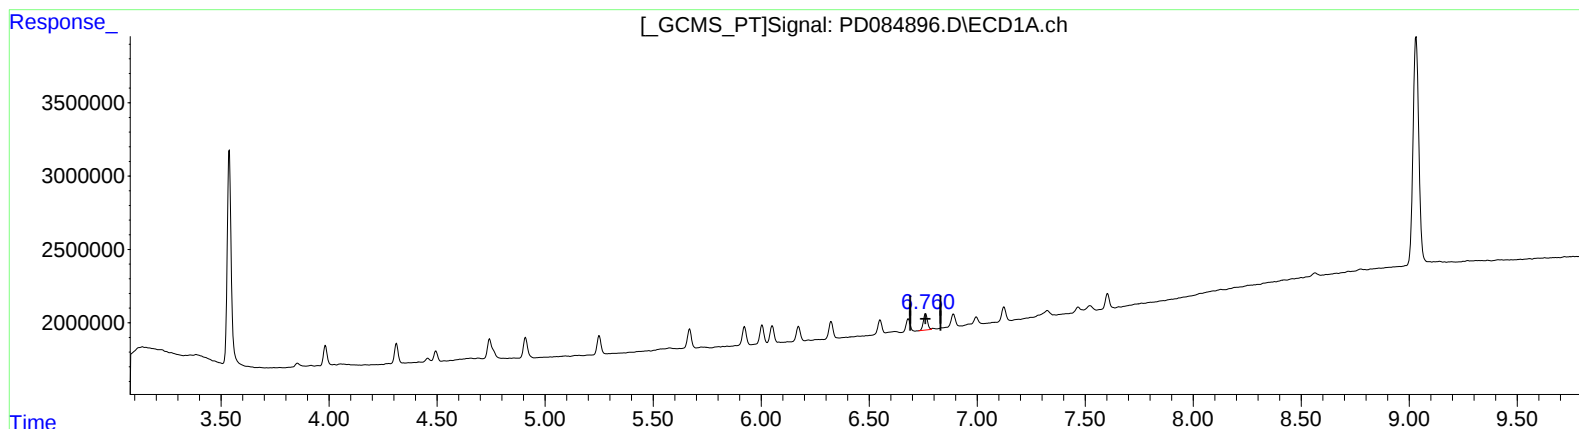

(15) Endosulfan II (B)  
6.760min 1.116 ng/ml m  
response 1472910

(15) Endosulfan II #2 (B)  
6.107min 1.405 ng/ml m  
response 5209860

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

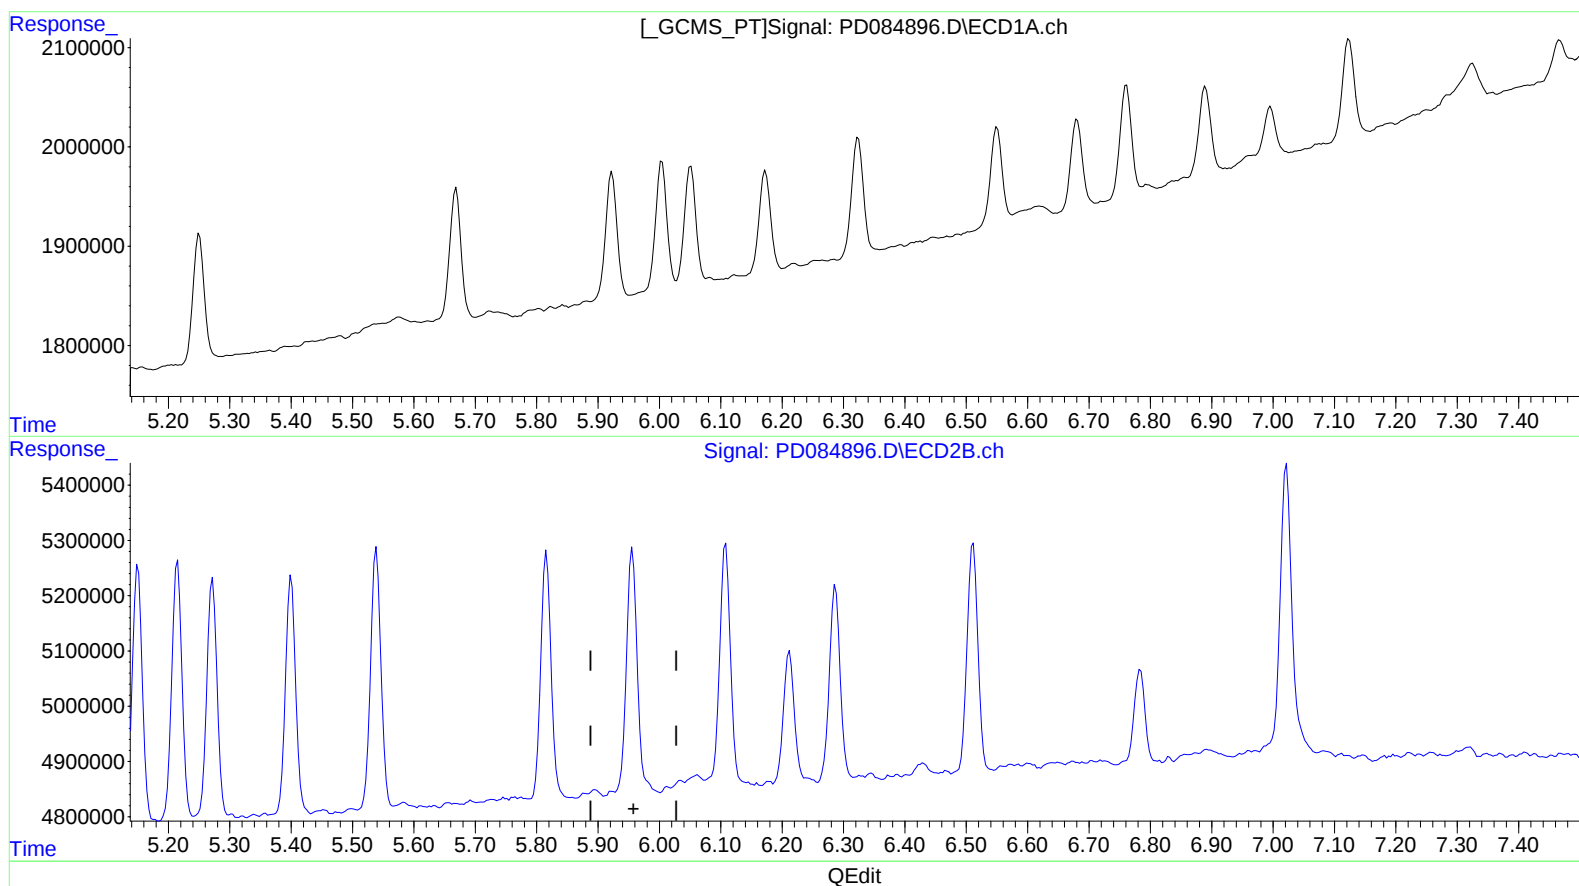

(16) 4,4'-DDD (A)

0.000min 0.000 ng/ml  
response 0

(16) 4,4'-DDD #2 (A)

0.000min 0.000 ng/ml  
response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

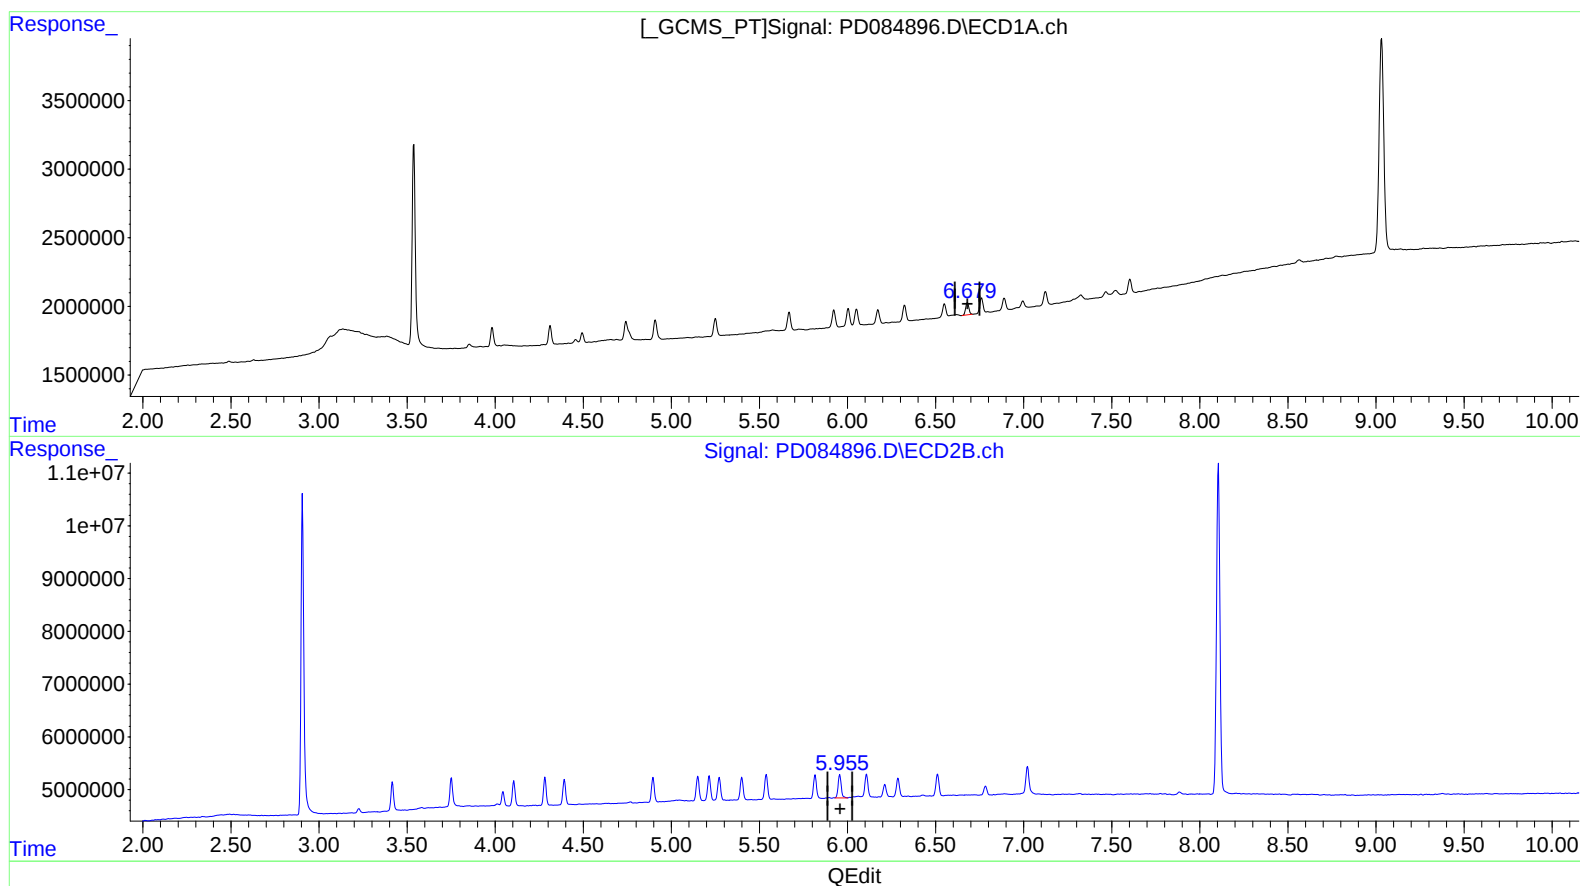

(16) 4,4'-DDD (A)

6.679min 1.185 ng/ml m  
response 1170326

(16) 4,4'-DDD #2 (A)

5.955min 1.598 ng/ml m  
response 5424349

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED



Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

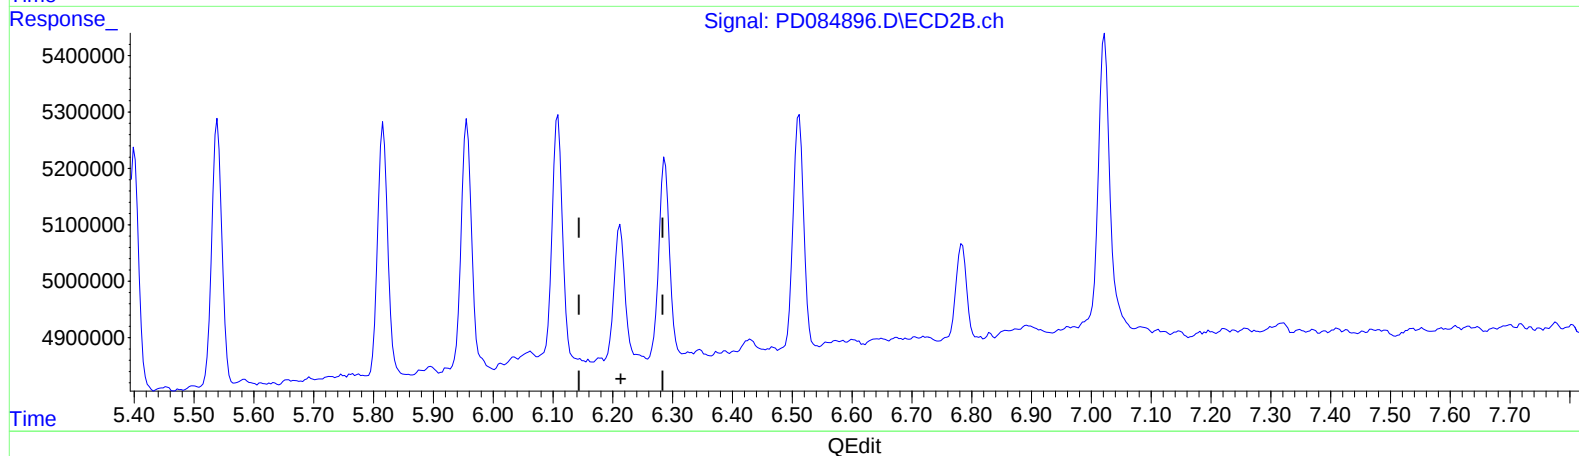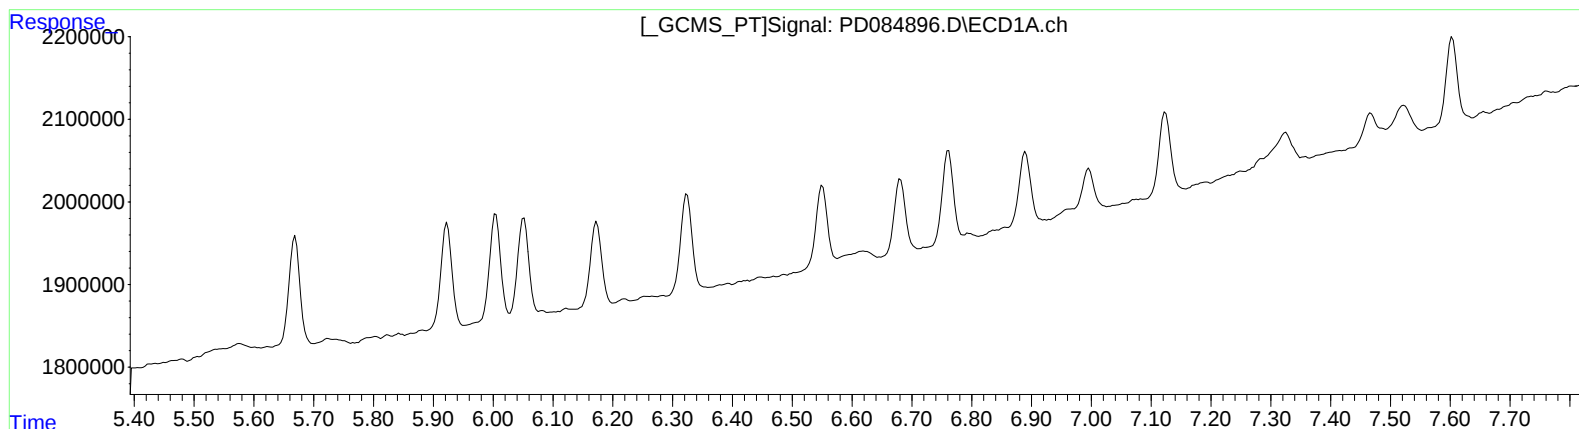

(17) 4,4'-DDT (MA)

0.000min 0.000 ng/ml

response 0

(17) 4,4'-DDT #2 (MA)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED



Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

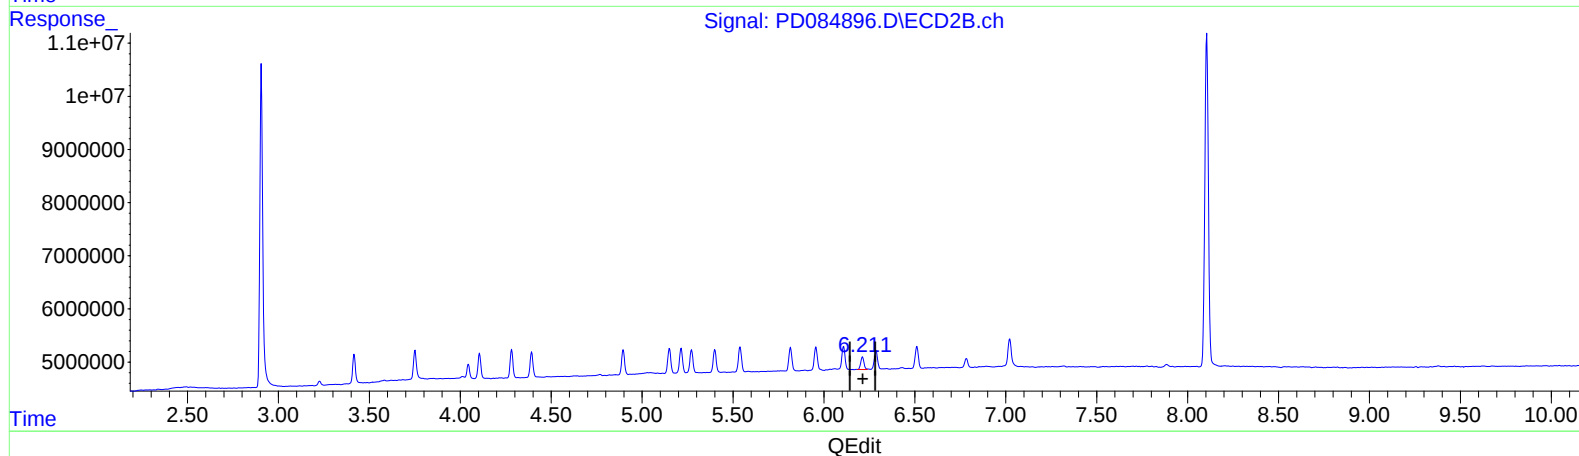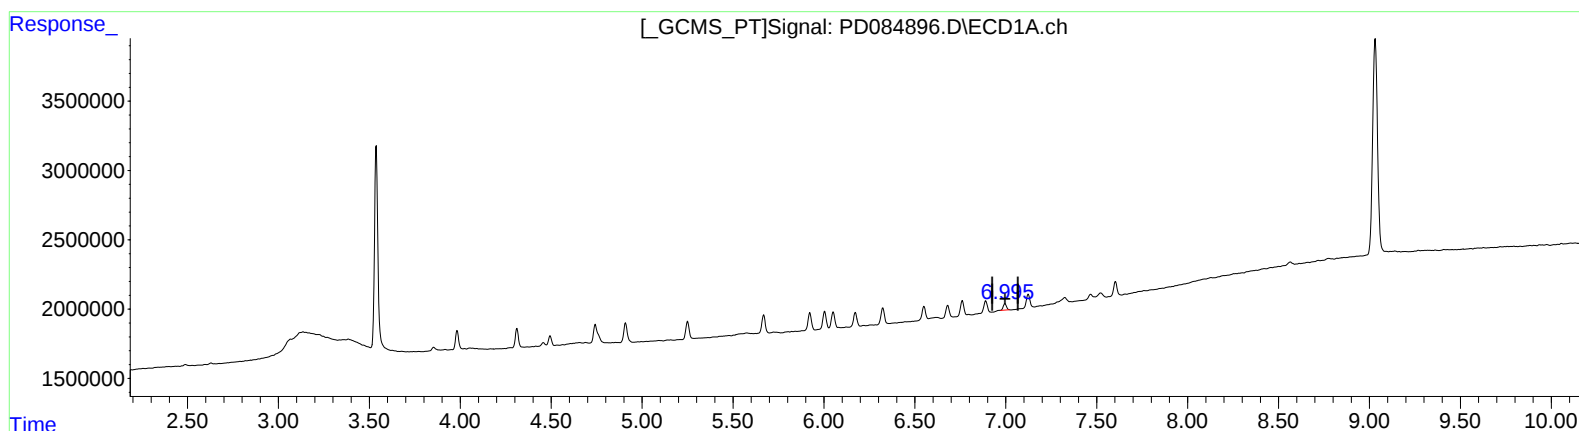

(17) 4,4'-DDT (MA)  
6.995min 0.649 ng/ml m  
response 581225

(17) 4,4'-DDT #2 (MA)  
6.211min 0.942 ng/ml m  
response 3013045

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

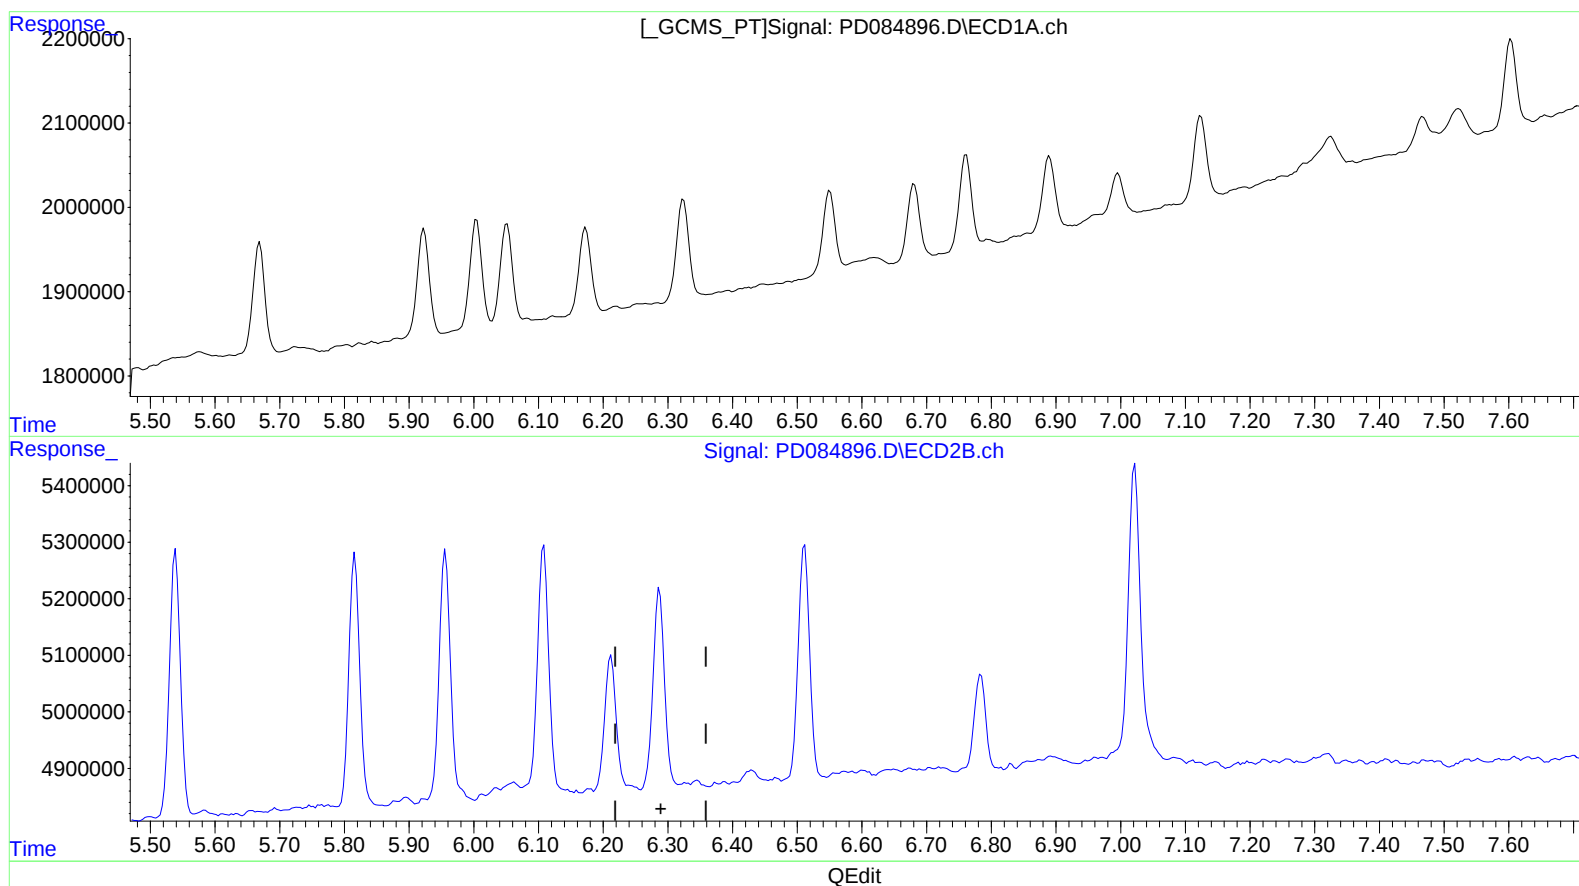

(18) Endrin aldehyde (B)

0.000min 0.000 ng/ml

response 0

(18) Endrin aldehyde #2 (B)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED



Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

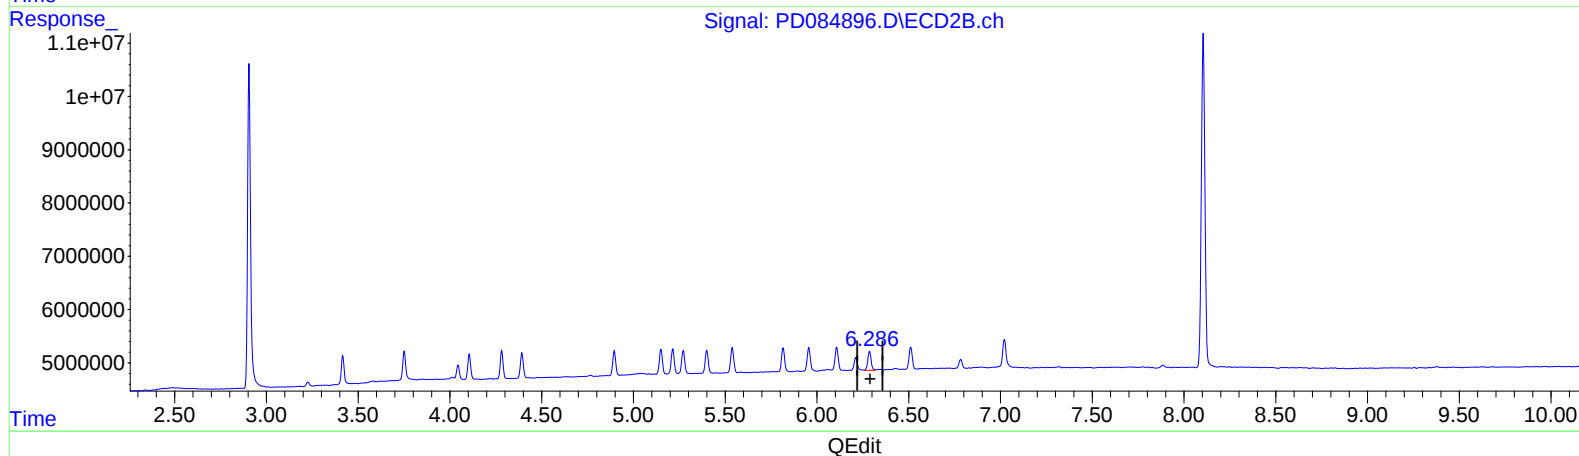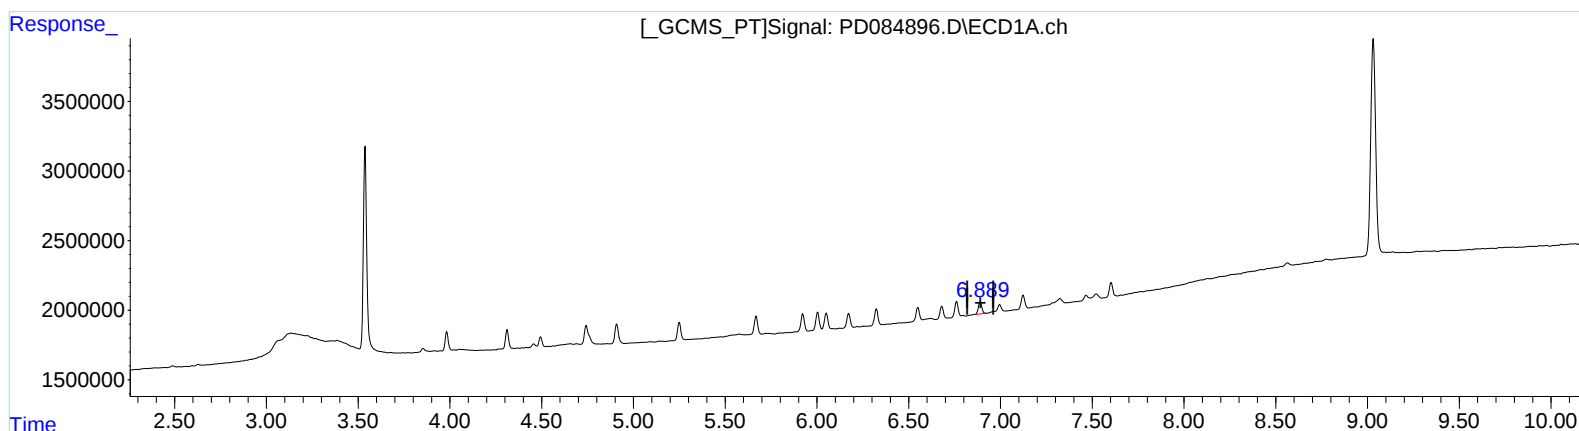

(18) Endrin aldehyde (B)

6.889min 1.289 ng/ml m  
response 1164046

(18) Endrin aldehyde #2 (B)

6.286min 1.568 ng/ml m  
response 4476635

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

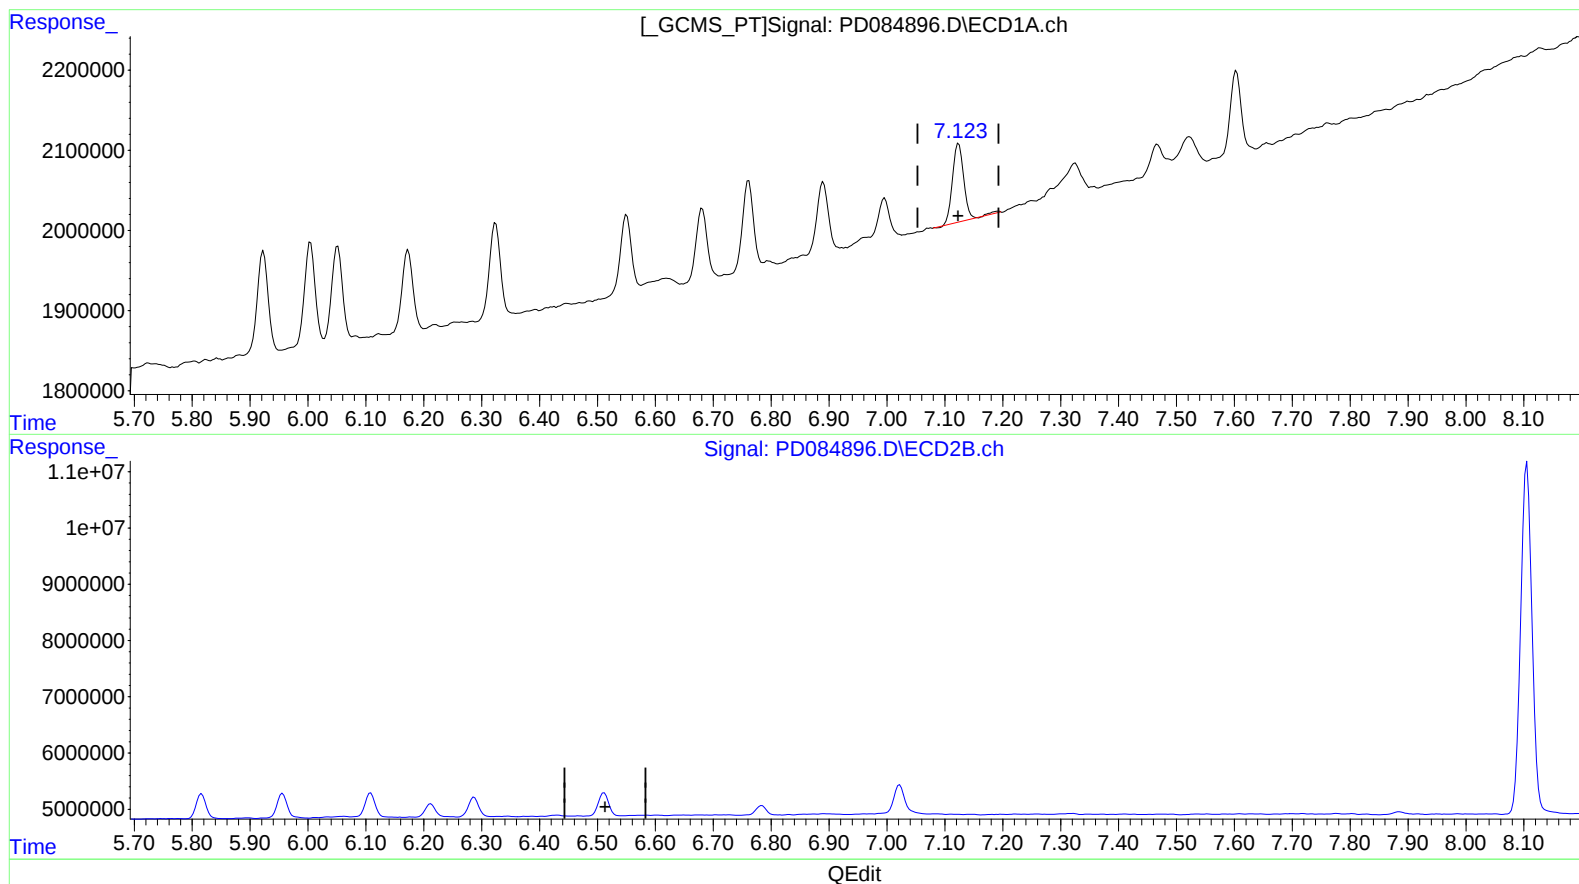

(19) Endosulfan Sulfate (B)

7.124min 1.188 ng/ml

response 1368096

(19) Endosulfan Sulfate #2 (B)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED



Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

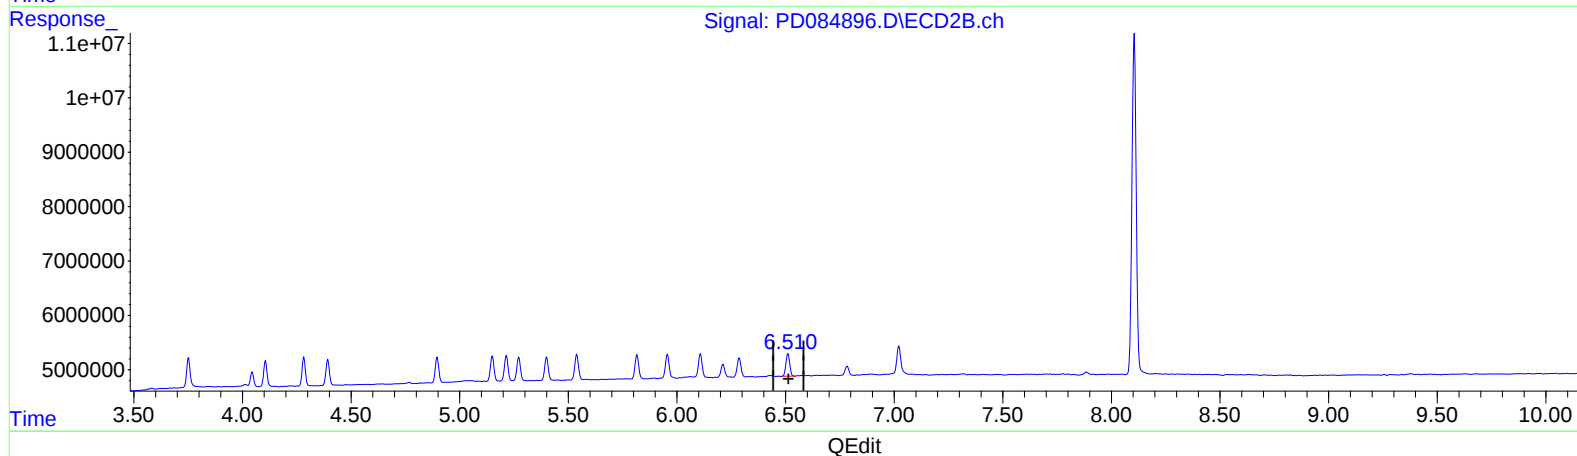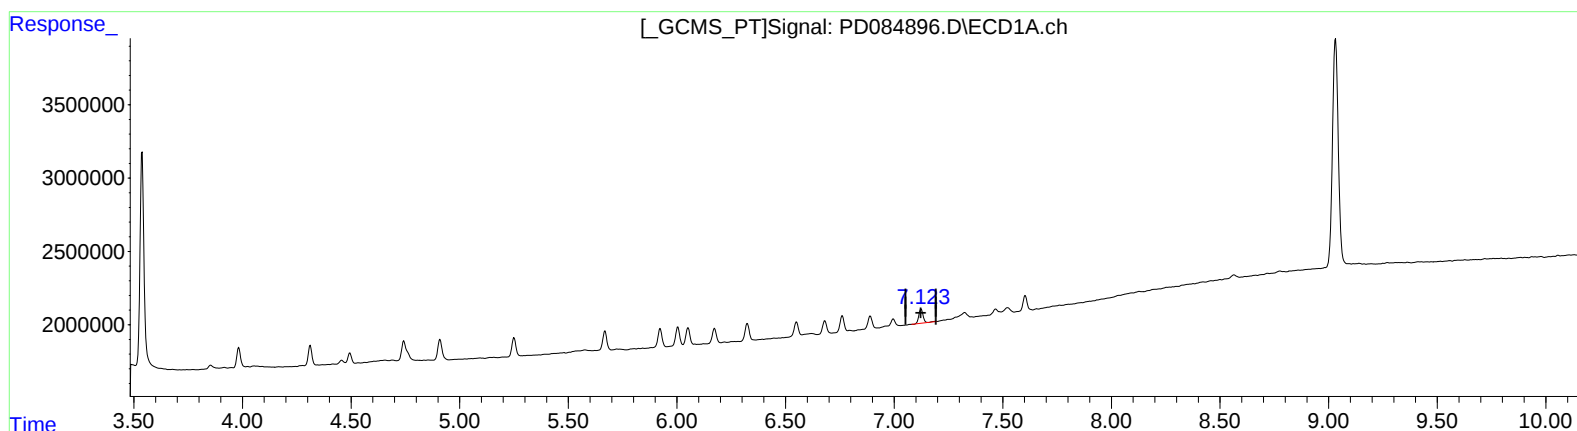

(19) Endosulfan Sulfate (B)

7.124min 1.188 ng/ml

response 1368096

(19) Endosulfan Sulfate #2 (B)

6.510min 1.419 ng/ml m

response 5066617

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED


Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

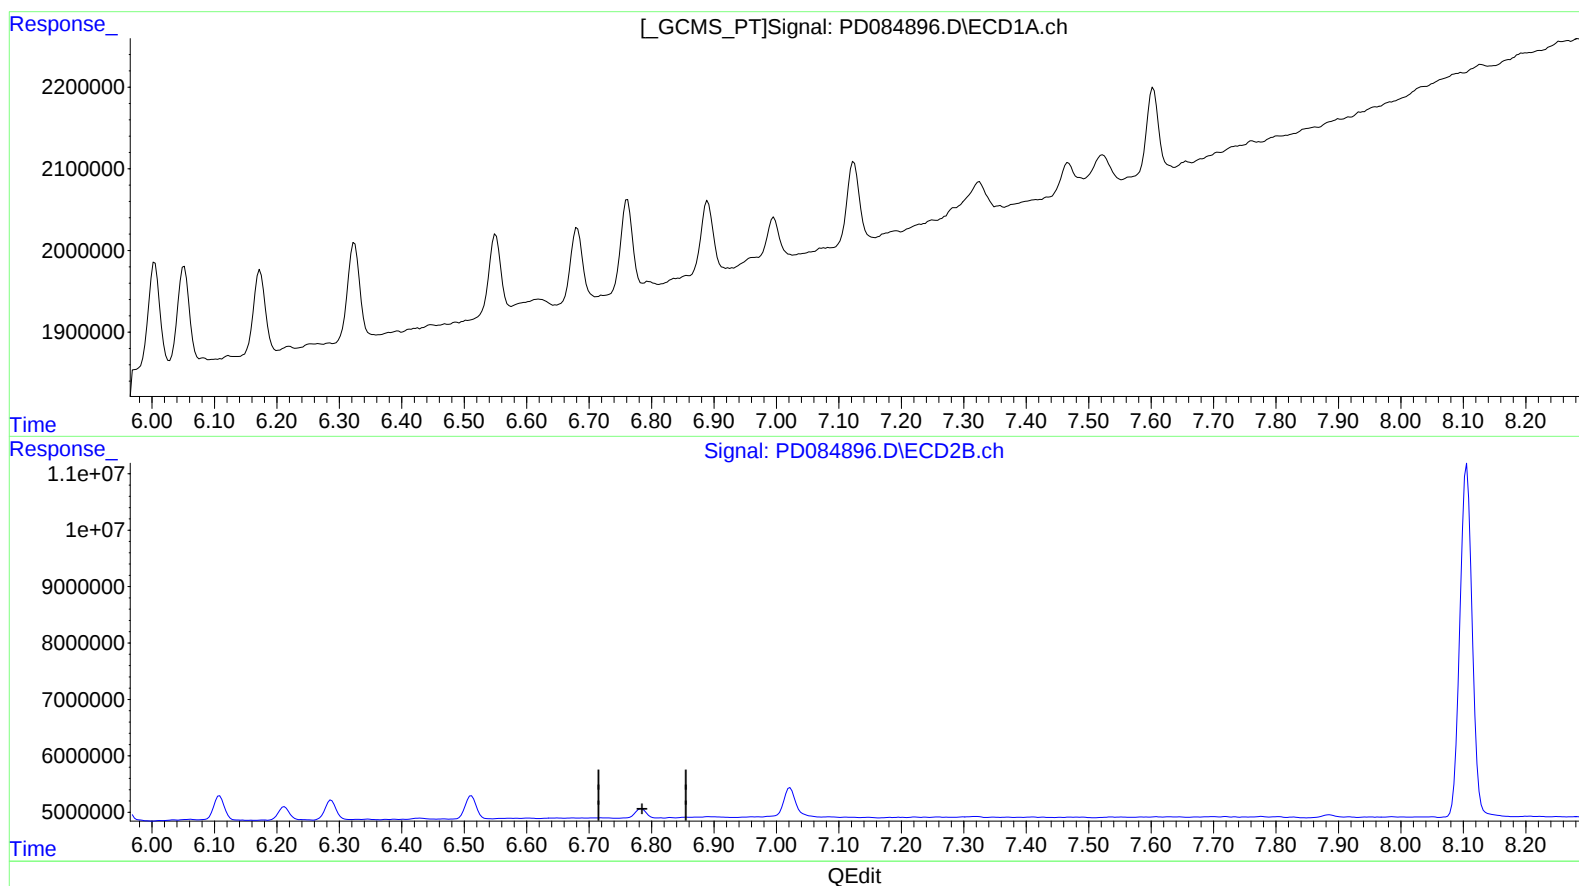

(20) Methoxychlor (A)

0.000min 0.000 ng/ml

response 0

(20) Methoxychlor #2 (A)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED



Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

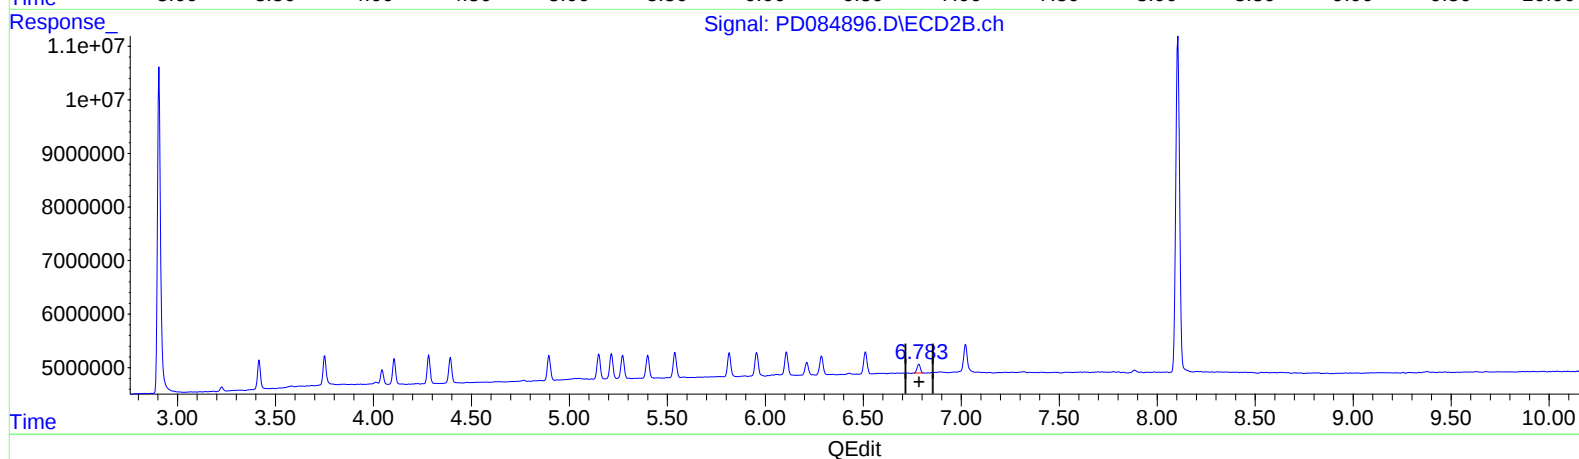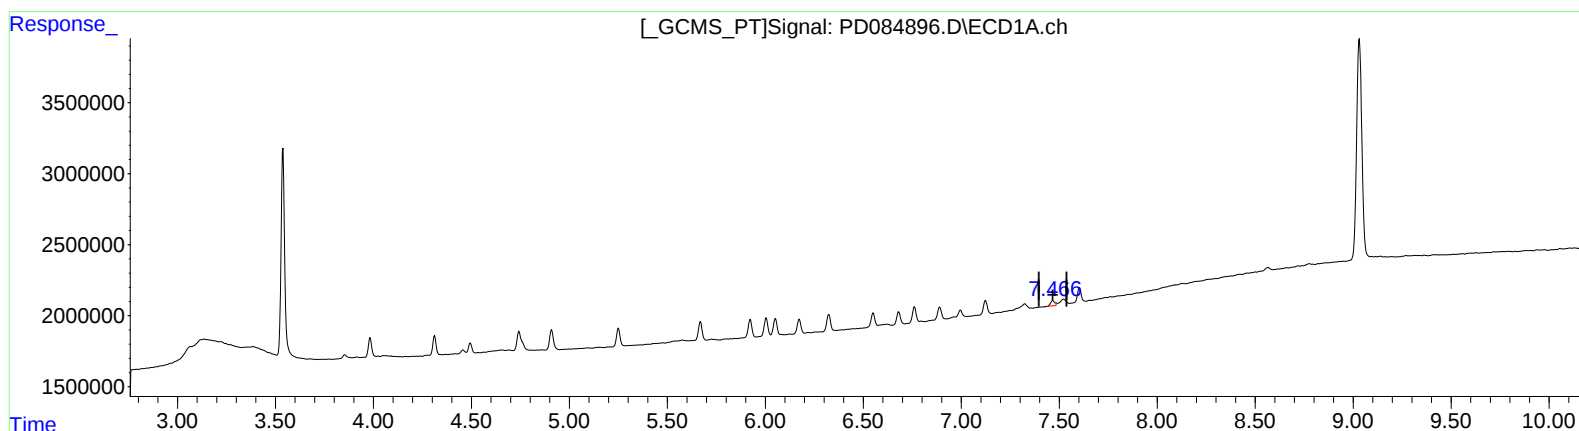

(20) Methoxychlor (A)  
7.466min 1.036 ng/ml m  
response 539681

(20) Methoxychlor #2 (A)  
6.783min 1.177 ng/ml m  
response 1946540

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED



Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

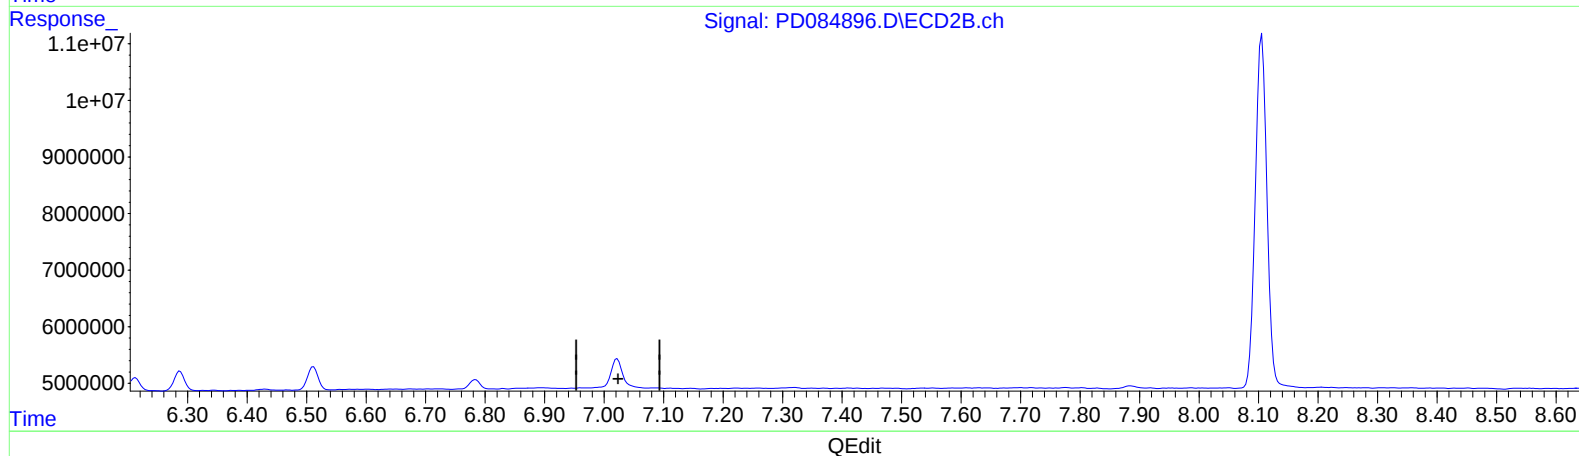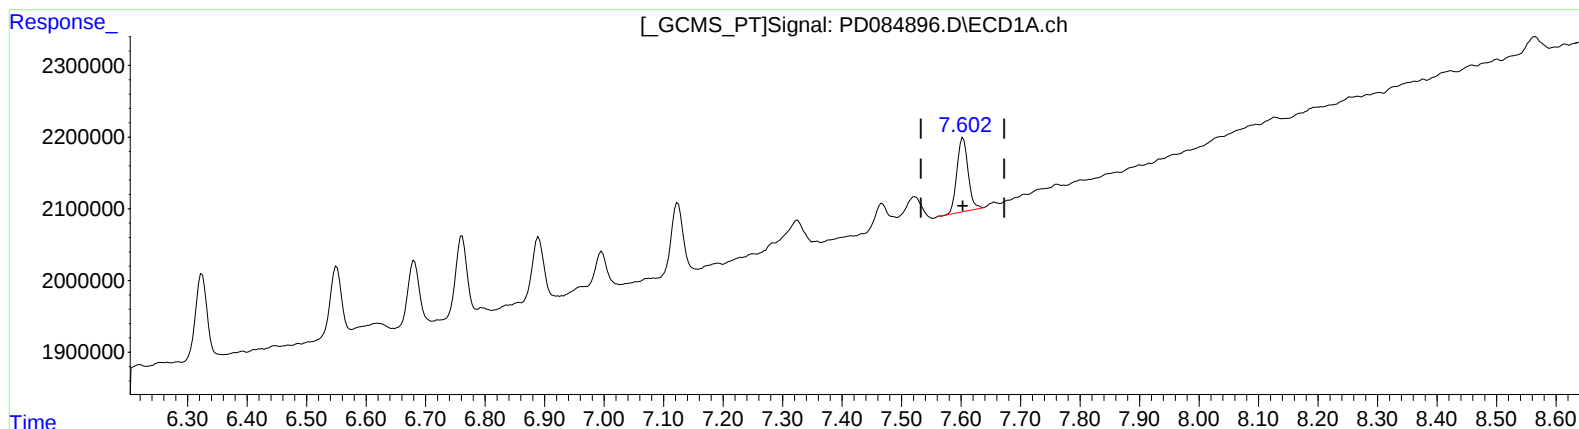

(21) Endrin ketone (B)

7.604min 1.114 ng/ml

response 1361872

(21) Endrin ketone #2 (B)

0.000min 0.000 ng/ml

response 0

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD090424\  
Data File : PD084896.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Sep 2024 10:51  
Operator : AR\AJ  
Sample : P3391-01  
Misc : PEST MDL WATER IPPB  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
MDL-WATER-QT3-2024-05

## Manual IntegrationsAPPROVED



Reviewed By :Abdul  
Mirza

09/05/2024  
Supervised By :Ankita  
Jodhani

09/06/2024

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 05 02:16:10 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD082524CLP.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 27 02:47:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

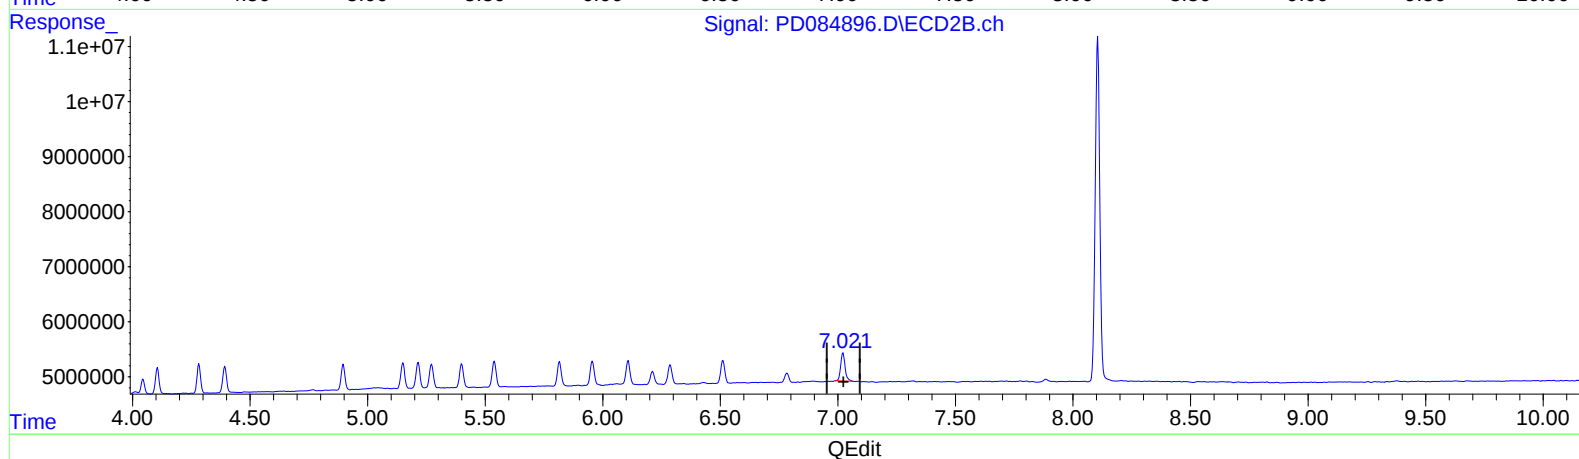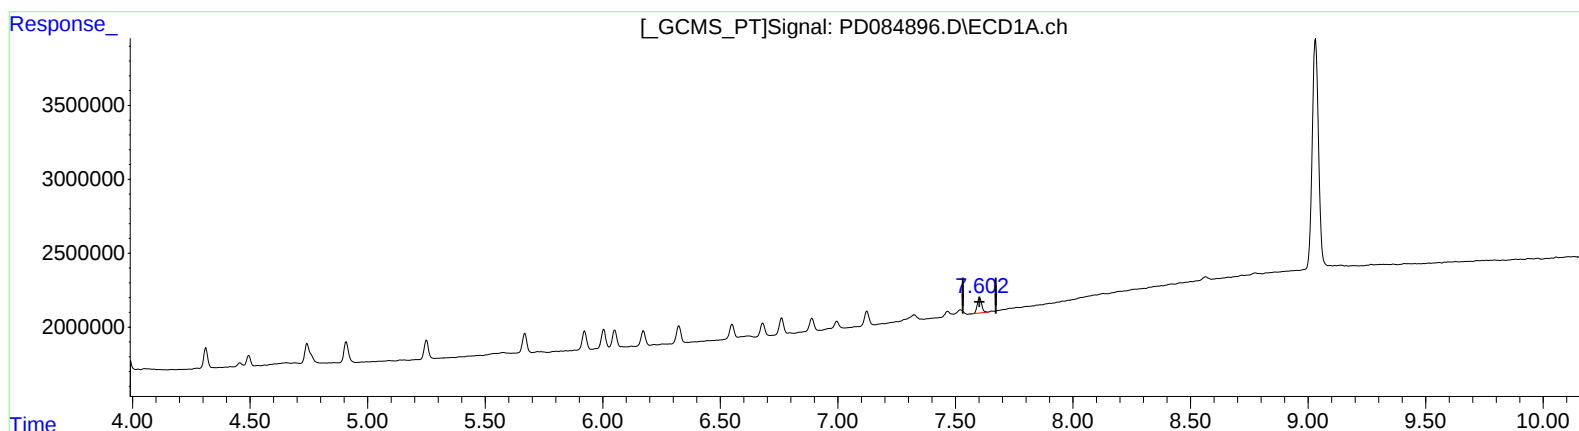

(21) Endrin ketone (B)

7.604min 1.114 ng/ml

response 1361872

(21) Endrin ketone #2 (B)

7.021min 1.523 ng/ml m

response 6706900