

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090518\
 Data File : PD049097.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Sep 2018 12:25
 Operator : AJ\SJ
 Sample : PIBLK18
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK18

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 02:00:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081618CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 16 13:32:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.369	3.967	23783372	357.9E6	19.486	20.358
27) SA Decachlor...	8.064	8.991	57613526	655.5E6	40.012	40.493
Target Compounds						
10) B trans-Chl...	0.000	6.008f	0	5870701	N.D.	0.253


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090518\
Data File : PD049097.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Sep 2018 12:25
Operator : AJ\SJ
Sample : PIBLK18
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK18

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 02:00:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081618CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 16 13:32:25 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

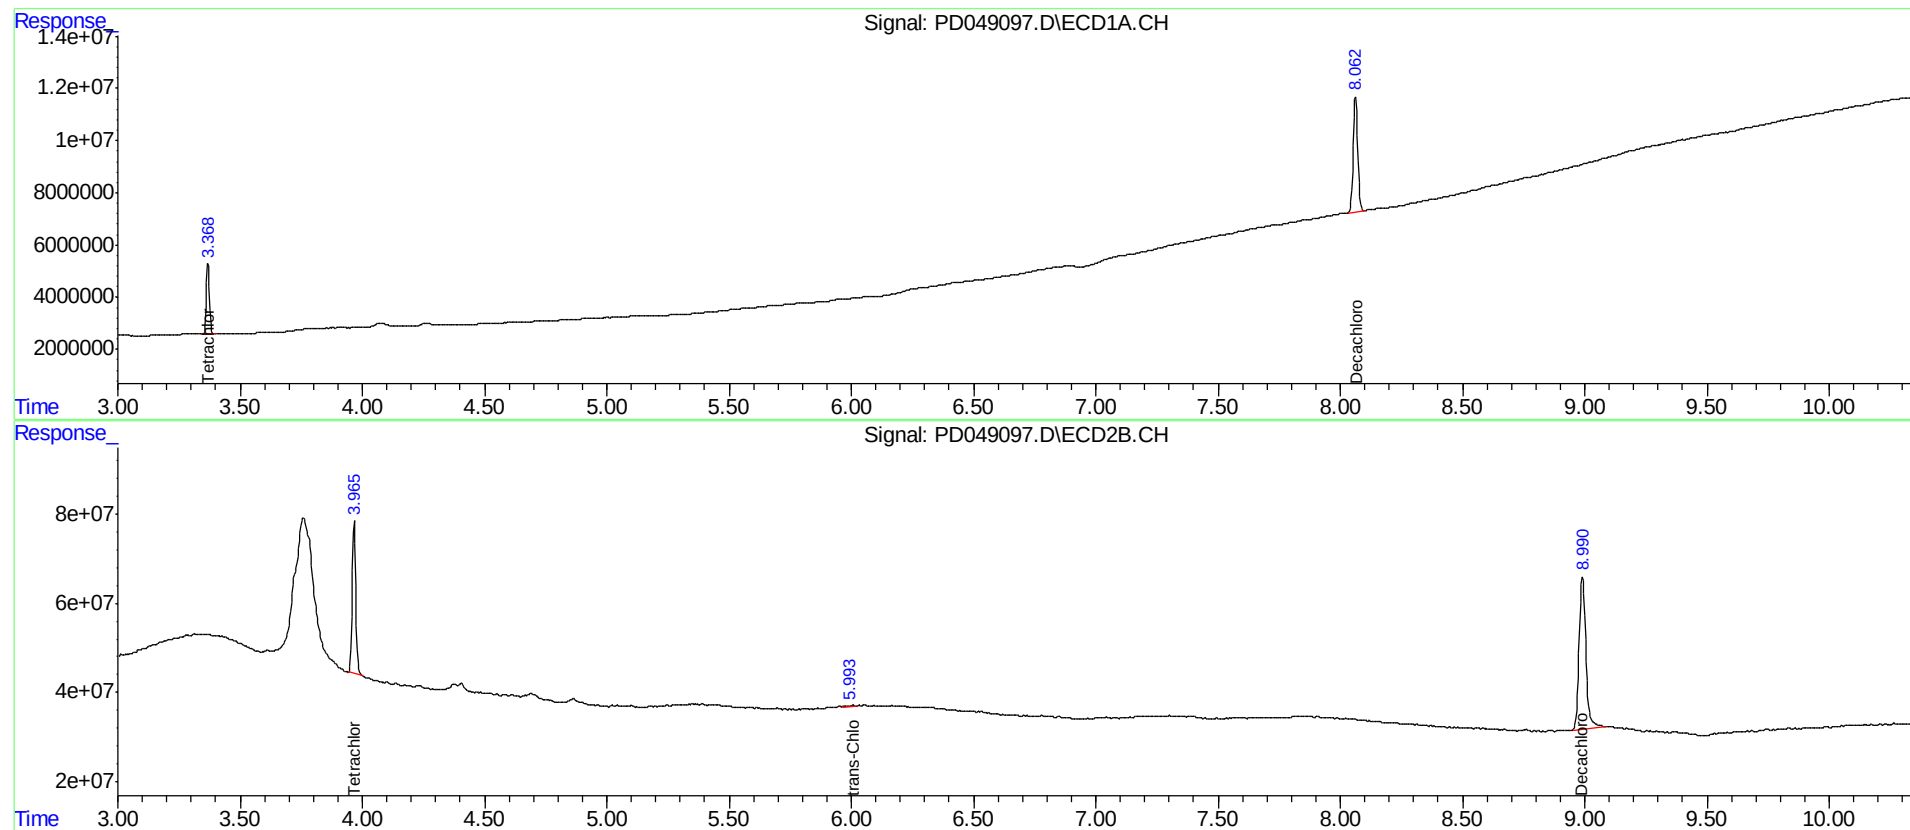


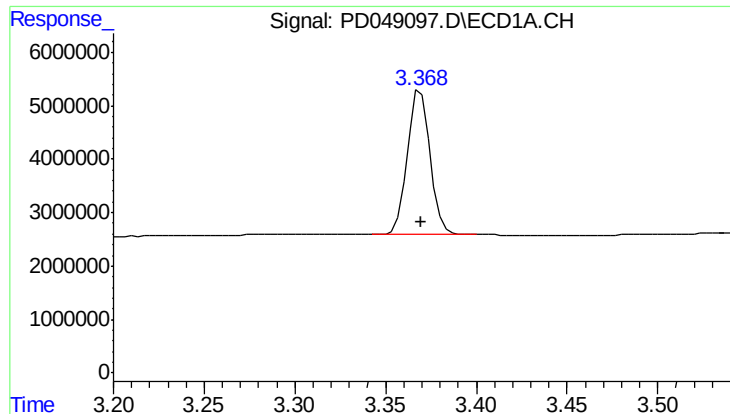

#1 Tetrachloro-m-xylene


R.T.: 3.369 min
Delta R.T.: 0.000 min
Response: 23783372
Conc: 19.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK18

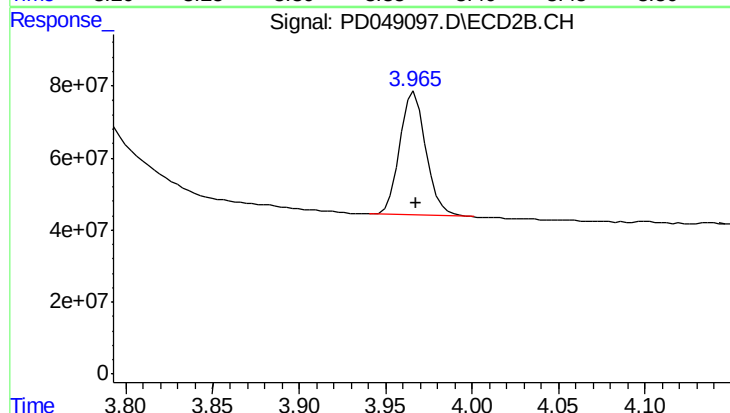


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: 0.000 min
Response: 357940338
Conc: 20.36 ng/ml

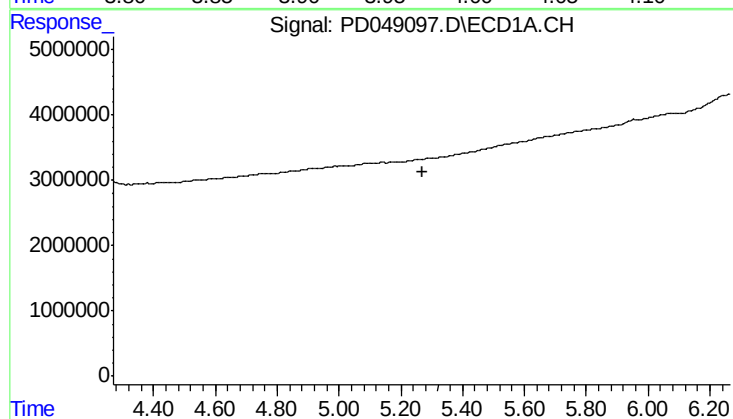


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.270 min
Response: 0
Conc: N.D.

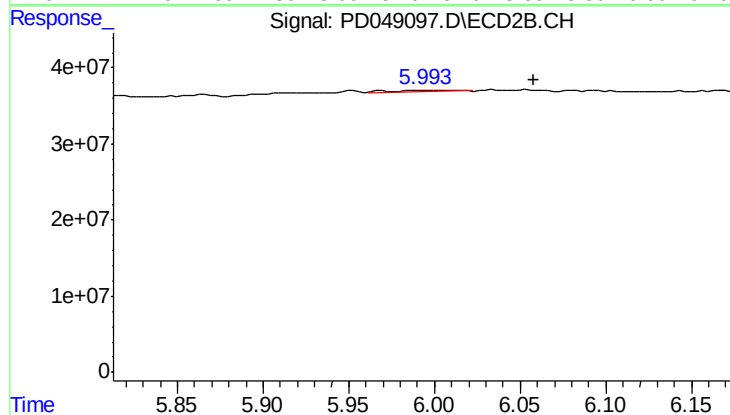

#10 trans-Chlordane


R.T.: 6.008 min
Delta R.T.: -0.051 min
Response: 5870701
Conc: 0.25 ng/ml

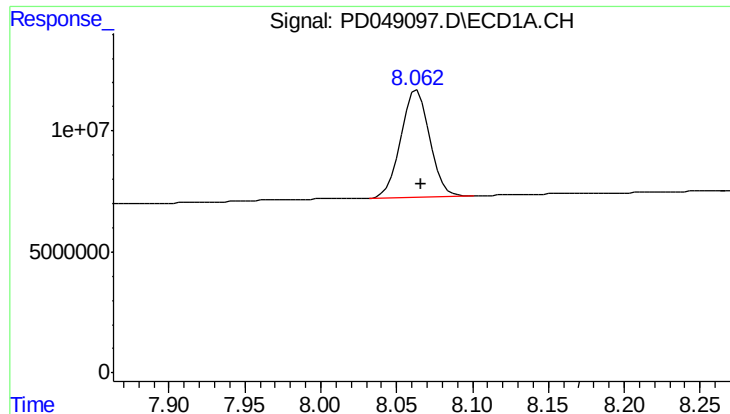

#27 Decachlorobiphenyl

R.T.: 8.064 min
Delta R.T.: -0.003 min
Response: 57613526
Conc: 40.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK18

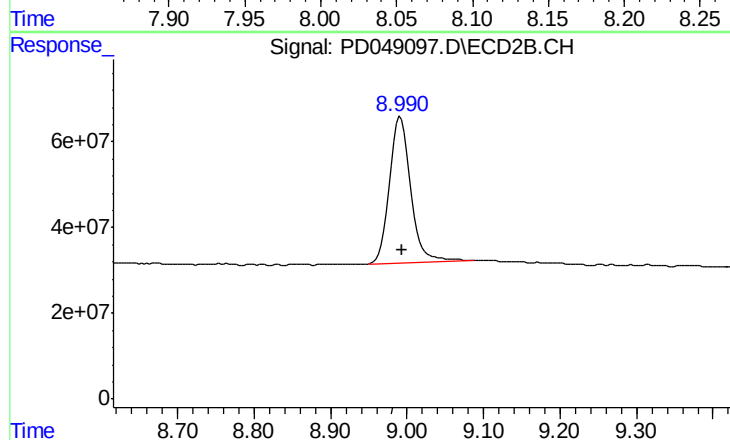

#27 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: -0.001 min
Response: 655524327
Conc: 40.49 ng/ml