

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090523\
 Data File : PD077650.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2023 17:39
 Operator : AR\AJ
 Sample : 04247-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 22:39:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.762	59068763	32929460	26.906	26.433
27)	SA Decachlor...	9.084	7.900	71595363	36438970	28.136	29.232
Target Compounds							
6)	B beta-BHC	0.000	3.847f	0	1363924	N.D.	1.671
7)	B delta-BHC	4.770	0.000	3524216	0	1.063	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090523\
Data File : PD077650.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2023 17:39
Operator : AR\AJ
Sample : 04247-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 22:39:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

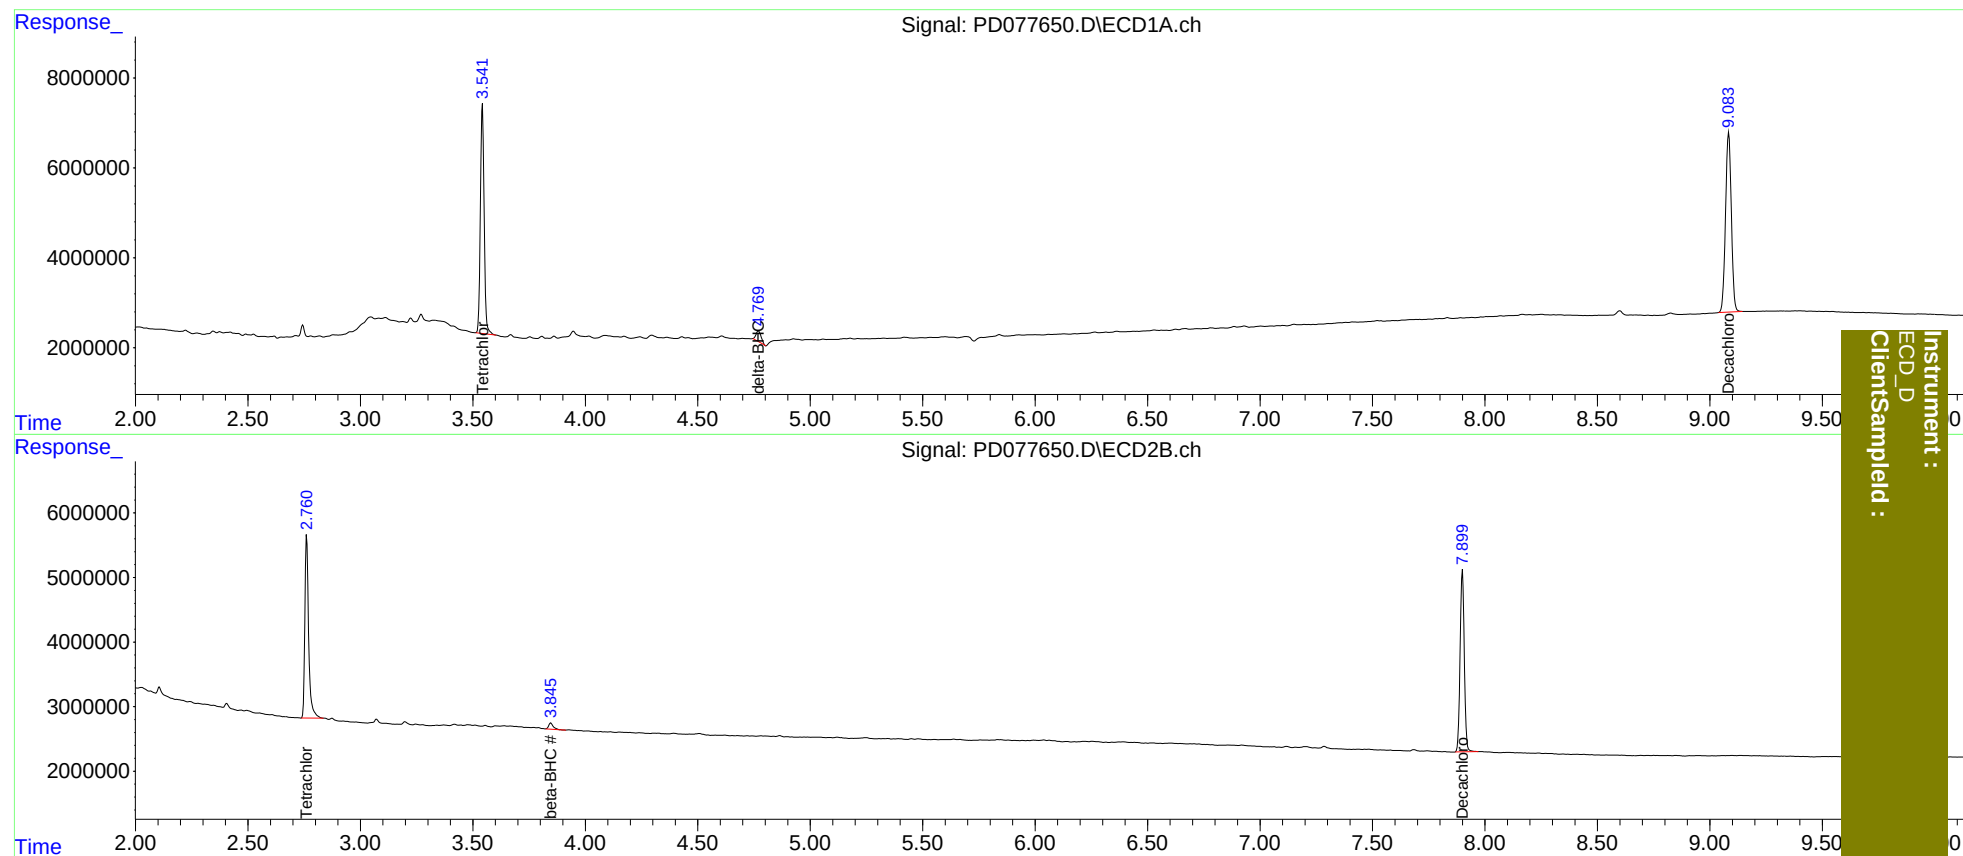


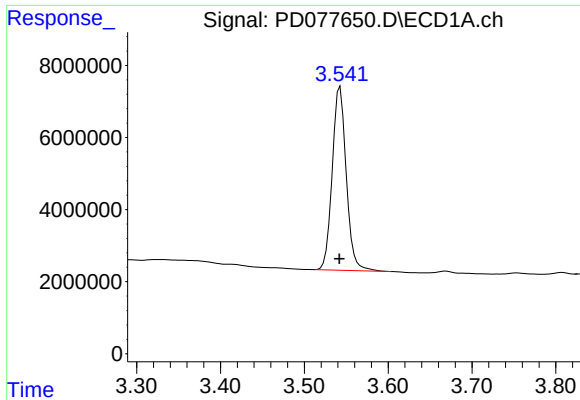

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 59068763
Conc: 26.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

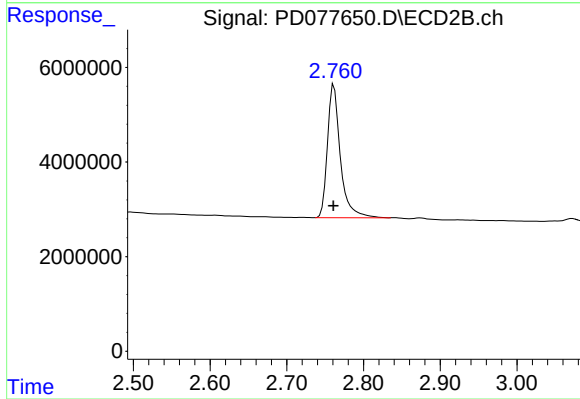


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 32929460
Conc: 26.43 ng/ml

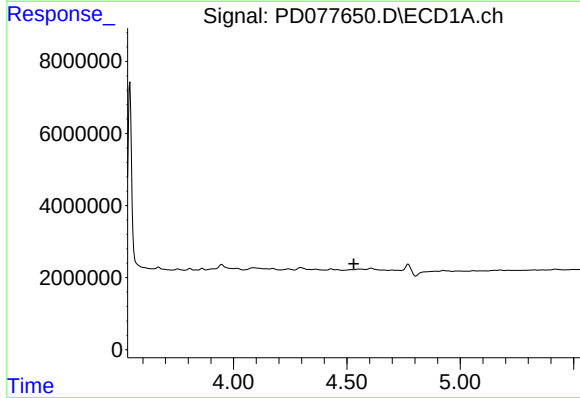


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.530 min
Response: 0
Conc: N.D.

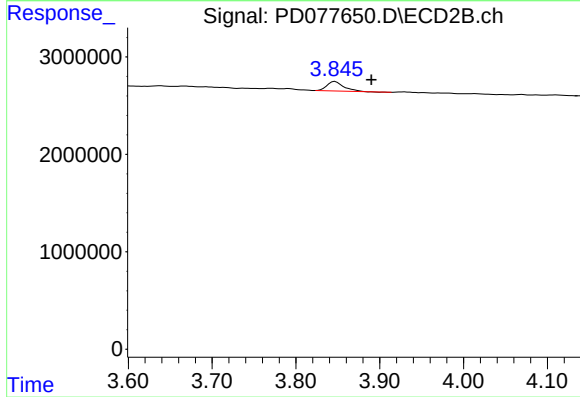

#6 beta-BHC


R.T.: 3.847 min
Delta R.T.: -0.043 min
Response: 1363924
Conc: 1.67 ng/ml

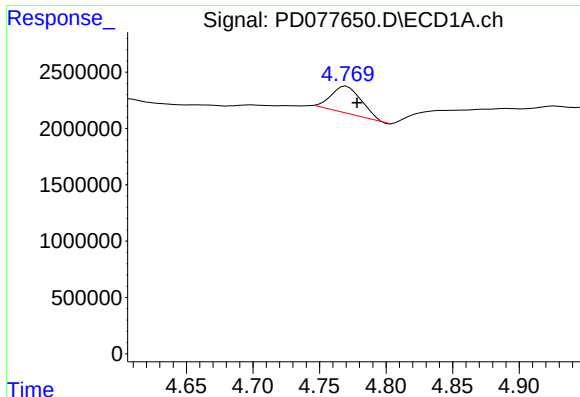

#7 delta-BHC


R.T.: 4.770 min
Delta R.T.: -0.008 min
Response: 3524216
Conc: 1.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

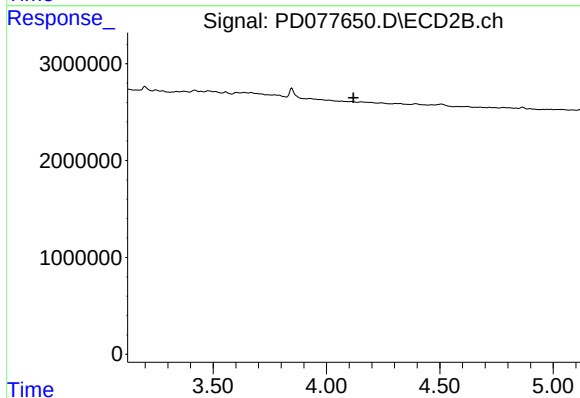


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.119 min
Response: 0
Conc: N.D.

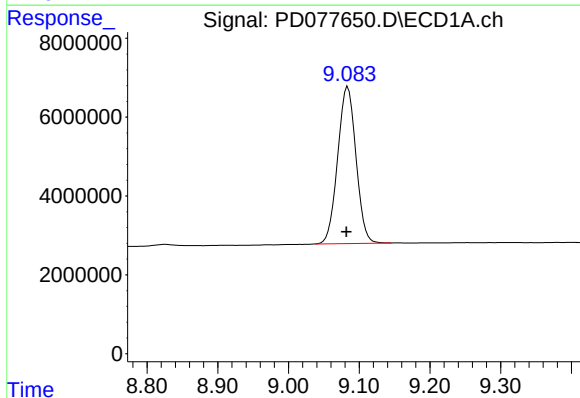

#27 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: 0.002 min
Response: 71595363
Conc: 28.14 ng/ml

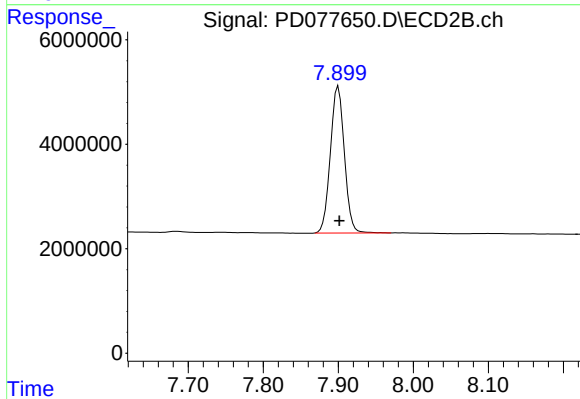

#27 Decachlorobiphenyl

R.T.: 7.900 min
Delta R.T.: -0.001 min
Response: 36438970
Conc: 29.23 ng/ml