

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090523\
 Data File : PD077686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2023 01:57
 Operator : AR\AJ
 Sample : 04262-01
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 05:34:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.761	58723164	32945913	26.748	26.447
27)	SA Decachlor...	9.082	7.899	75972118	38246809	29.856	30.683
Target Compounds							
6)	B beta-BHC	0.000	3.847f	0	441146	N.D.	0.540
7)	B delta-BHC	0.000	4.130	0	303032	N.D.	0.174
8)	B Heptachlo...	0.000	4.781f	0	172977	N.D.	0.106
9)	A Endosulfan I	0.000	5.127f	0	538852	N.D.	0.382
13)	MA Dieldrin	6.356	5.348	1443538	623479	0.463	0.393


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090523\
Data File : PD077686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2023 01:57
Operator : AR\AJ
Sample : 04262-01
Misc :
ALS Vial : 48 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 05:34:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

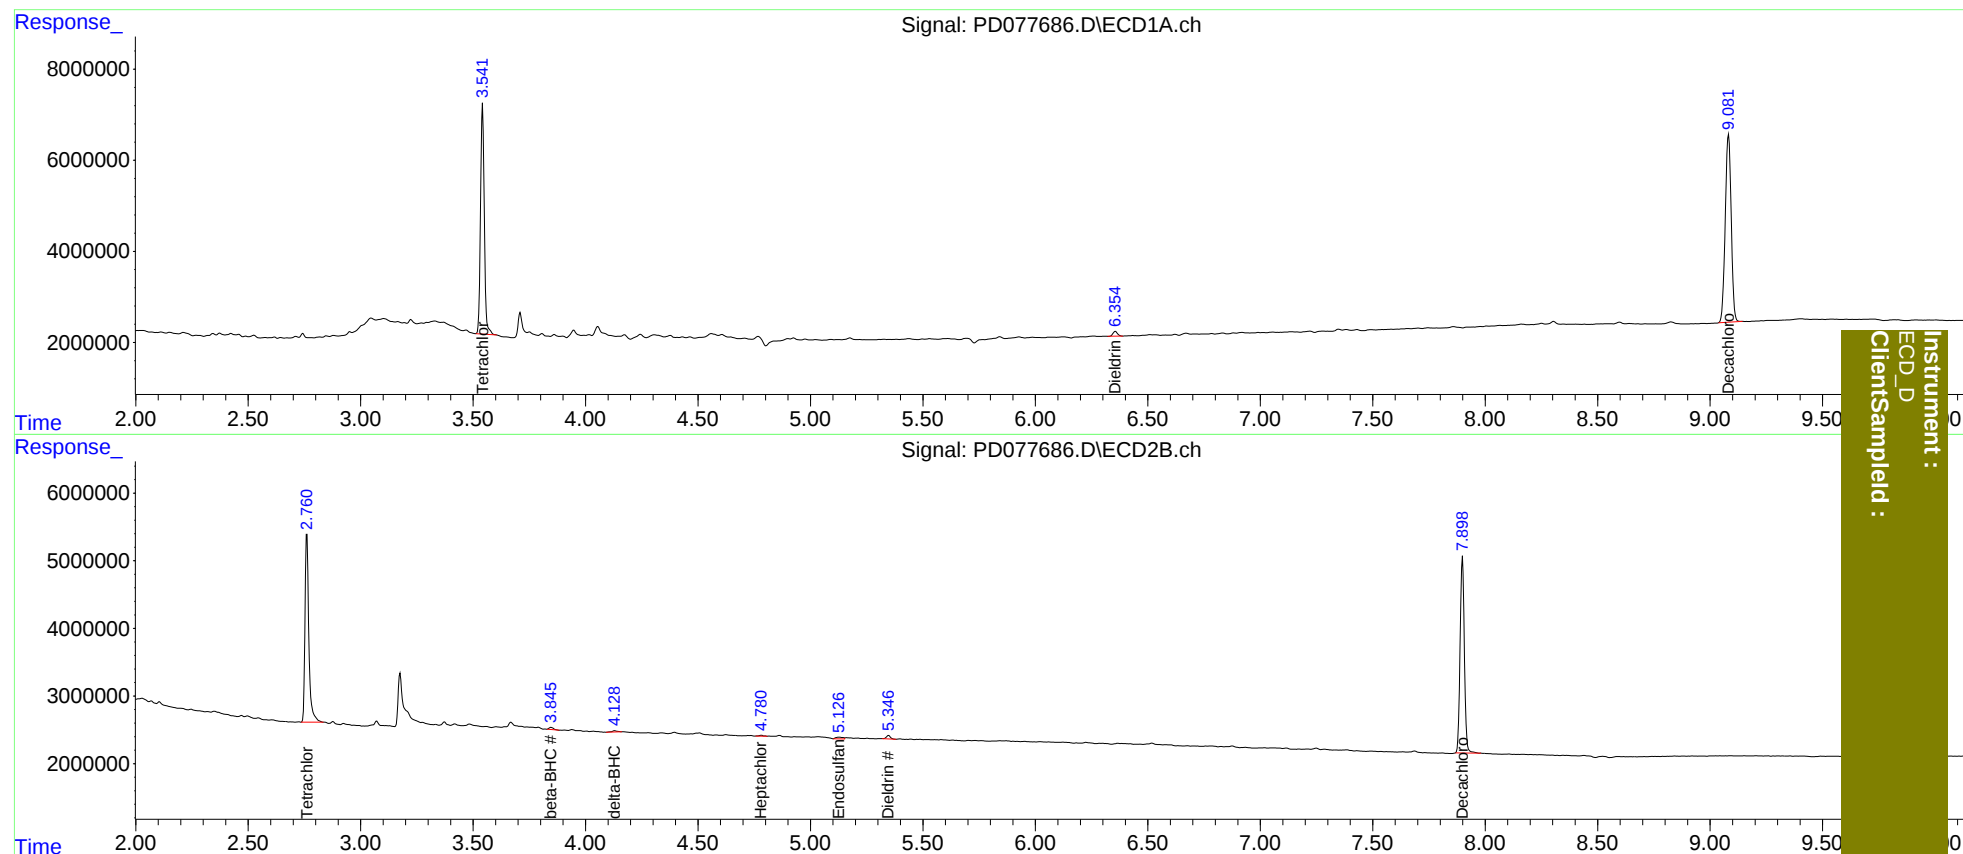


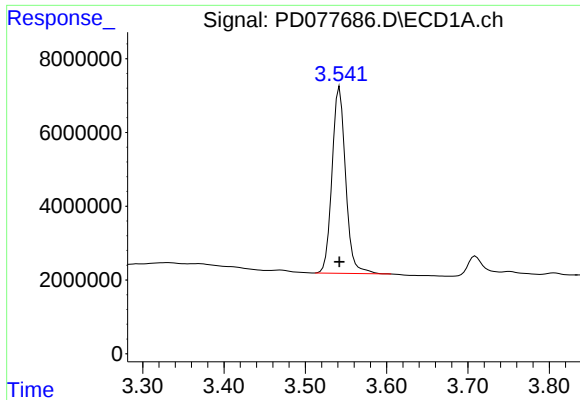

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 58723164
Conc: 26.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

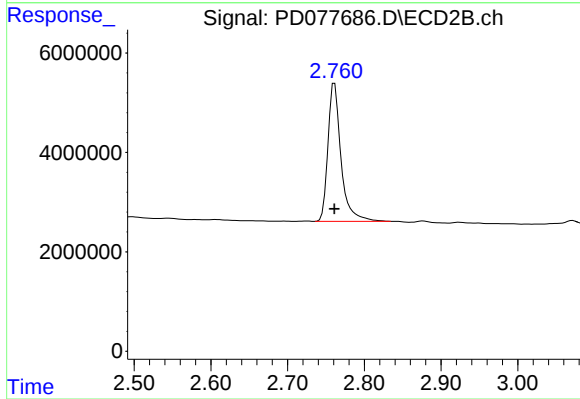


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 32945913
Conc: 26.45 ng/ml

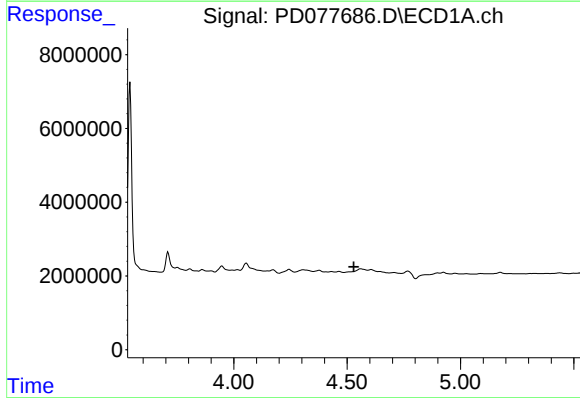


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.530 min
Response: 0
Conc: N.D.

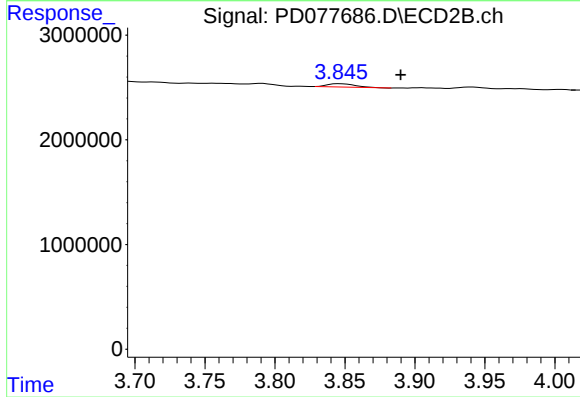

#6 beta-BHC


R.T.: 3.847 min
Delta R.T.: -0.043 min
Response: 441146
Conc: 0.54 ng/ml

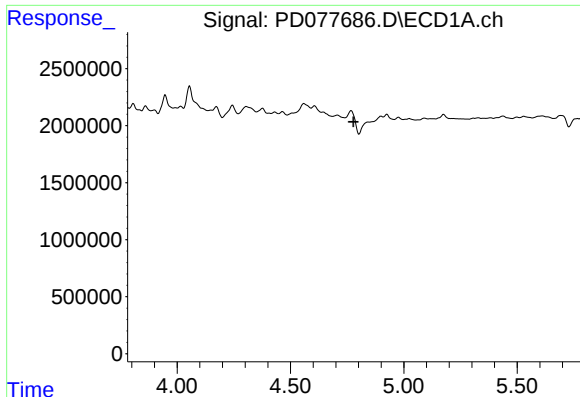

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.778 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

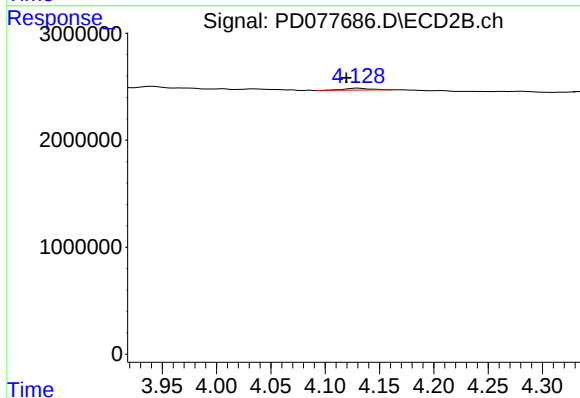


#7 delta-BHC

R.T.: 4.130 min
Delta R.T.: 0.011 min
Response: 303032
Conc: 0.17 ng/ml

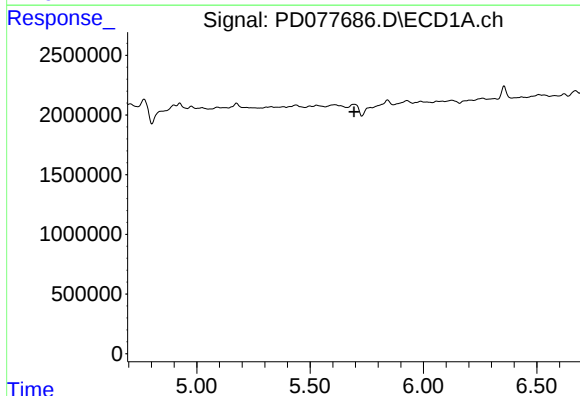


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.694 min
Response: 0
Conc: N.D.

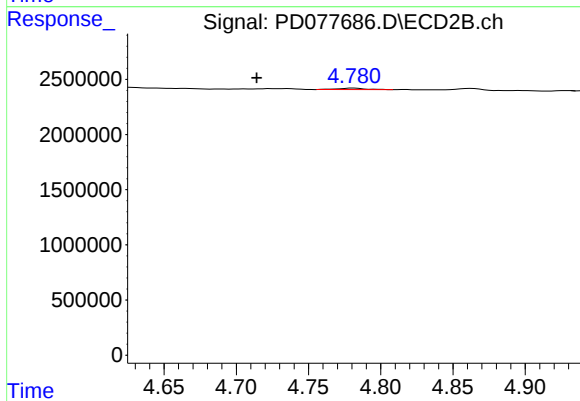

#8 Heptachlor epoxide


R.T.: 4.781 min
Delta R.T.: 0.067 min
Response: 172977
Conc: 0.11 ng/ml

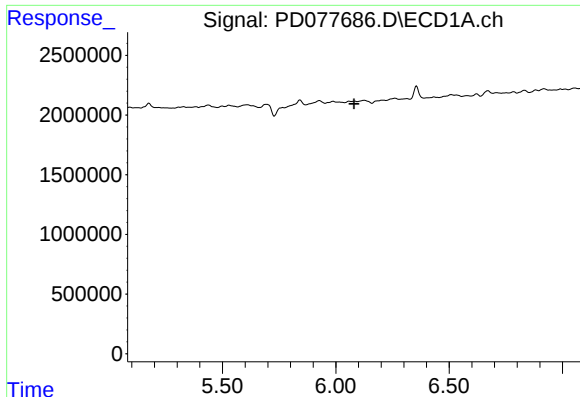

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.080 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

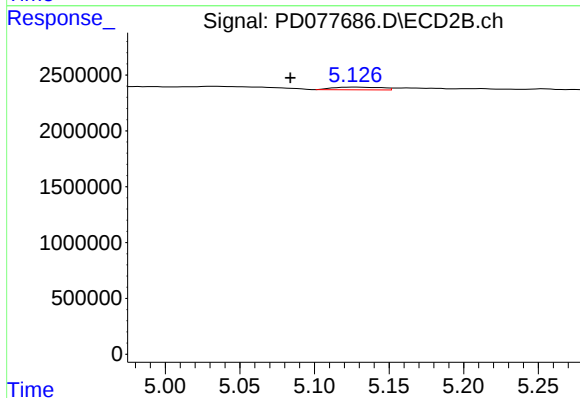


#9 Endosulfan I

R.T.: 5.127 min
Delta R.T.: 0.043 min
Response: 538852
Conc: 0.38 ng/ml

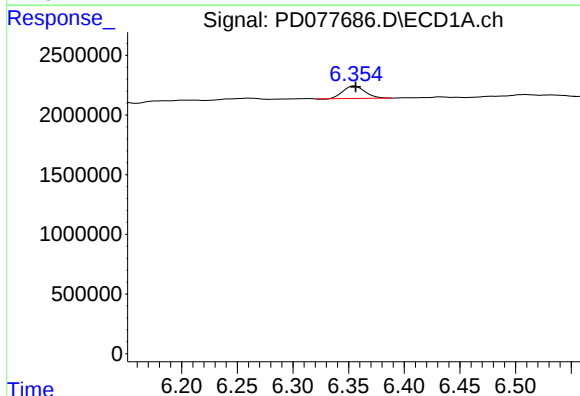


#13 Dieldrin

R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 1443538
Conc: 0.46 ng/ml

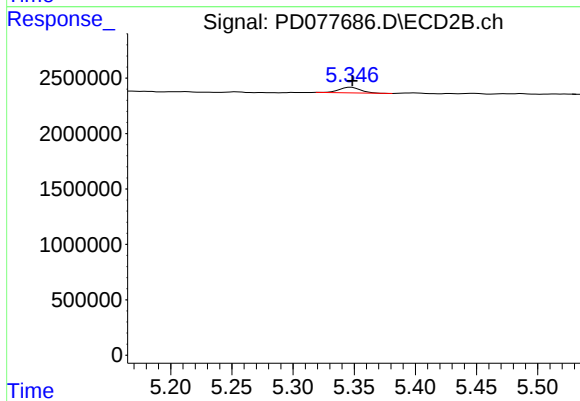

#13 Dieldrin


R.T.: 5.348 min
Delta R.T.: 0.000 min
Response: 623479
Conc: 0.39 ng/ml

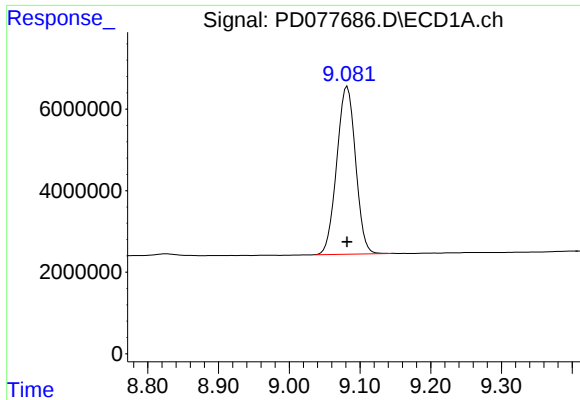

#27 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: 0.000 min
Response: 75972118
Conc: 29.86 ng/ml

Instrument :
ECD_D
ClientSampleId :

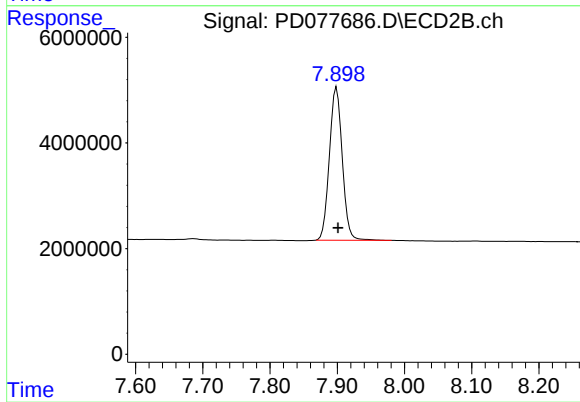

#27 Decachlorobiphenyl

R.T.: 7.899 min
Delta R.T.: -0.002 min
Response: 38246809
Conc: 30.68 ng/ml