

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090523\
 Data File : PD077688.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2023 02:23
 Operator : AR\AJ
 Sample : 04262-03
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 06 05:34:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.761	59813056	33548314	27.245	26.930
27)	SA Decachlor...	9.082	7.899	70840549	36146431	27.839	28.998
Target Compounds							
6)	B beta-BHC	0.000	3.847f	0	1185297	N.D.	1.452
7)	B delta-BHC	4.769	0.000	3017864	0	0.910	N.D. #
8)	B Heptachlo...	0.000	4.779f	0	217110	N.D.	0.133
16)	A 4,4'-DDD	0.000	5.780	0	96916	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090523\
Data File : PD077688.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2023 02:23
Operator : AR\AJ
Sample : 04262-03
Misc :
ALS Vial : 50 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 06 05:34:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

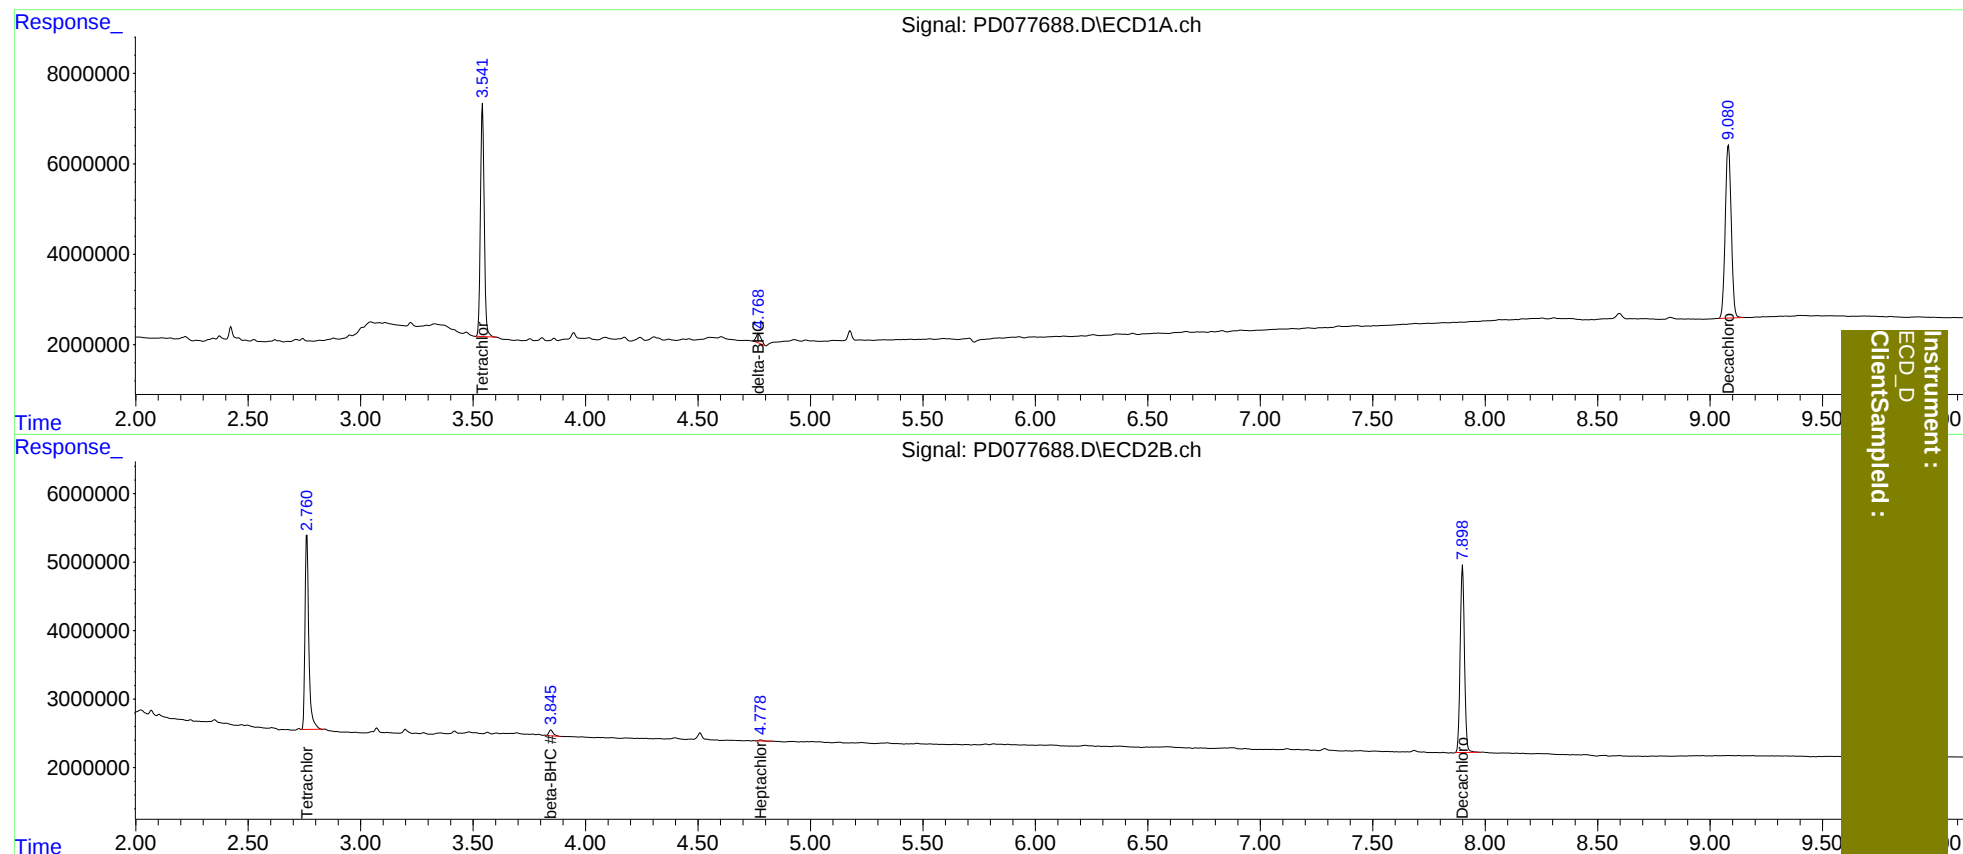


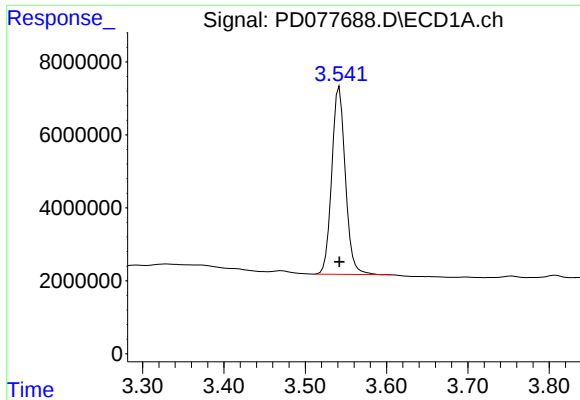

#1 Tetrachloro-m-xylene


R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 59813056
Conc: 27.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

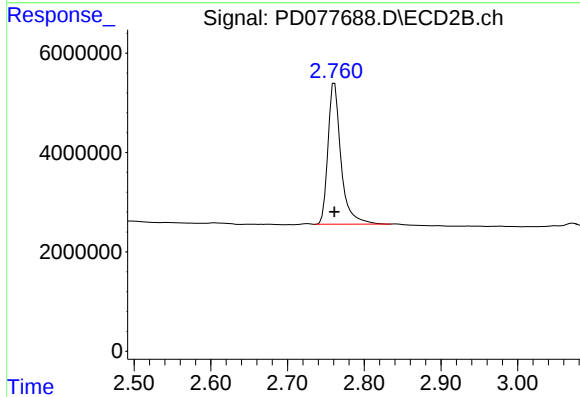


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: 0.000 min
Response: 33548314
Conc: 26.93 ng/ml

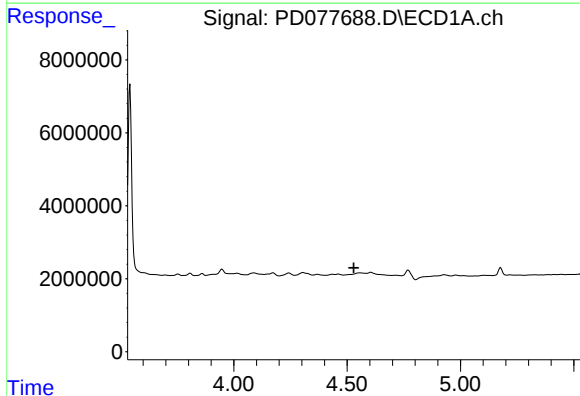


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.530 min
Response: 0
Conc: N.D.

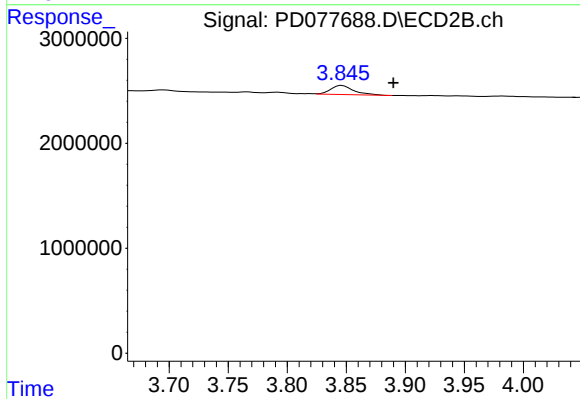

#6 beta-BHC


R.T.: 3.847 min
Delta R.T.: -0.043 min
Response: 1185297
Conc: 1.45 ng/ml

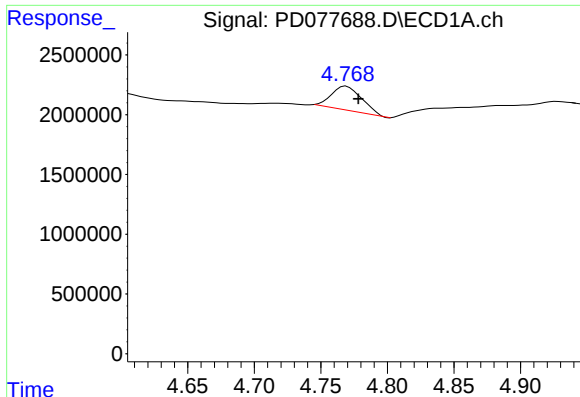

#7 delta-BHC


R.T.: 4.769 min
Delta R.T.: -0.009 min
Response: 3017864
Conc: 0.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

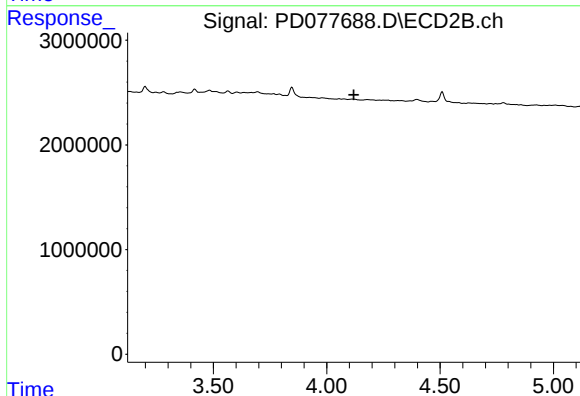


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.119 min
Response: 0
Conc: N.D.

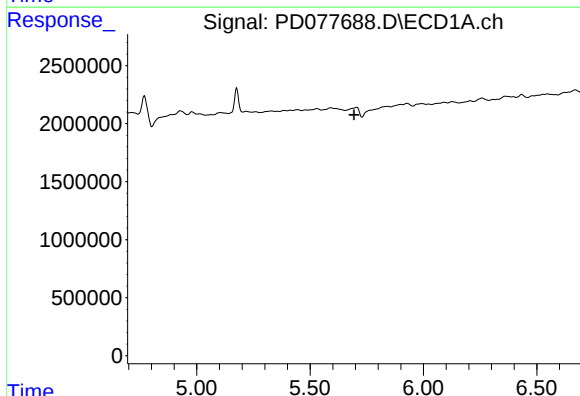


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.694 min
Response: 0
Conc: N.D.

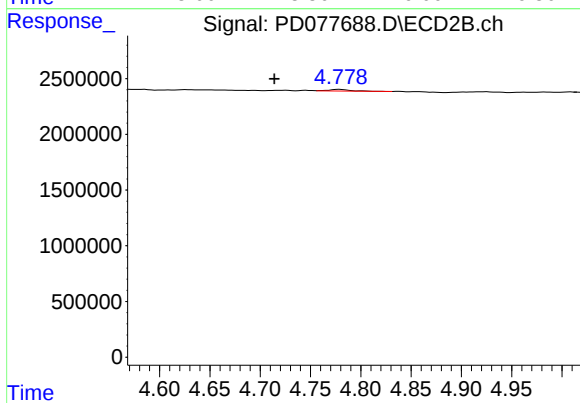

#8 Heptachlor epoxide


R.T.: 4.779 min
Delta R.T.: 0.065 min
Response: 217110
Conc: 0.13 ng/ml

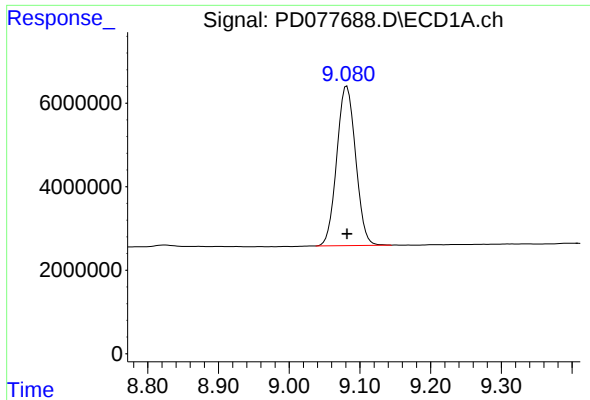

#27 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: 0.000 min
Response: 70840549
Conc: 27.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

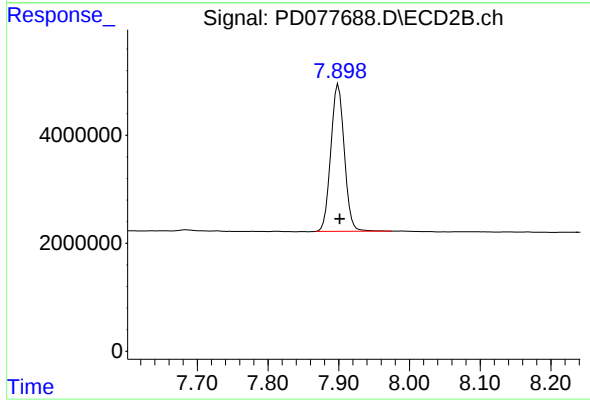

#27 Decachlorobiphenyl

R.T.: 7.899 min
Delta R.T.: -0.002 min
Response: 36146431
Conc: 29.00 ng/ml