

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090523\
 Data File : PD077637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2023 13:38
 Operator : AR\AJ
 Sample : 04227-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BH9W1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/06/2023
 Supervised By : Ankita Jodhani 09/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 22:34:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.540	2.760	37897813	9900656	17.262m	7.948m#
2)	SA Decachlor...	9.085	7.899	50353490	22844929	19.788	18.327m
Target Compounds							
7)	B delta-BHC	4.778	4.142	27537217	21617368	8.308	12.447m#
8)	B Heptachlo...	5.721	4.712	84134683	15474344	26.365m	9.459m#
11)	B cis-Chlor...	6.031	5.029	35263207	34653751	11.014	21.517m#
18)	B Endrin al...	6.940	6.090	30652198	9439371	14.240	8.690 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090523\
Data File : PD077637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2023 13:38
Operator : AR\AJ
Sample : 04227-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 22:34:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 15 01:53:32 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

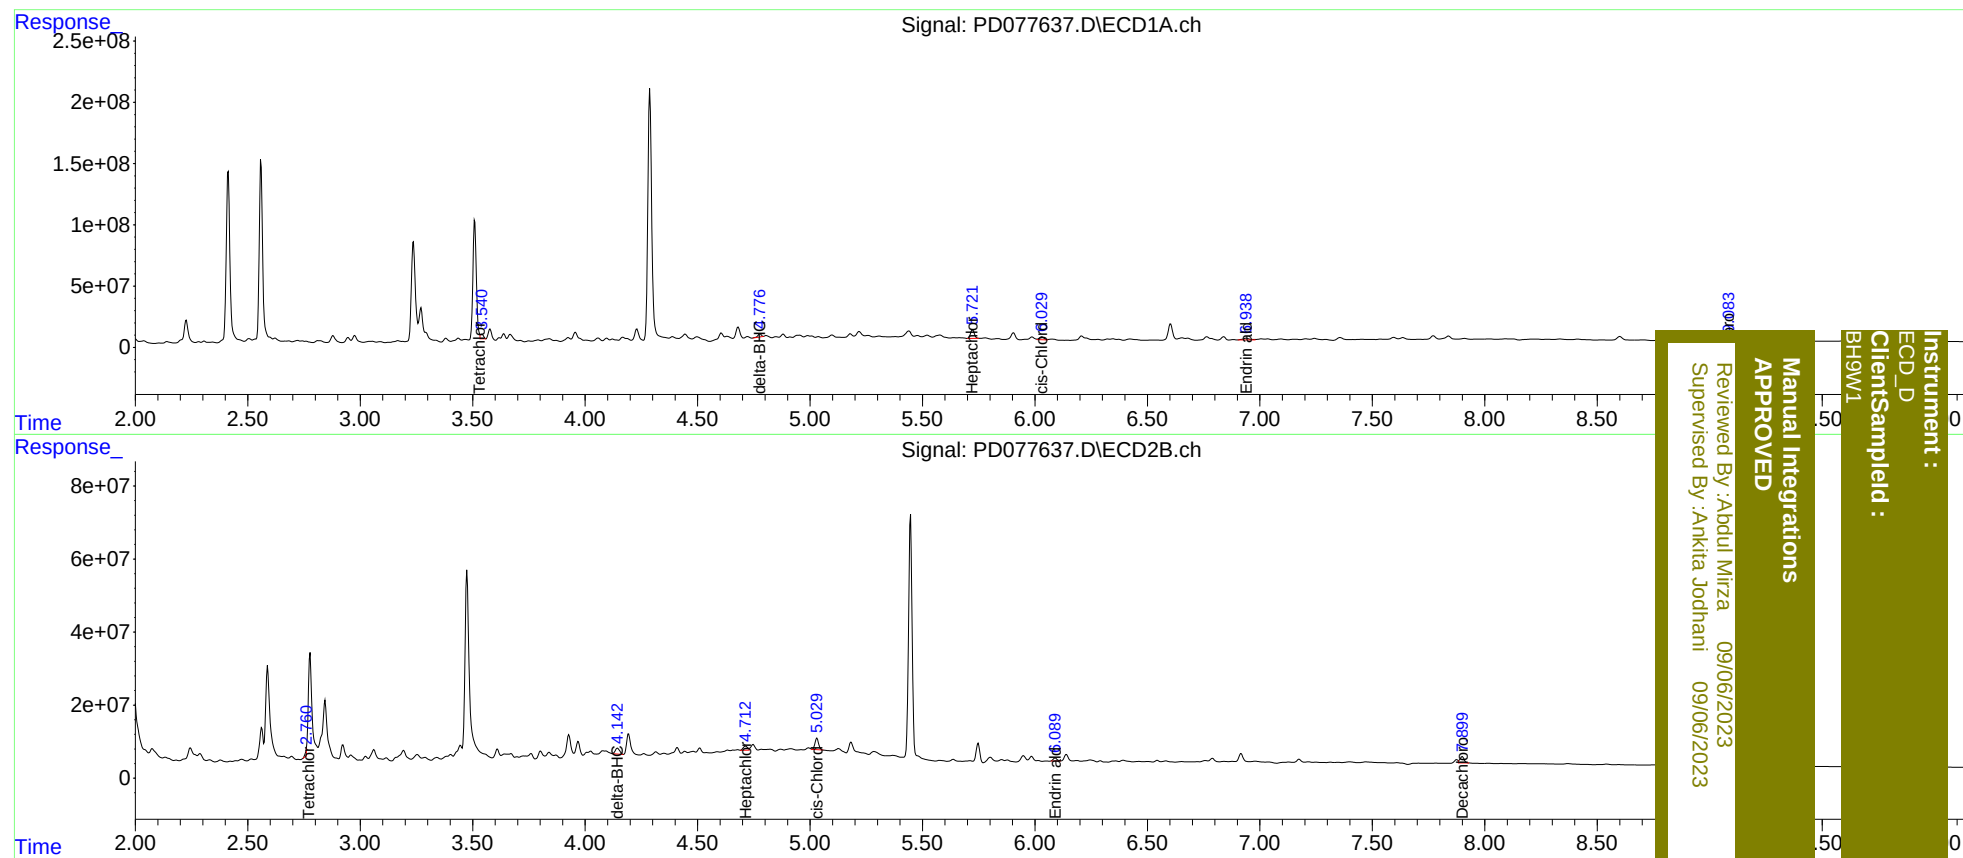

Reviewed By: Abdul Mirza 09/06/2023
Supervised By: Ankita Jodhani 09/06/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BH9W1