

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090523\
 Data File : PD077657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2023 19:30
 Operator : AR\AJ
 Sample : 04247-14
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
ClientSampleId :
 BBJ10

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/06/2023
 Supervised By :Ankita Jodhani 09/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 22:42:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.761	37628532	27074601	17.140	21.734 #
27) SA Decachlor...	9.082	7.899	55877095	28220095	21.959	22.639
Target Compounds						
13) MA Dieldrin	6.357	5.352	1512468	2862580	0.485	1.805m#
15) B Endosulfa...	6.781	5.922	3836011	1126830	1.357	0.842m#
19) B Endosulfa...	7.185	6.341	4460943	6395833	1.792m	5.108m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090523\
 Data File : PD077657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2023 19:30
 Operator : AR\AJ
 Sample : 04247-14
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 22:42:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081423CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 15 01:53:32 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

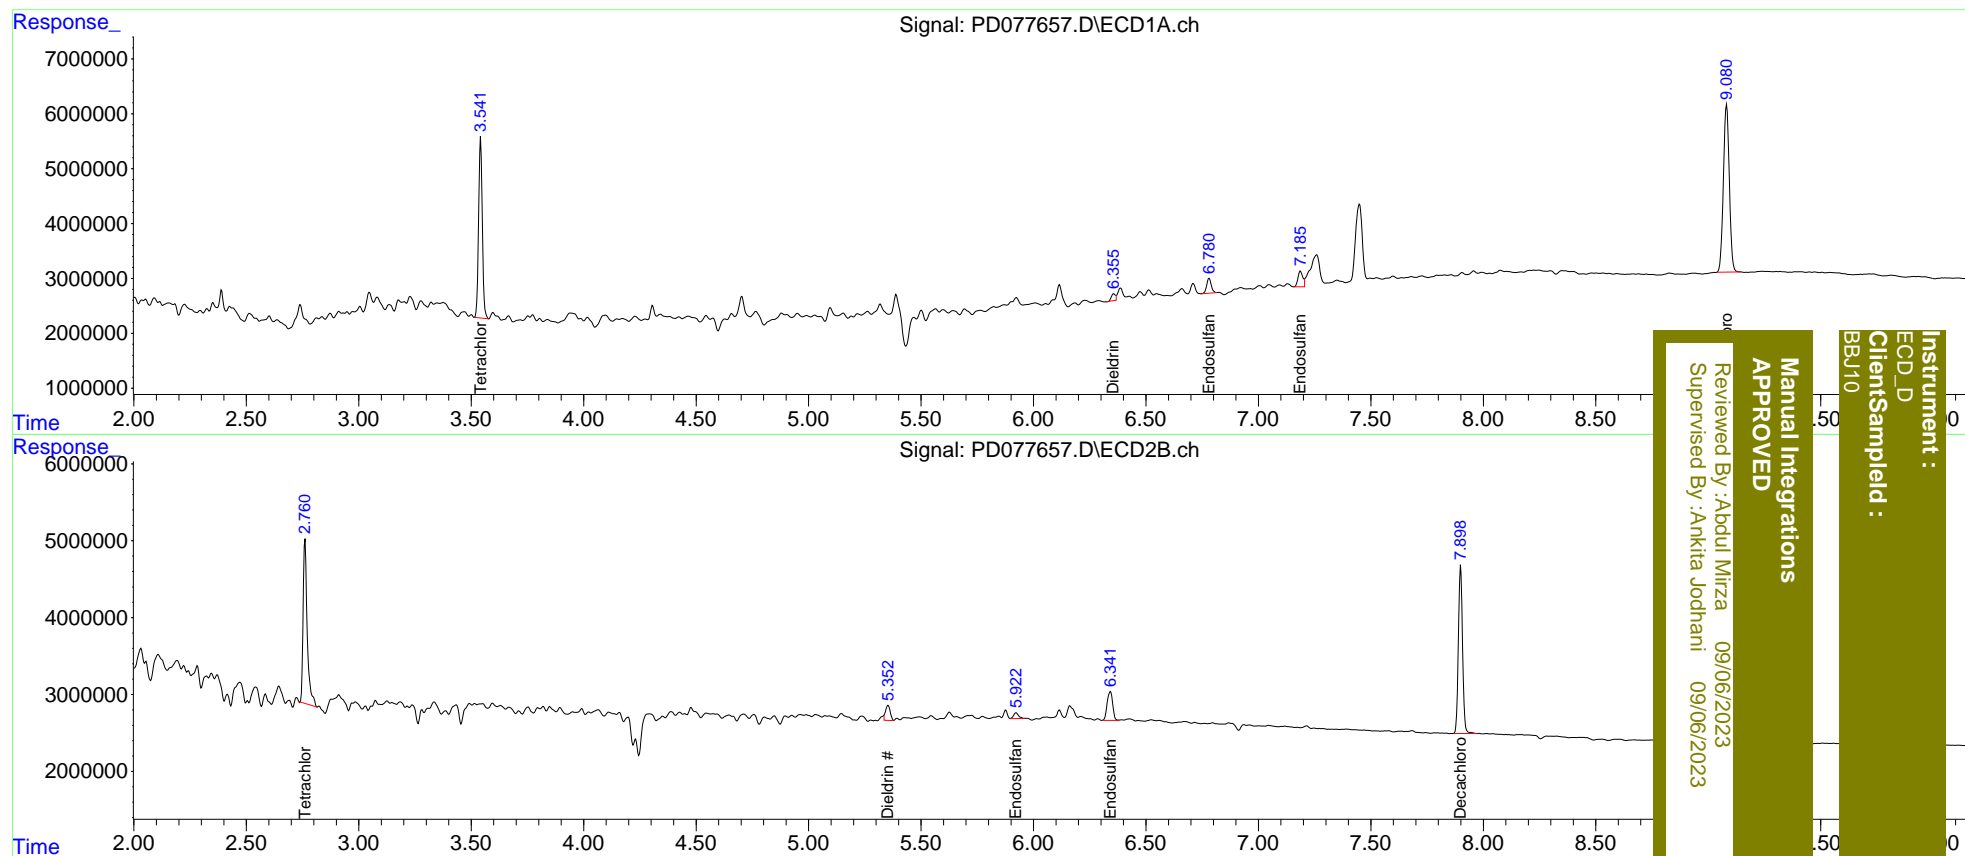

Instrument : ECD_D
 ClientSampled : BBJ10
 Manual Integrations
 APPROVED
 Reviewed By : Abdul Mirza 09/06/2023
 Supervised By : Ankita Jodhani 09/06/2023