

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090623\
 Data File : PD077730.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2023 23:03
 Operator : AR\AJ
 Sample : 04262-06
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BBHM8

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/07/2023
 Supervised By : Ankita Jodhani 09/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 00:20:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.761	57106458	33785129	22.503	22.861
27) SA Decachlor...	9.083	7.899	67541352	35349022	21.621	21.827
Target Compounds						
5) MB Aldrin	5.283	4.191	1675641	911534	0.401	0.407
8) B Heptachlo...	5.714	4.745	11633629	2627654	3.010m	1.251 #
13) MA Dieldrin	6.354	5.346	54970043	30506852	14.686m	14.763m
17) MA 4,4'-DDT	7.024	6.026	2522063	443762	0.921m	0.314 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090623\
Data File : PD077730.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2023 23:03
Operator : AR\AJ
Sample : 04262-06
Misc :
ALS Vial : 45 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 00:20:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

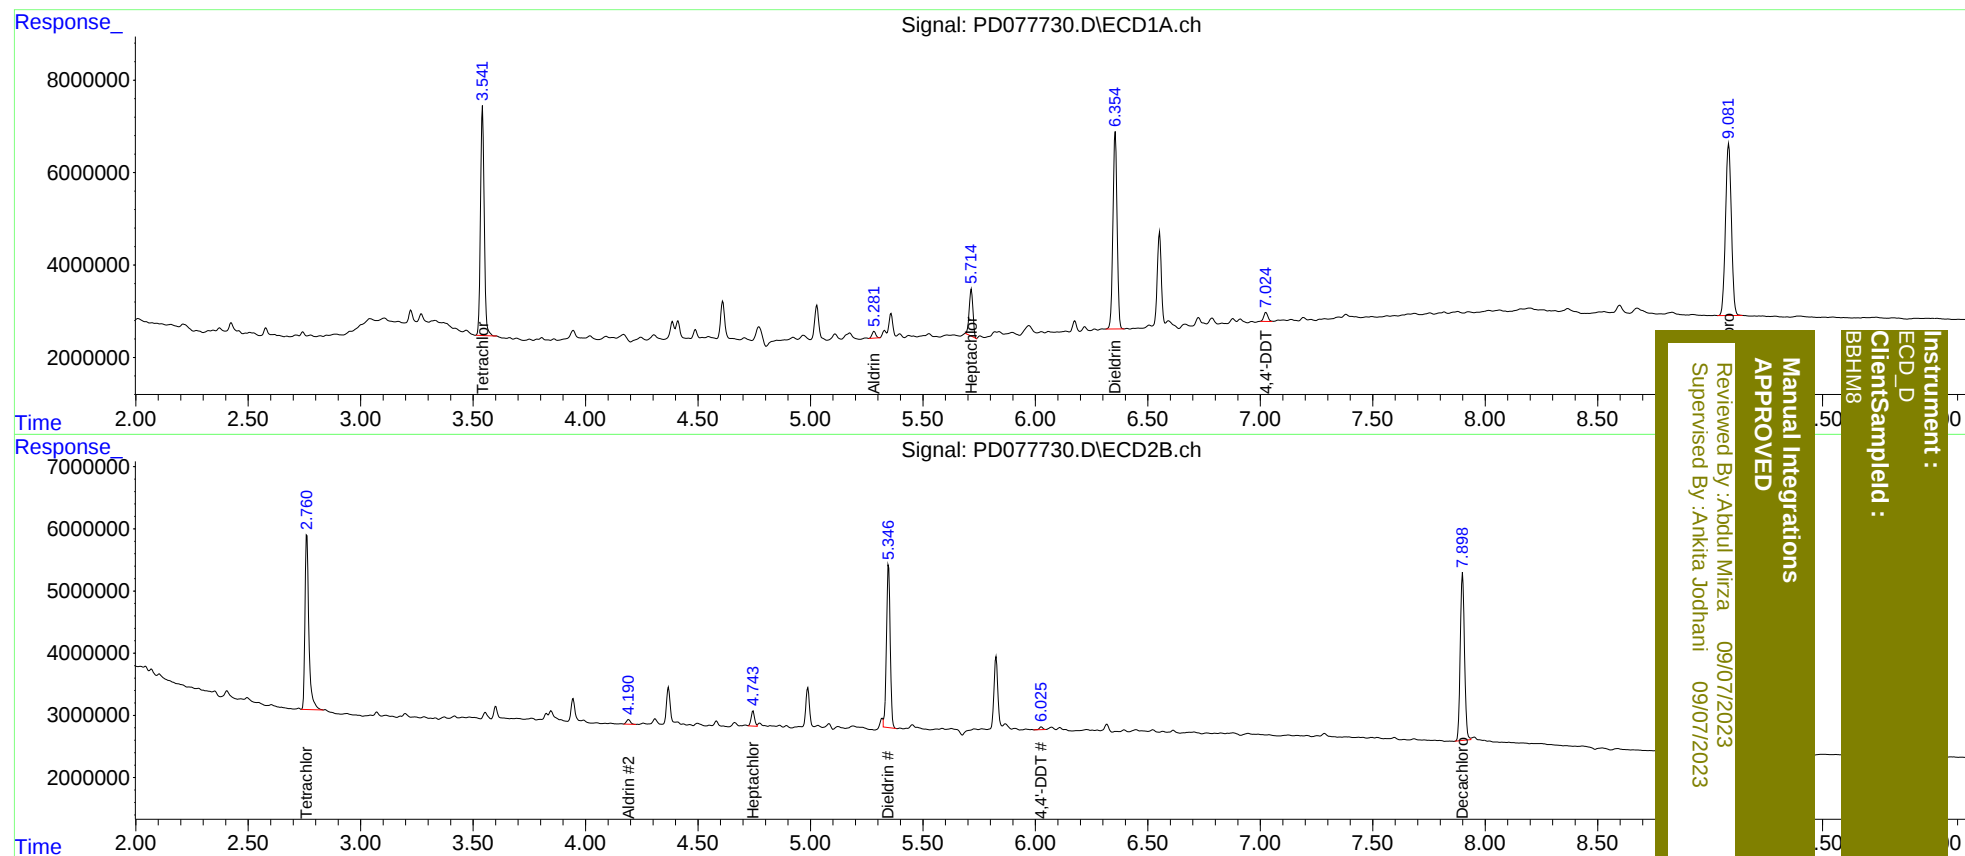

Instrument :
ECD_D
ClientSampled :
BBHM8

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 09/07/2023
Supervised By: Ankita Jodhani 09/07/2023