

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090721\
 Data File : PD065571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2021 08:51
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 15:31:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 04 01:23:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	22081950	177.2E6	22.532	24.179
28)	SA Decachlor...	8.239	9.085	34940359	116.5E6	20.266	21.837
Target Compounds							
21)	B Endrin ke...	0.000	7.775	0	8862541	N.D.	1.171 #
22)	Mirex	7.387	8.234f	893118	3707731	0.570	0.701
23)	Chlordane-1	4.393f	0.000	2095930	0	50.688	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090721\
Data File : PD065571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2021 08:51
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 15:31:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Sat Sep 04 01:23:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

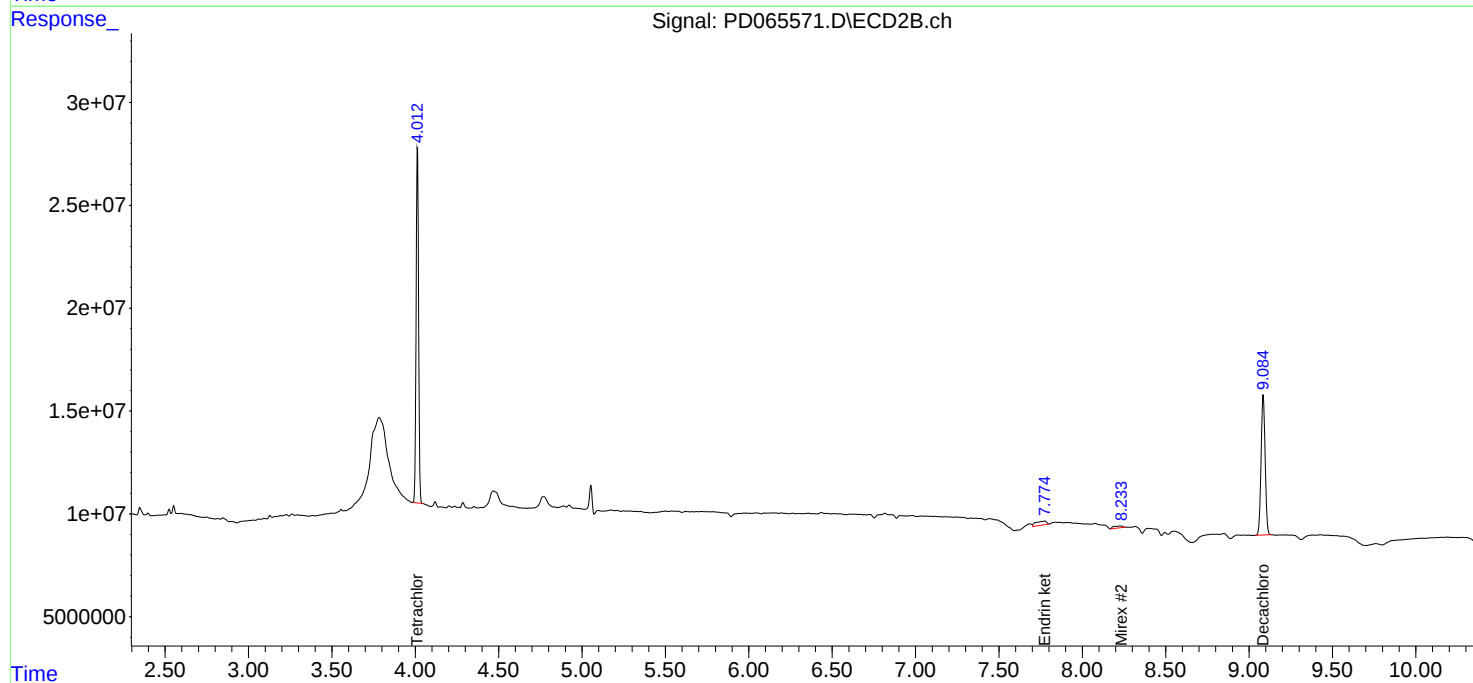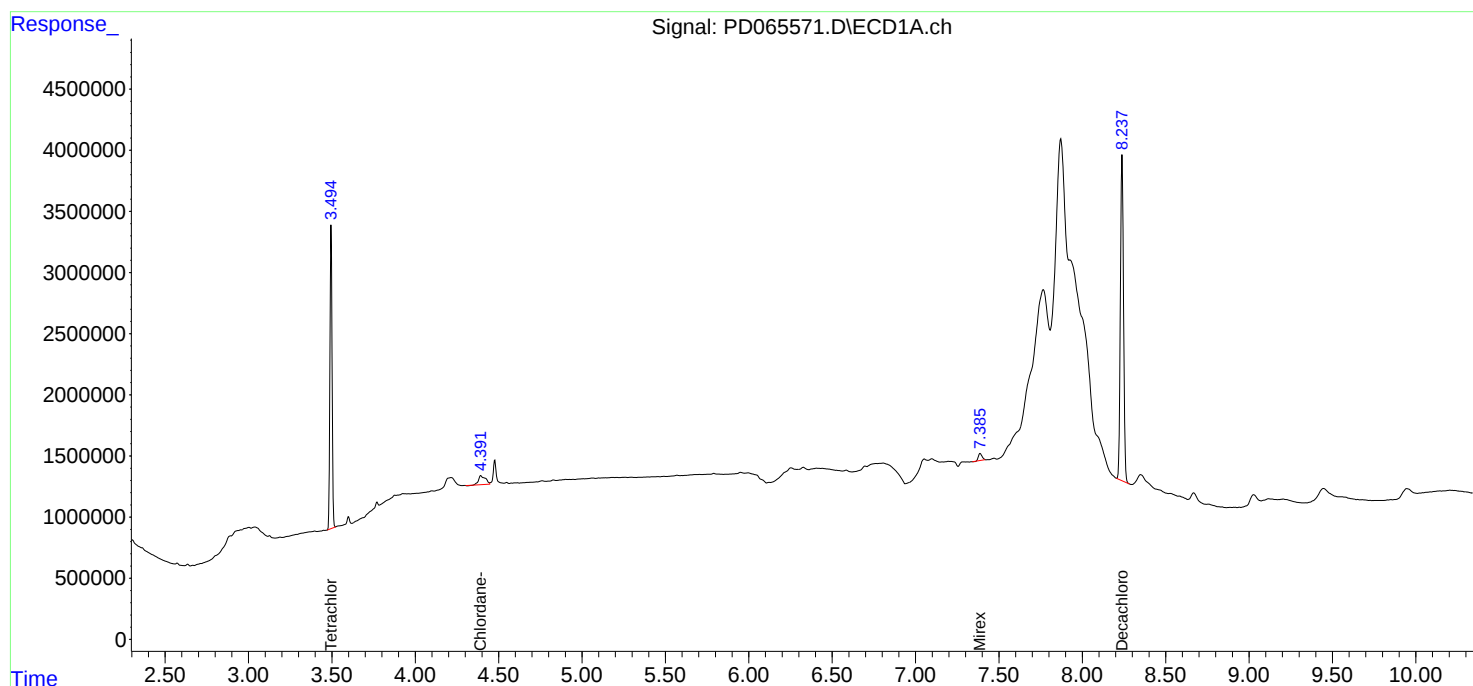


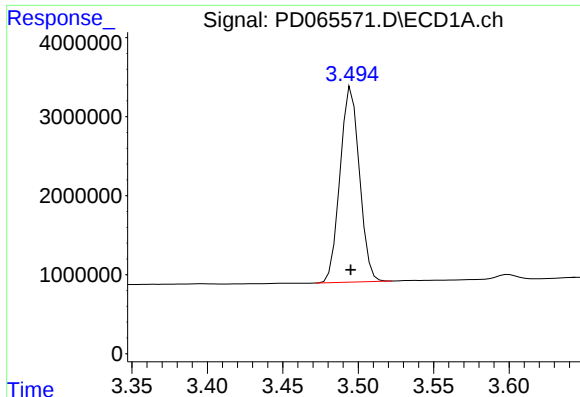

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 22081950
Conc: 22.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

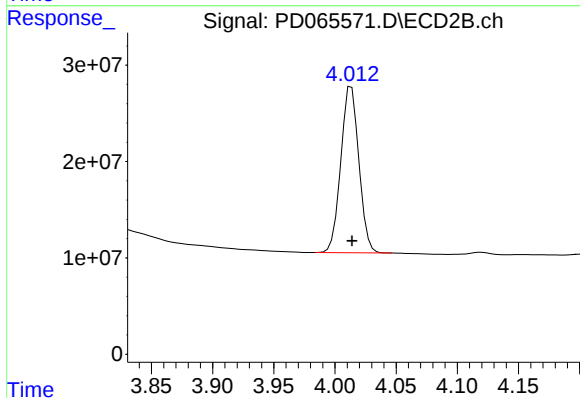


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 177217589
Conc: 24.18 ng/ml

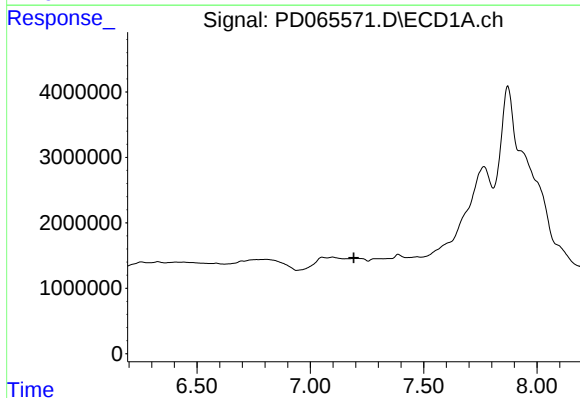


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.192 min
Response: 0
Conc: N.D.

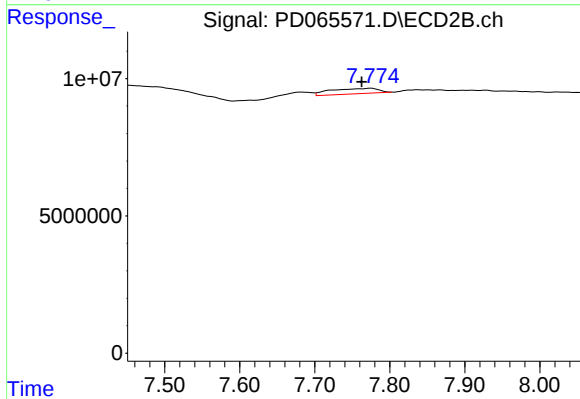

#21 Endrin ketone


R.T.: 7.775 min
Delta R.T.: 0.012 min
Response: 8862541
Conc: 1.17 ng/ml

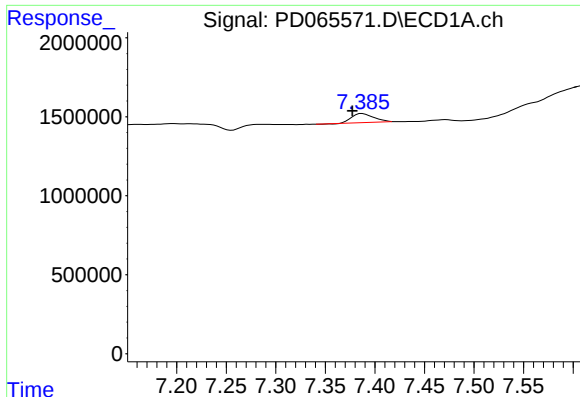

#22 Mirex


R.T.: 7.387 min
Delta R.T.: 0.010 min
Response: 893118
Conc: 0.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

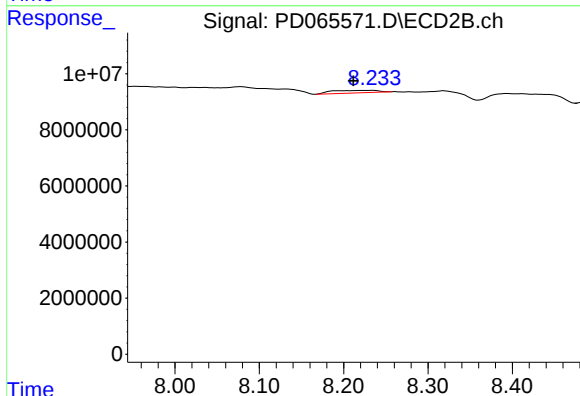


#22 Mirex

R.T.: 8.234 min
Delta R.T.: 0.023 min
Response: 3707731
Conc: 0.70 ng/ml

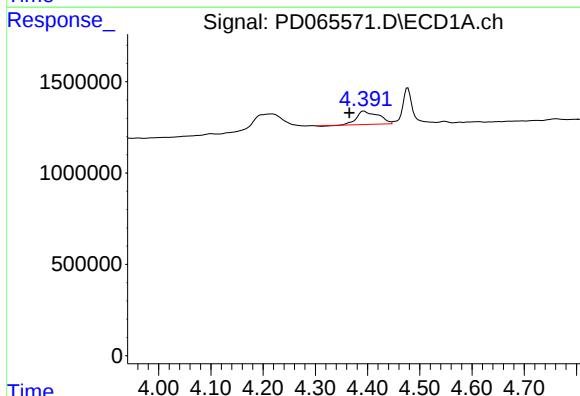


#23 Chlordane-1

R.T.: 4.393 min
Delta R.T.: 0.028 min
Response: 2095930
Conc: 50.69 ng/ml

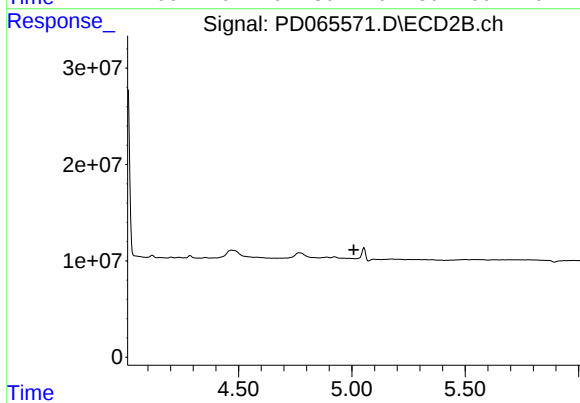

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.008 min
Response: 0
Conc: N.D.

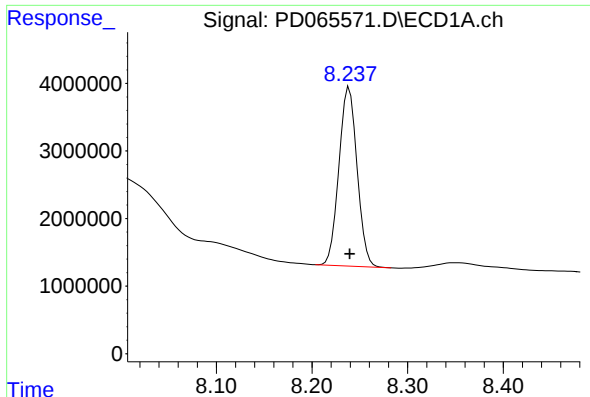

#28 Decachlorobiphenyl

R.T.: 8.239 min
Delta R.T.: 0.000 min
Response: 34940359
Conc: 20.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

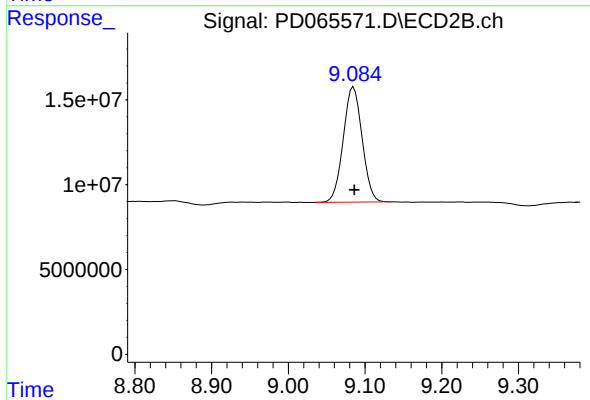

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: -0.001 min
Response: 116520883
Conc: 21.84 ng/ml