

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090721\
 Data File : PD065574.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2021 09:42
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 16:52:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX090421.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 04 01:38:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.499	4.014	48365505	375.9E6	49.922	51.335
7) SA Decachlor...	8.244	9.088	76910726	249.5E6	45.959	47.675
Target Compounds						
2) Toxaphene-1	5.751	6.409	5143964	17835293	478.261	542.739
3) Toxaphene-2	5.913	6.601	5788594	29450881	480.670	475.739
4) Toxaphene-3	6.355	7.185	12705338	55542765	483.819	493.700
5) Toxaphene-4	6.601	7.271	13926661	55226924	478.706	478.837
6) Toxaphene-5	7.087	7.689	16089628	43544822	472.130	480.358

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090721\
Data File : PD065574.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2021 09:42
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 16:52:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX090421.M
Quant Title : GC Extractables
QLast Update : Sat Sep 04 01:38:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

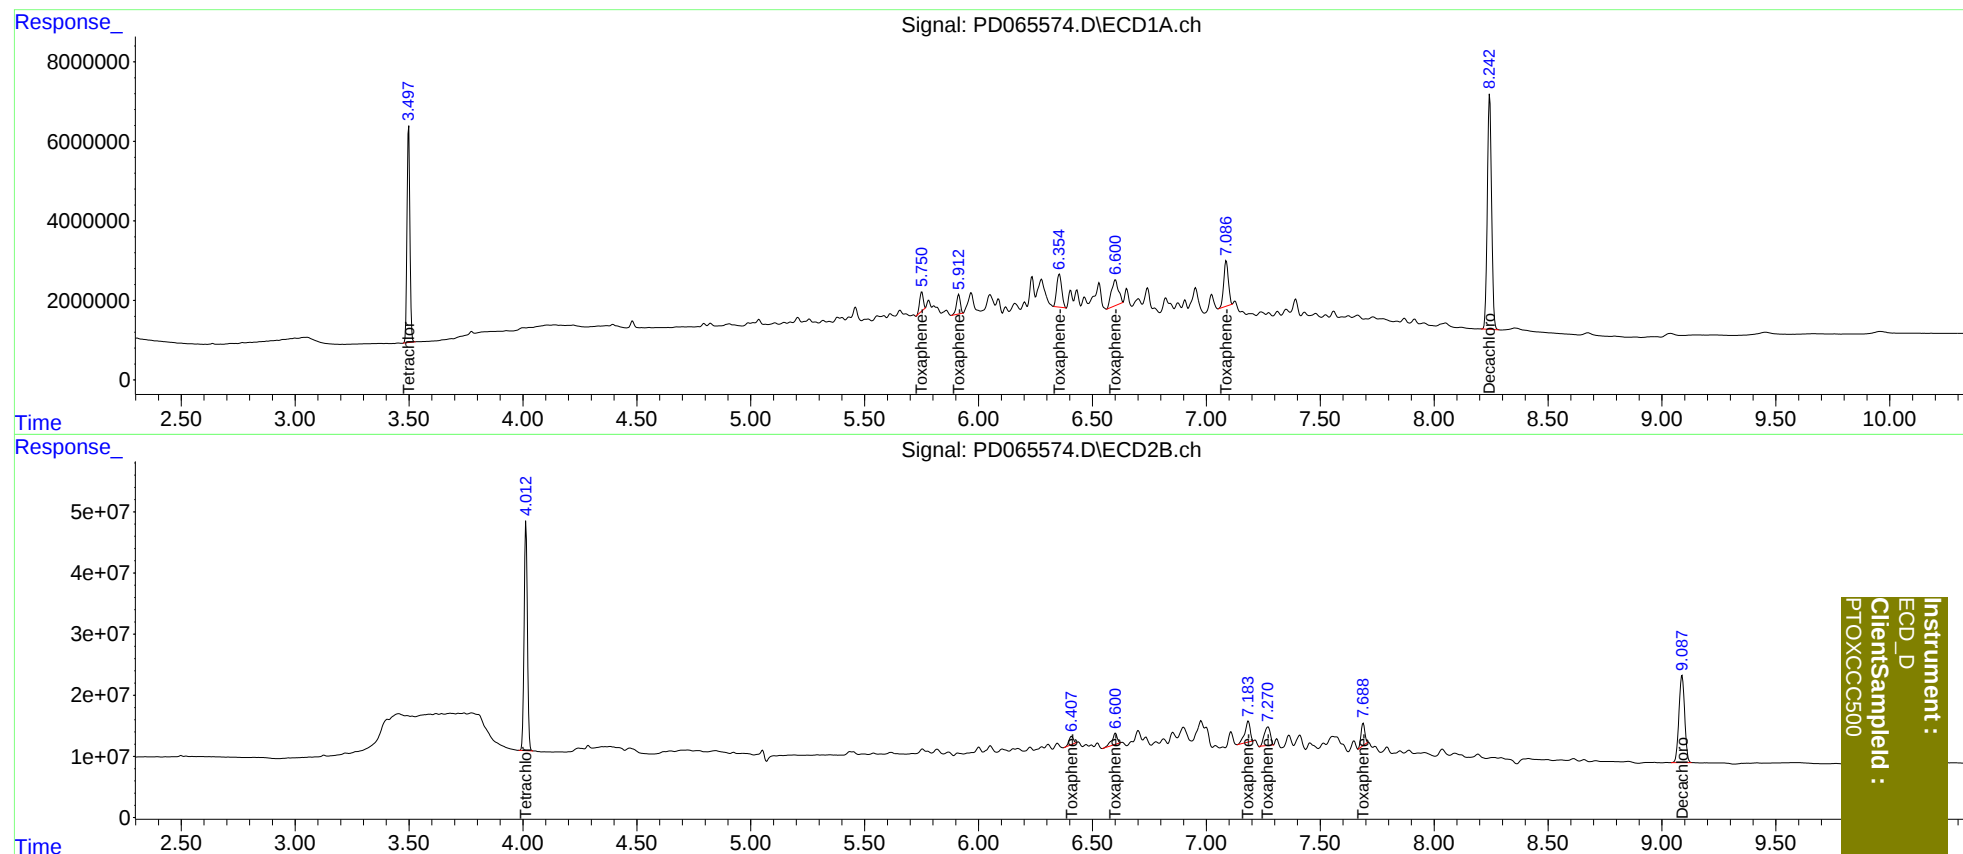

Instrument :
ECD_D
ClientSampled :
PTOXCCC500