

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090721\
 Data File : PD065583.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2021 12:32
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 16:52:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX090421.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 04 01:38:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.495	4.013	49190285	379.5E6	50.773	51.829
7) SA Decachlor...	8.238	9.085	79711017	255.0E6	47.632	48.723
Target Compounds						
2) Toxaphene-1	5.747	6.407	5225489	17816015	485.841	542.153
3) Toxaphene-2	5.909	6.599	5701497	31542048	473.437	509.519
4) Toxaphene-3	6.350	7.182	12771679	56138660	486.345	498.996
5) Toxaphene-4	6.595	7.268	14175582	56878252	487.262	493.155
6) Toxaphene-5	7.081	7.687	16062153	45979812	471.324	507.220

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090721\
Data File : PD065583.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2021 12:32
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 16:52:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX090421.M
Quant Title : GC Extractables
QLast Update : Sat Sep 04 01:38:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

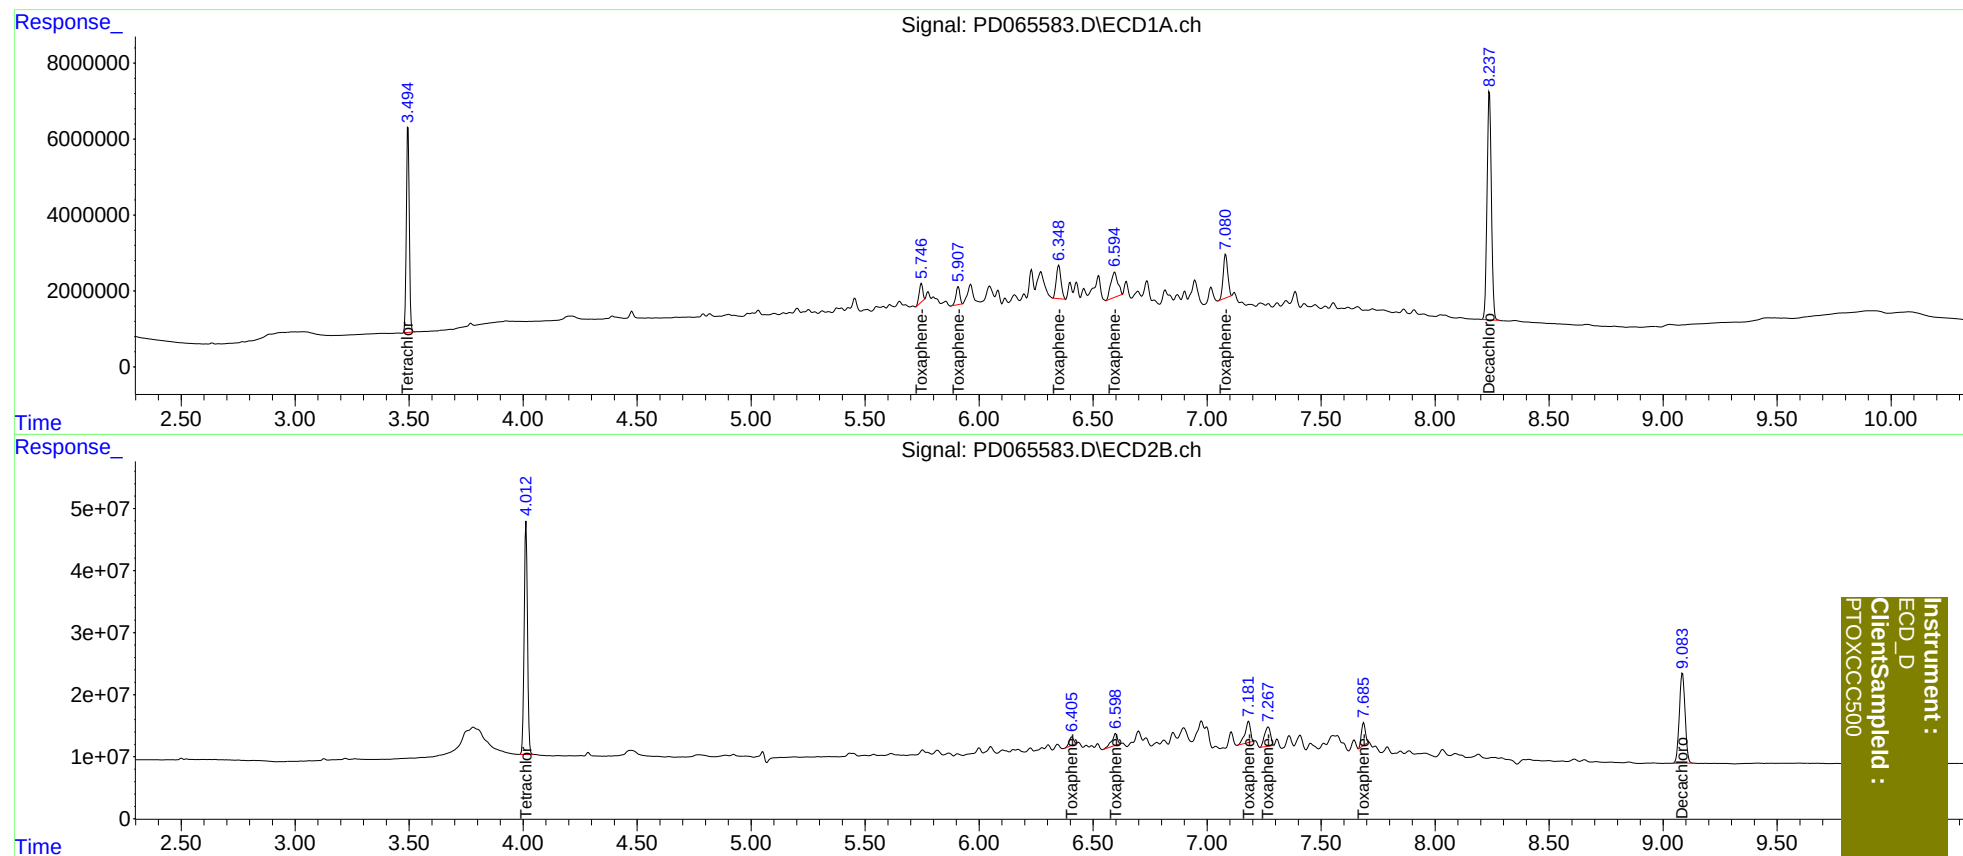

Instrument :
ECD_D
ClientSampled :
PTOXCCC500