

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090723\
 Data File : PD077733.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2023 08:44
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 00:30:14 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
4) MA	Heptachlor	0.000	3.935	0	256057	N.D. 0.115
5) MB	Aldrin	0.000	4.194	0	7322349	N.D. 3.267
6) B	beta-BHC	0.000	3.844f	0	849860	N.D. 0.860
8) B	Heptachlo...	5.699	0.000	13746379	0	3.557 N.D. #
9) A	Endosulfan I	0.000	5.134f	0	3512802	N.D. 1.957
12) B	4,4'-DDE	0.000	5.167f	0	249970	N.D. 0.132
14) MA	Endrin	6.533f	5.645	9661385	651536	3.131 0.356 #
15) B	Endosulfa...	0.000	5.903	0	1114638	N.D. 0.616
17) MA	4,4'-DDT	0.000	5.954f	0	318801	N.D. 0.226
22)	Toxaphene-1	6.275	0.000	1589430	0	59.568 N.D. #
23)	Toxaphene-2	0.000	5.645	0	651536	N.D. 54.030
24)	Toxaphene-3	0.000	5.954	0	318801	N.D. 23.376


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090723\
Data File : PD077733.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2023 08:44
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 00:30:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

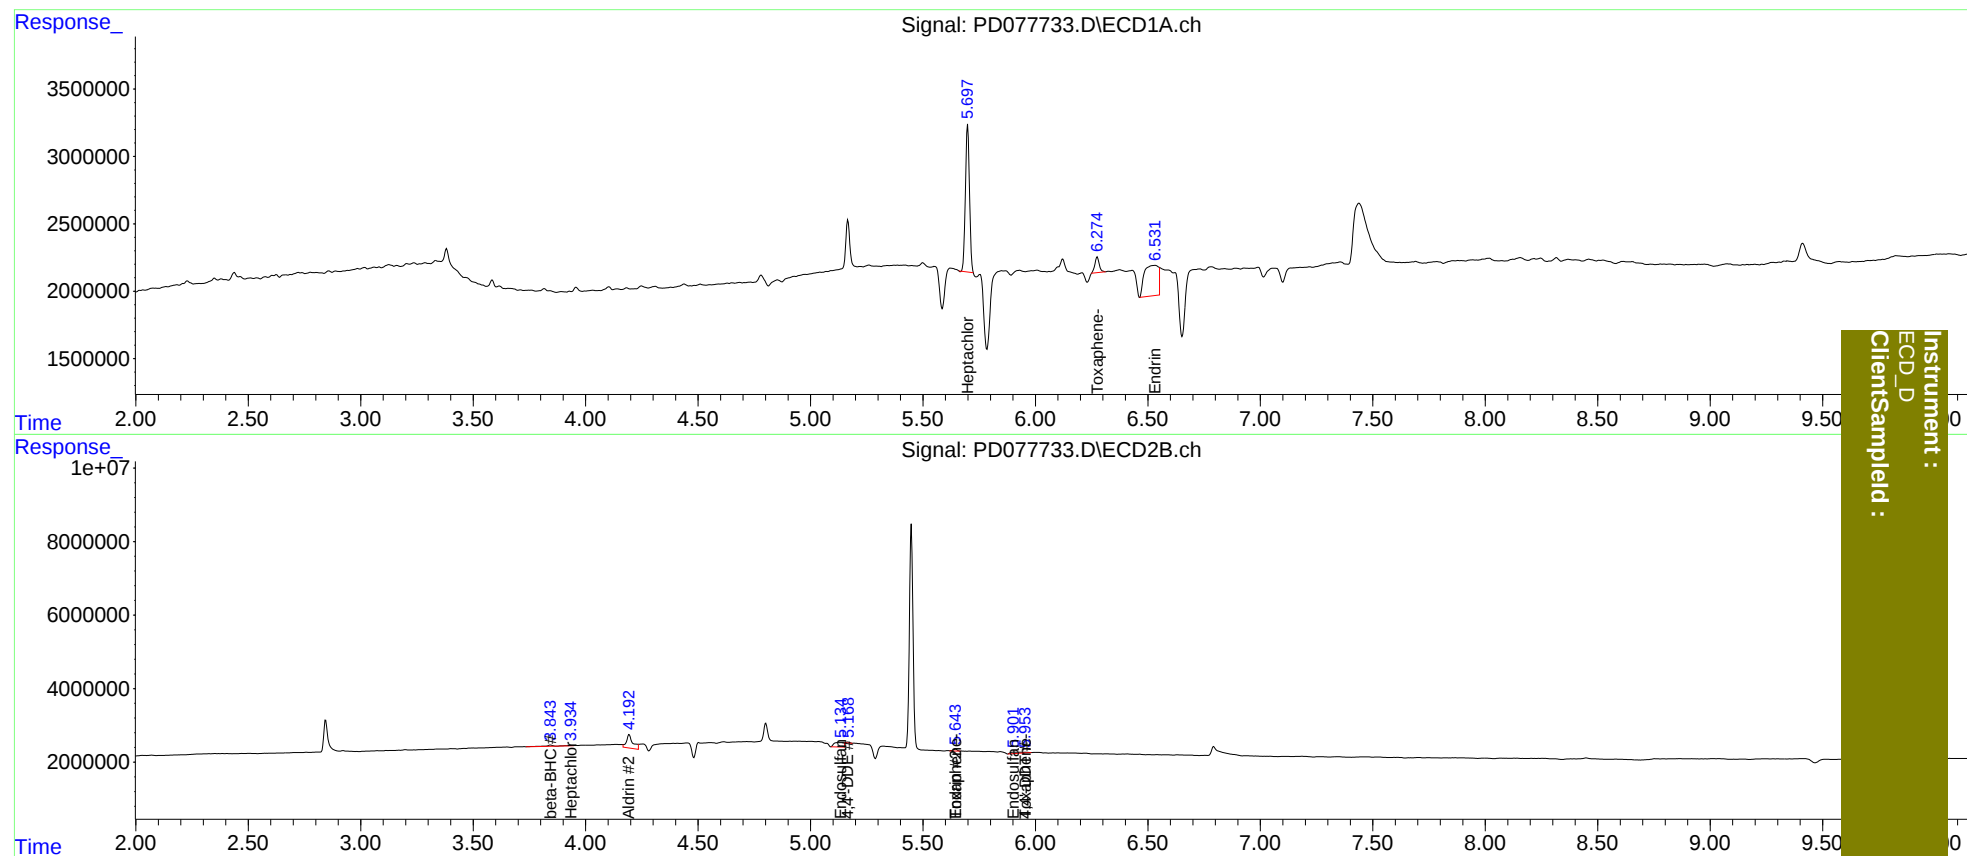


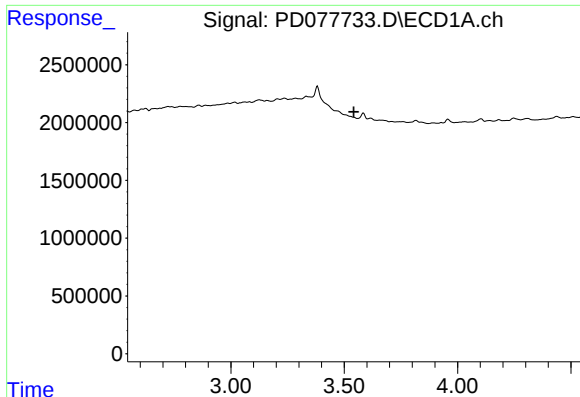

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

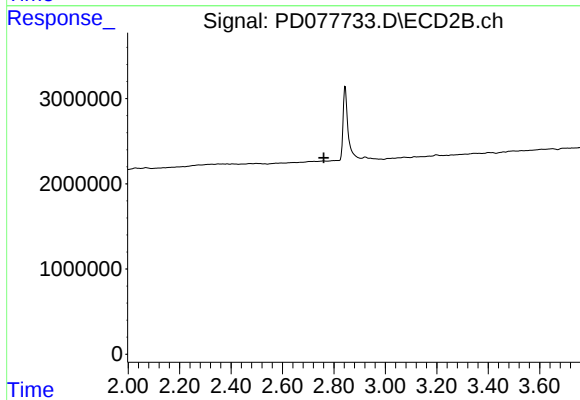


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.761 min
Response: 0
Conc: N.D.

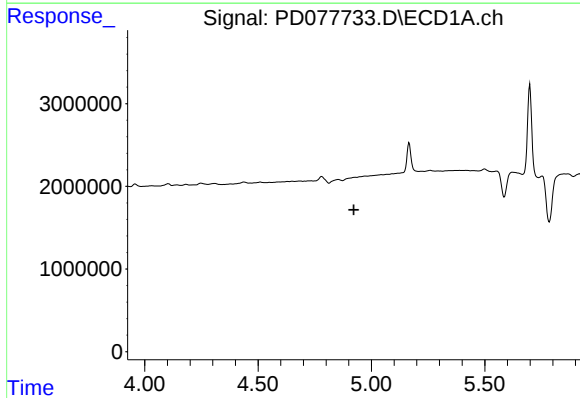


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.923 min
Response: 0
Conc: N.D.

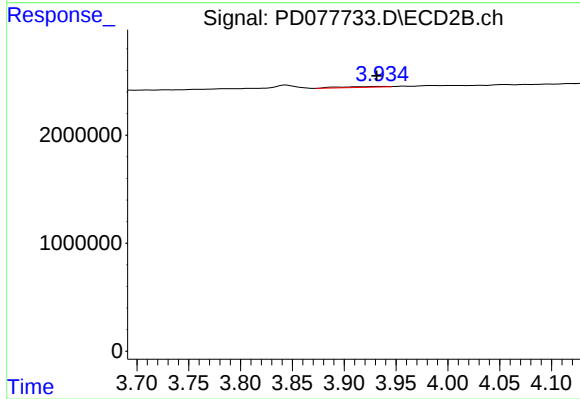

#4 Heptachlor


R.T.: 3.935 min
Delta R.T.: 0.004 min
Response: 256057
Conc: 0.12 ng/ml

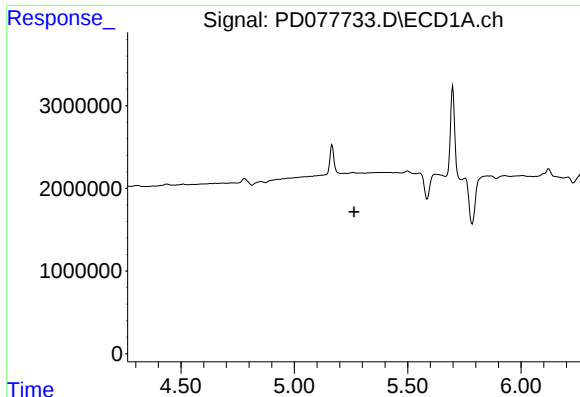

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

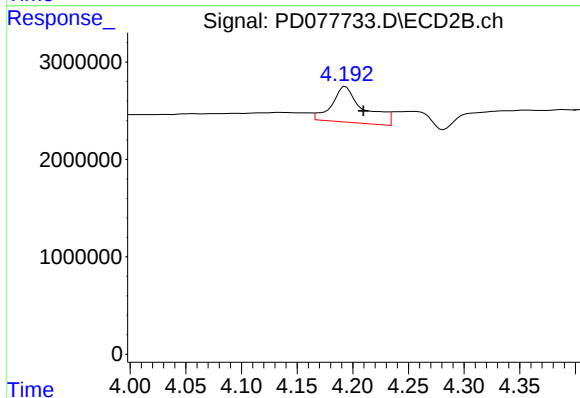


#5 Aldrin

R.T.: 4.194 min
Delta R.T.: -0.016 min
Response: 7322349
Conc: 3.27 ng/ml

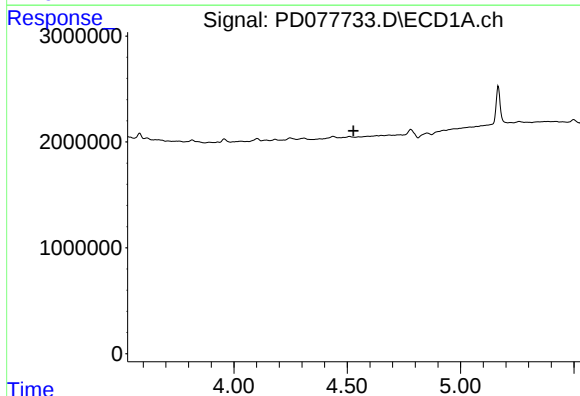


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.528 min
Response: 0
Conc: N.D.

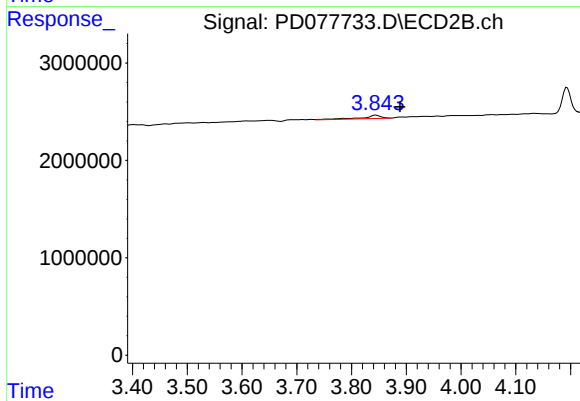

#6 beta-BHC


R.T.: 3.844 min
Delta R.T.: -0.044 min
Response: 849860
Conc: 0.86 ng/ml

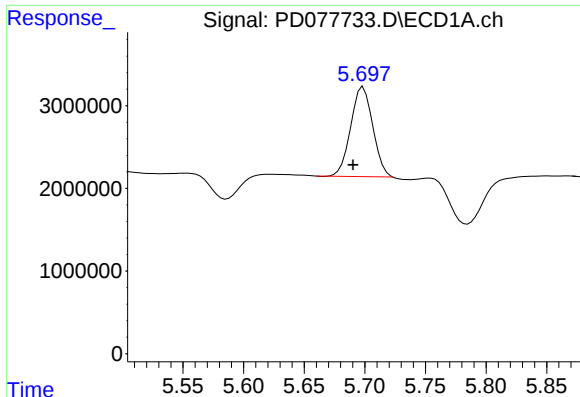

#8 Heptachlor epoxide


R.T.: 5.699 min
Delta R.T.: 0.008 min
Response: 13746379
Conc: 3.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

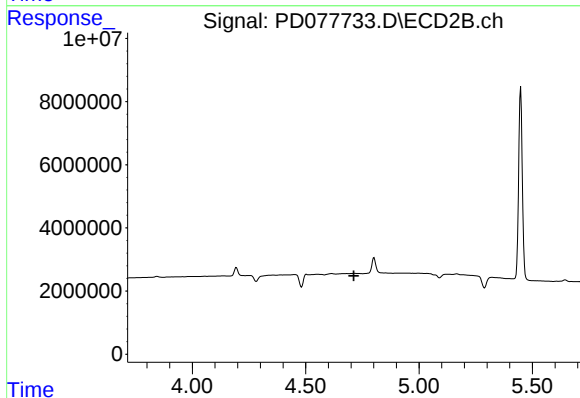


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.712 min
Response: 0
Conc: N.D.

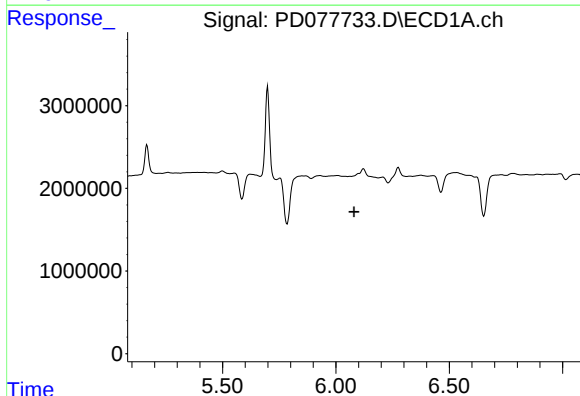


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.081 min
Response: 0
Conc: N.D.

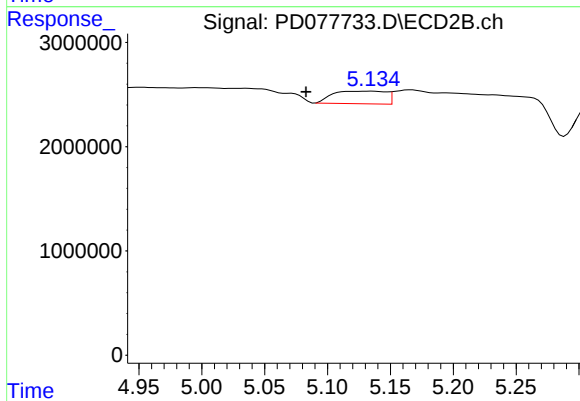

#9 Endosulfan I


R.T.: 5.134 min
Delta R.T.: 0.051 min
Response: 3512802
Conc: 1.96 ng/ml

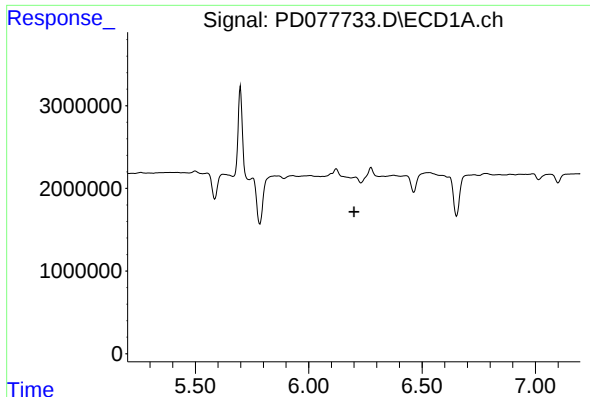

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.201 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

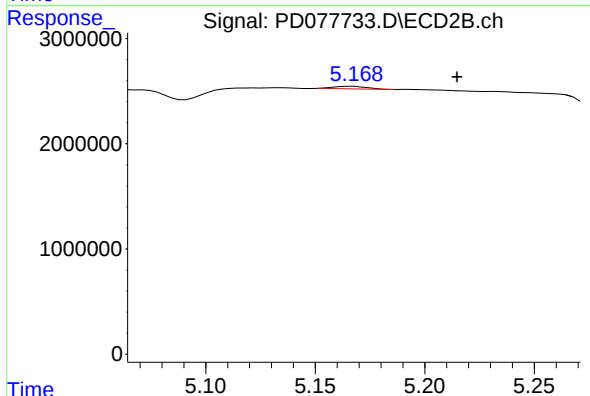


#12 4,4'-DDE

R.T.: 5.167 min
Delta R.T.: -0.048 min
Response: 249970
Conc: 0.13 ng/ml

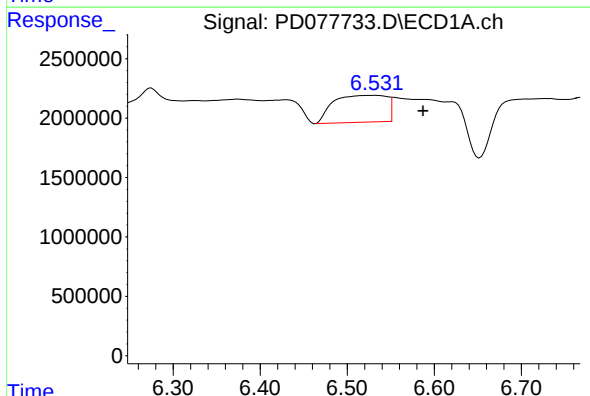


#14 Endrin

R.T.: 6.533 min
Delta R.T.: -0.055 min
Response: 9661385
Conc: 3.13 ng/ml

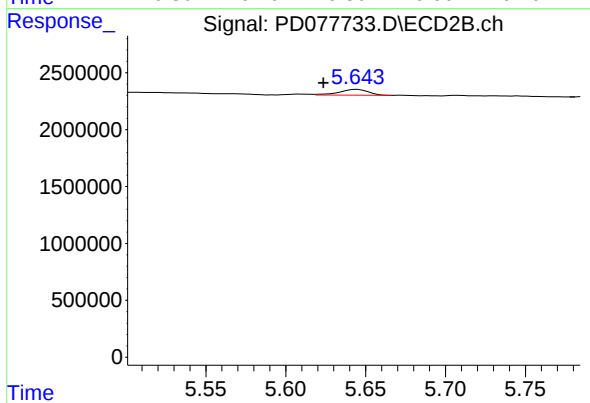

#14 Endrin


R.T.: 5.645 min
Delta R.T.: 0.021 min
Response: 651536
Conc: 0.36 ng/ml

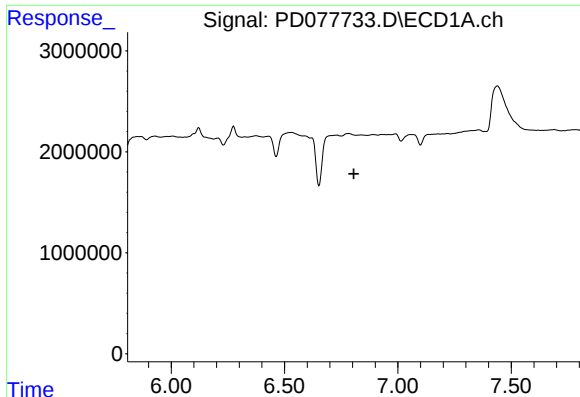

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

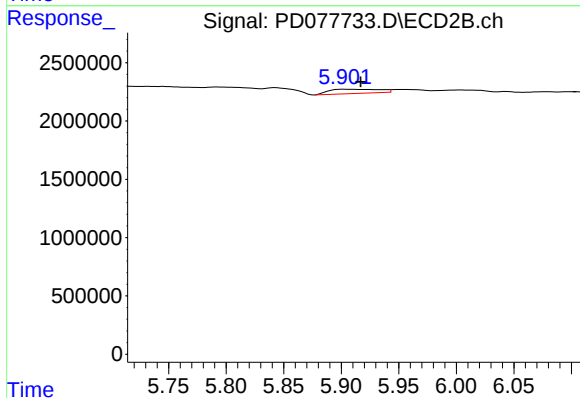


#15 Endosulfan II

R.T.: 5.903 min
Delta R.T.: -0.014 min
Response: 1114638
Conc: 0.62 ng/ml

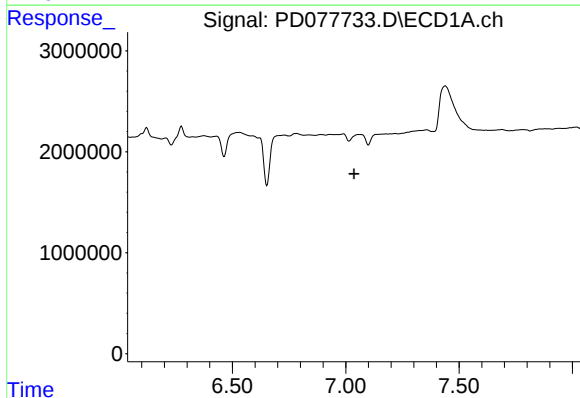


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 7.036 min
Response: 0
Conc: N.D.

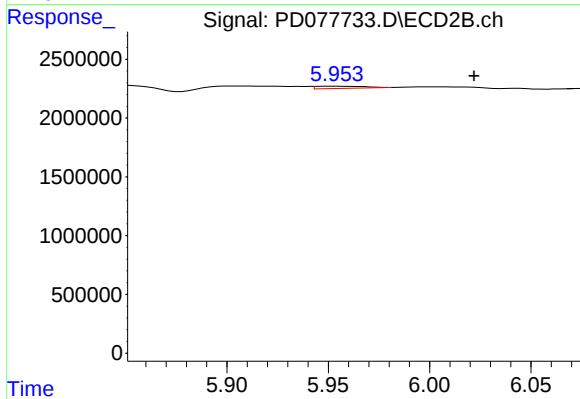

#17 4,4'-DDT


R.T.: 5.954 min
Delta R.T.: -0.068 min
Response: 318801
Conc: 0.23 ng/ml

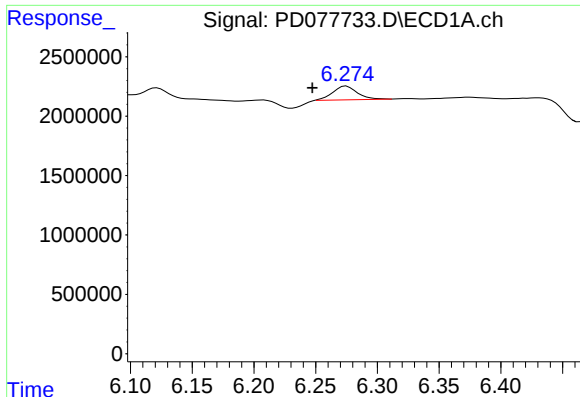

#22 Toxaphene-1


R.T.: 6.275 min
Delta R.T.: 0.027 min
Response: 1589430
Conc: 59.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

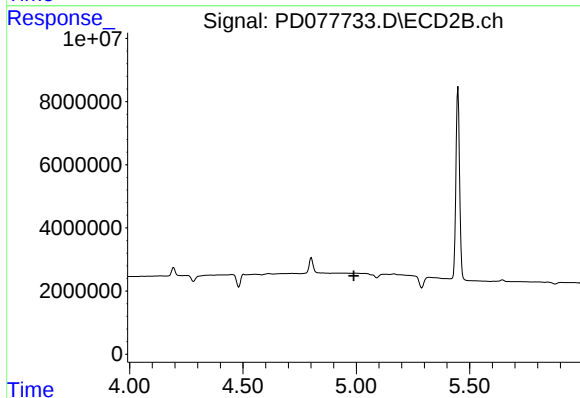


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

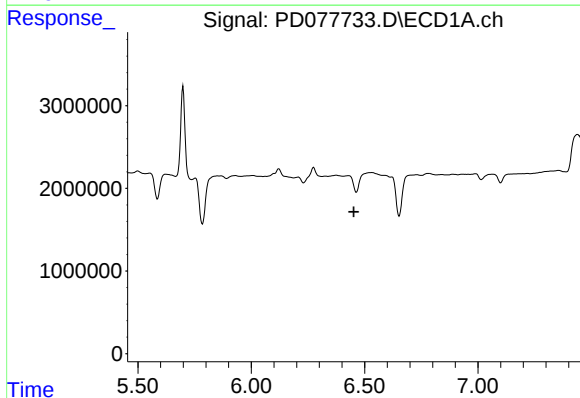


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 6.452 min
Response: 0
Conc: N.D.

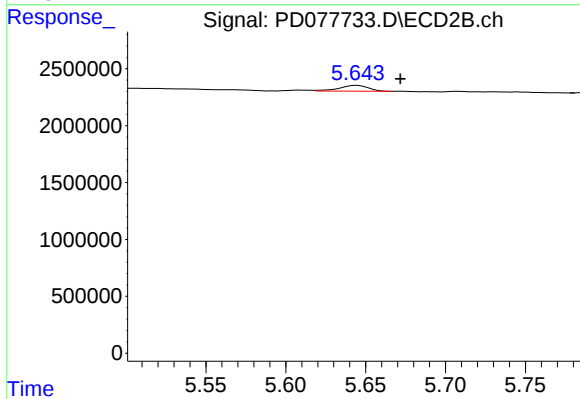

#23 Toxaphene-2


R.T.: 5.645 min
Delta R.T.: -0.027 min
Response: 651536
Conc: 54.03 ng/ml

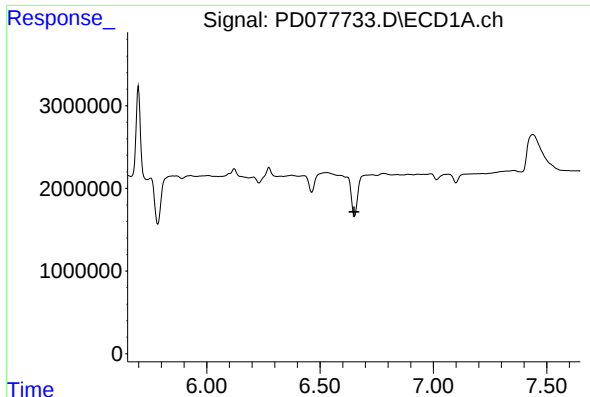

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 6.650 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

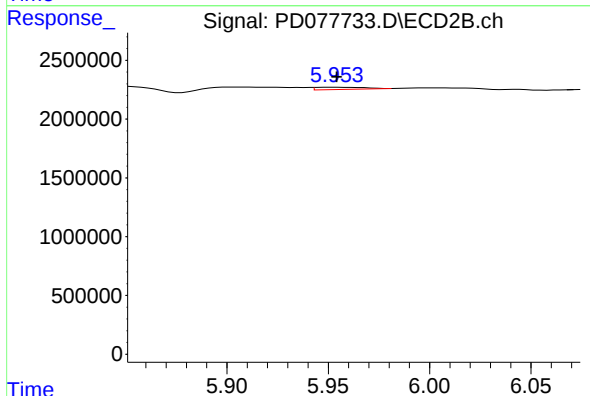


#24 Toxaphene-3

R.T.: 5.954 min
Delta R.T.: 0.000 min
Response: 318801
Conc: 23.38 ng/ml

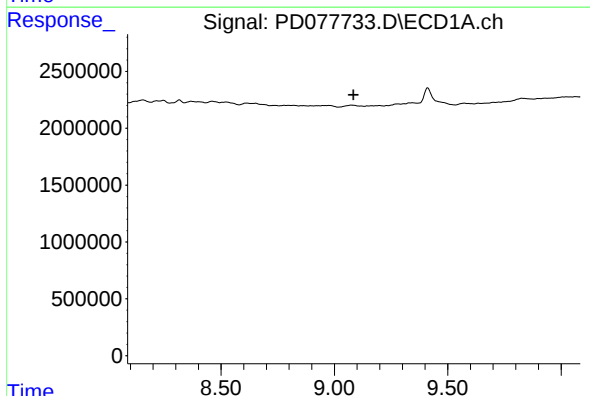

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.085 min
Response: 0
Conc: N.D.

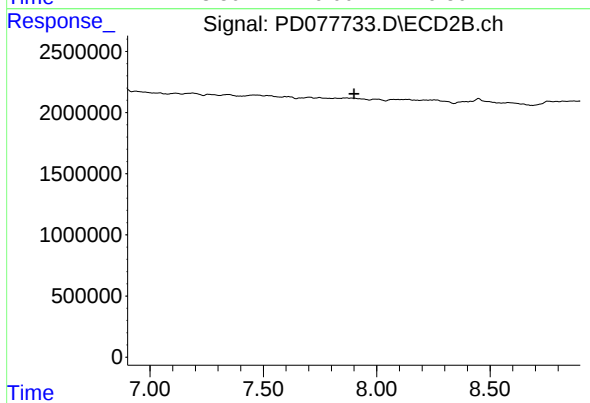

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.901 min
Response: 0
Conc: N.D.