

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090723\
 Data File : PD077734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2023 09:57
 Operator : AR\AJ
 Sample : PIBLK260
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 00:30:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.759	56294836	32468674	22.183	21.970
27)	SA Decachlor...	9.091	7.901	132.9E6	69054451	42.552	42.639
Target Compounds							
2)	A alpha-BHC	0.000	3.220f	0	40034	N.D.	<MDL
3)	MA gamma-BHC...	0.000	3.601	0	327193	N.D.	0.152
6)	B beta-BHC	0.000	3.846f	0	874489	N.D.	0.885
7)	B delta-BHC	4.774	0.000	2156695	0	0.537	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090723\
Data File : PD077734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2023 09:57
Operator : AR\AJ
Sample : PIBLK260
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 00:30:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

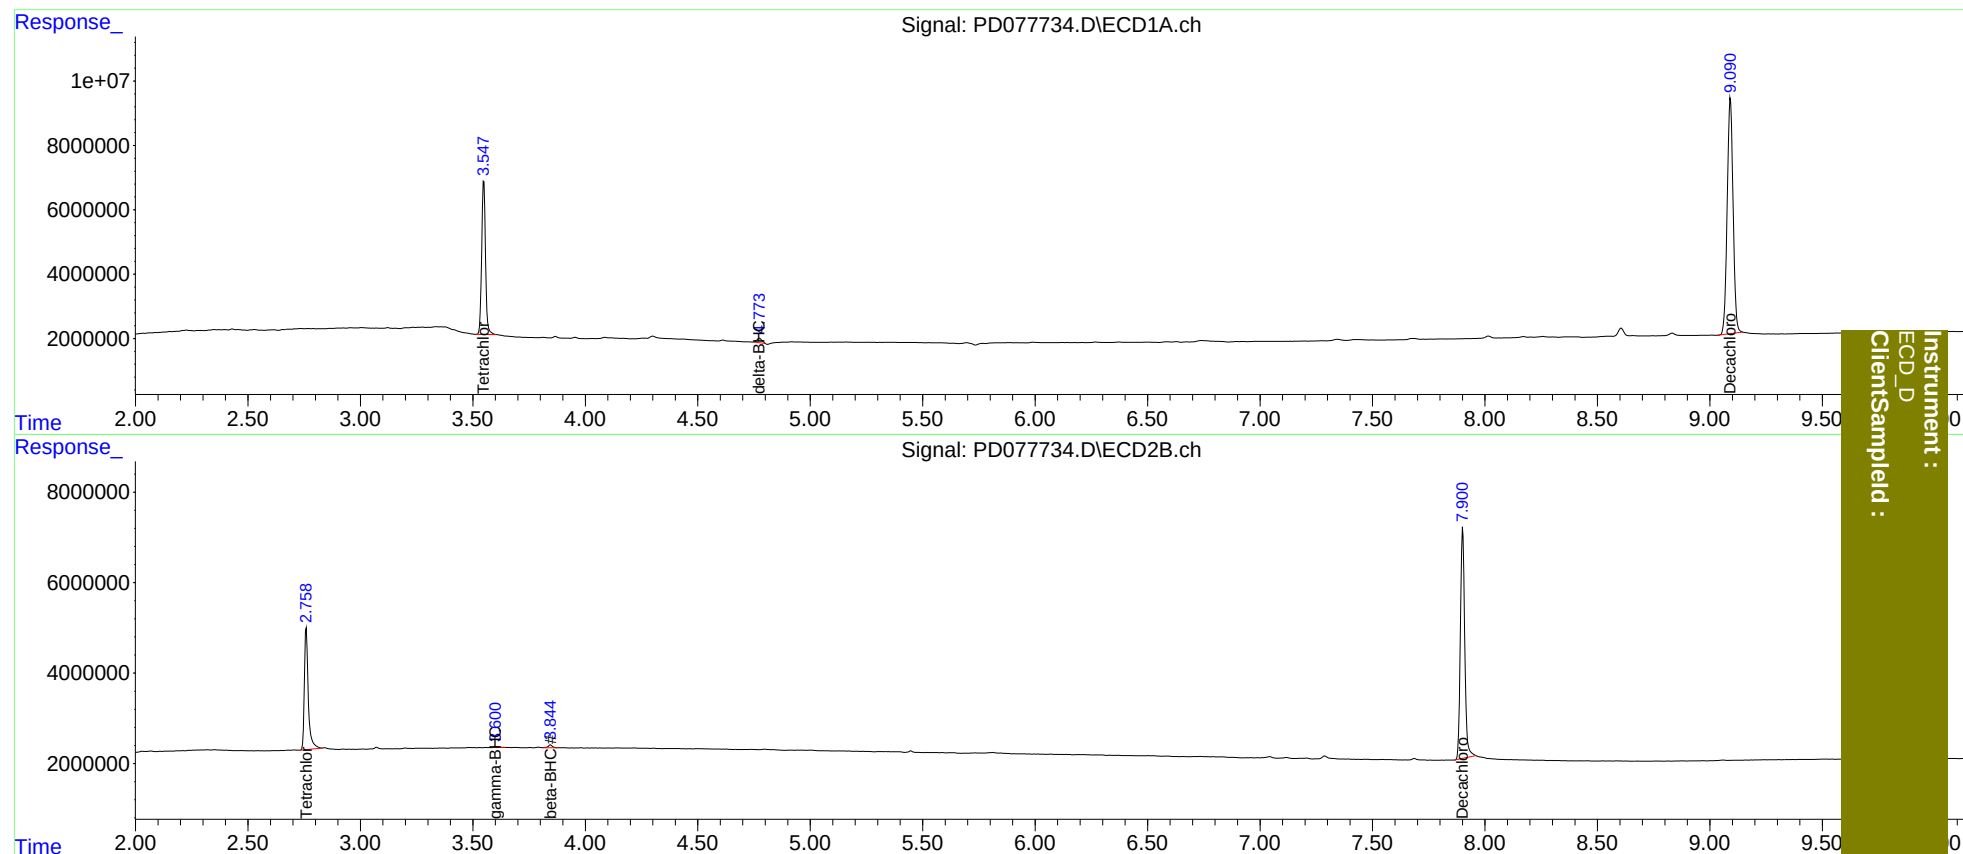


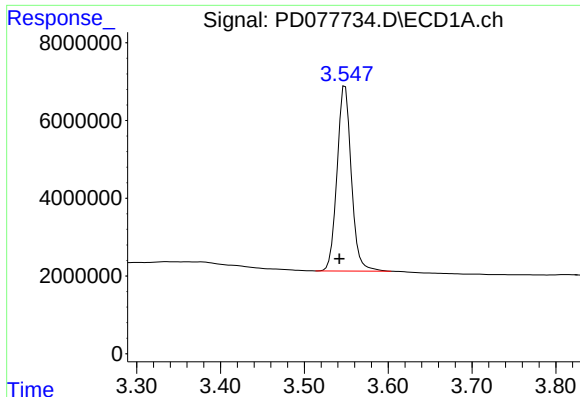

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.007 min
Response: 56294836
Conc: 22.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

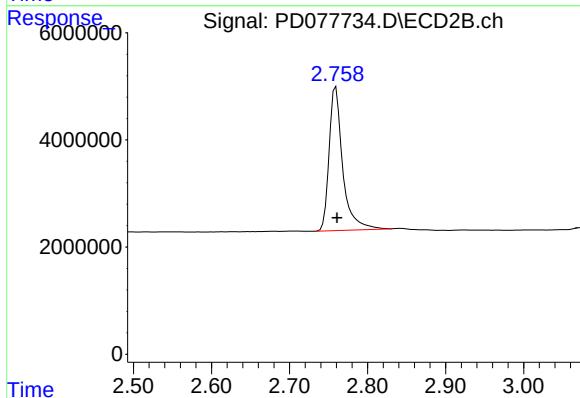


#1 Tetrachloro-m-xylene

R.T.: 2.759 min
Delta R.T.: -0.001 min
Response: 32468674
Conc: 21.97 ng/ml

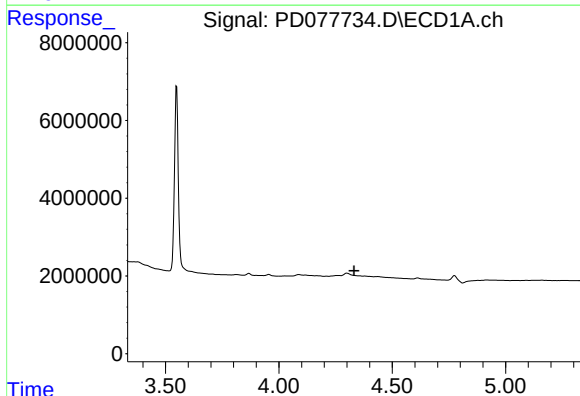


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.332 min
Response: 0
Conc: N.D.

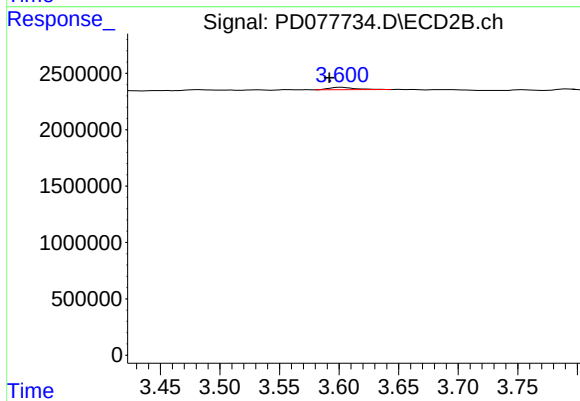

#3 gamma-BHC (Lindane)


R.T.: 3.601 min
Delta R.T.: 0.010 min
Response: 327193
Conc: 0.15 ng/ml

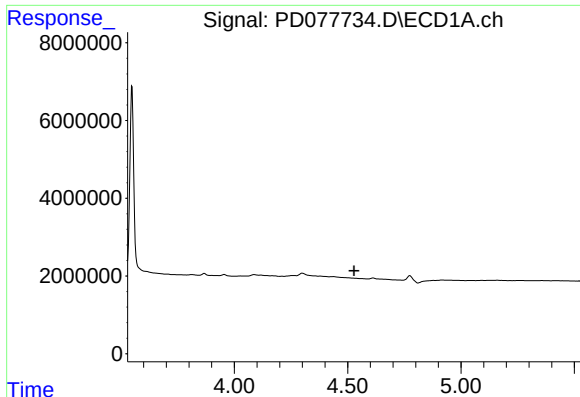

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

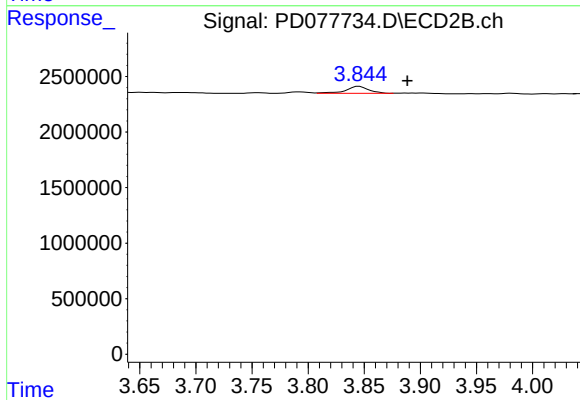


#6 beta-BHC

R.T.: 3.846 min
Delta R.T.: -0.043 min
Response: 874489
Conc: 0.89 ng/ml

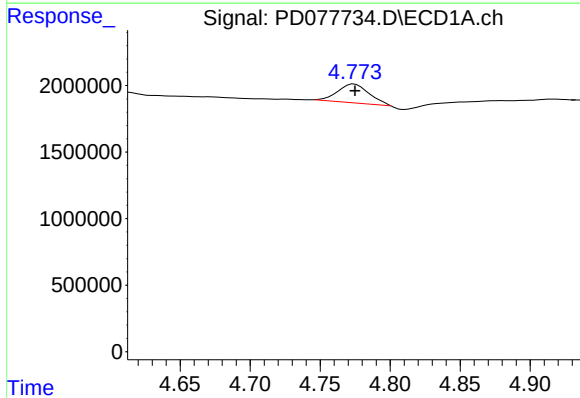


#7 delta-BHC

R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 2156695
Conc: 0.54 ng/ml

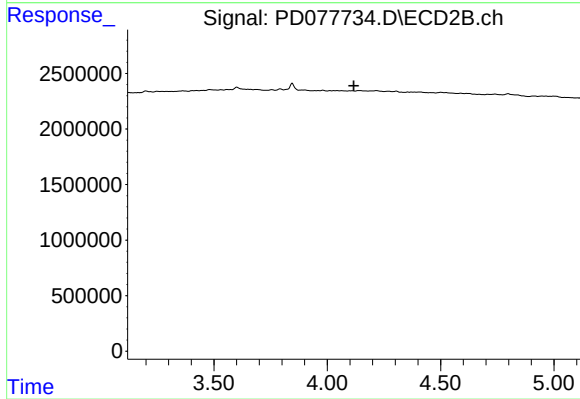

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.118 min
Response: 0
Conc: N.D.

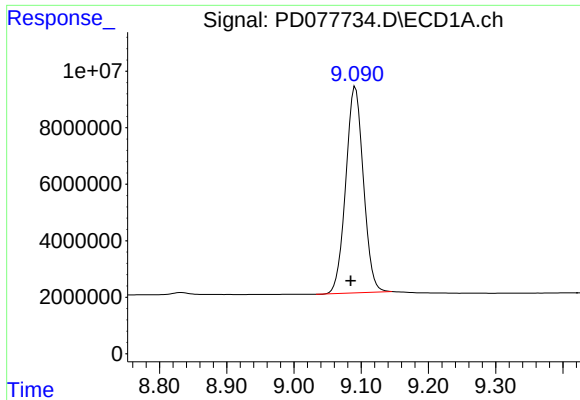

#27 Decachlorobiphenyl

R.T.: 9.091 min
Delta R.T.: 0.007 min
Response: 132929651
Conc: 42.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

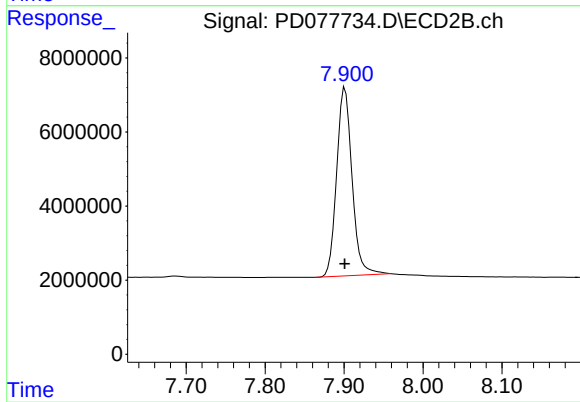

#27 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: 0.000 min
Response: 69054451
Conc: 42.64 ng/ml