

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090723\
 Data File : PD077744.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2023 12:36
 Operator : AR\AJ
 Sample : 04235-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYE0

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/08/2023
 Supervised By :Ankita Jodhani 09/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 00:32:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.760	26748685	18925716	10.541	12.806m
2)	SA Decachlor...	9.071	7.898	49033114	33326316	15.696	20.578 #
Target Compounds							
12)	B 4,4'-DDE	6.201	5.215	44991849	40428940	12.691	21.282 #
16)	A 4,4'-DDD	6.708	5.770	32249960	7214893	12.125	5.360m#
17)	MA 4,4'-DDT	7.035	6.019	32188784	19838514	11.749	14.036

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090723\
Data File : PD077744.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2023 12:36
Operator : AR\AJ
Sample : 04235-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 00:32:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

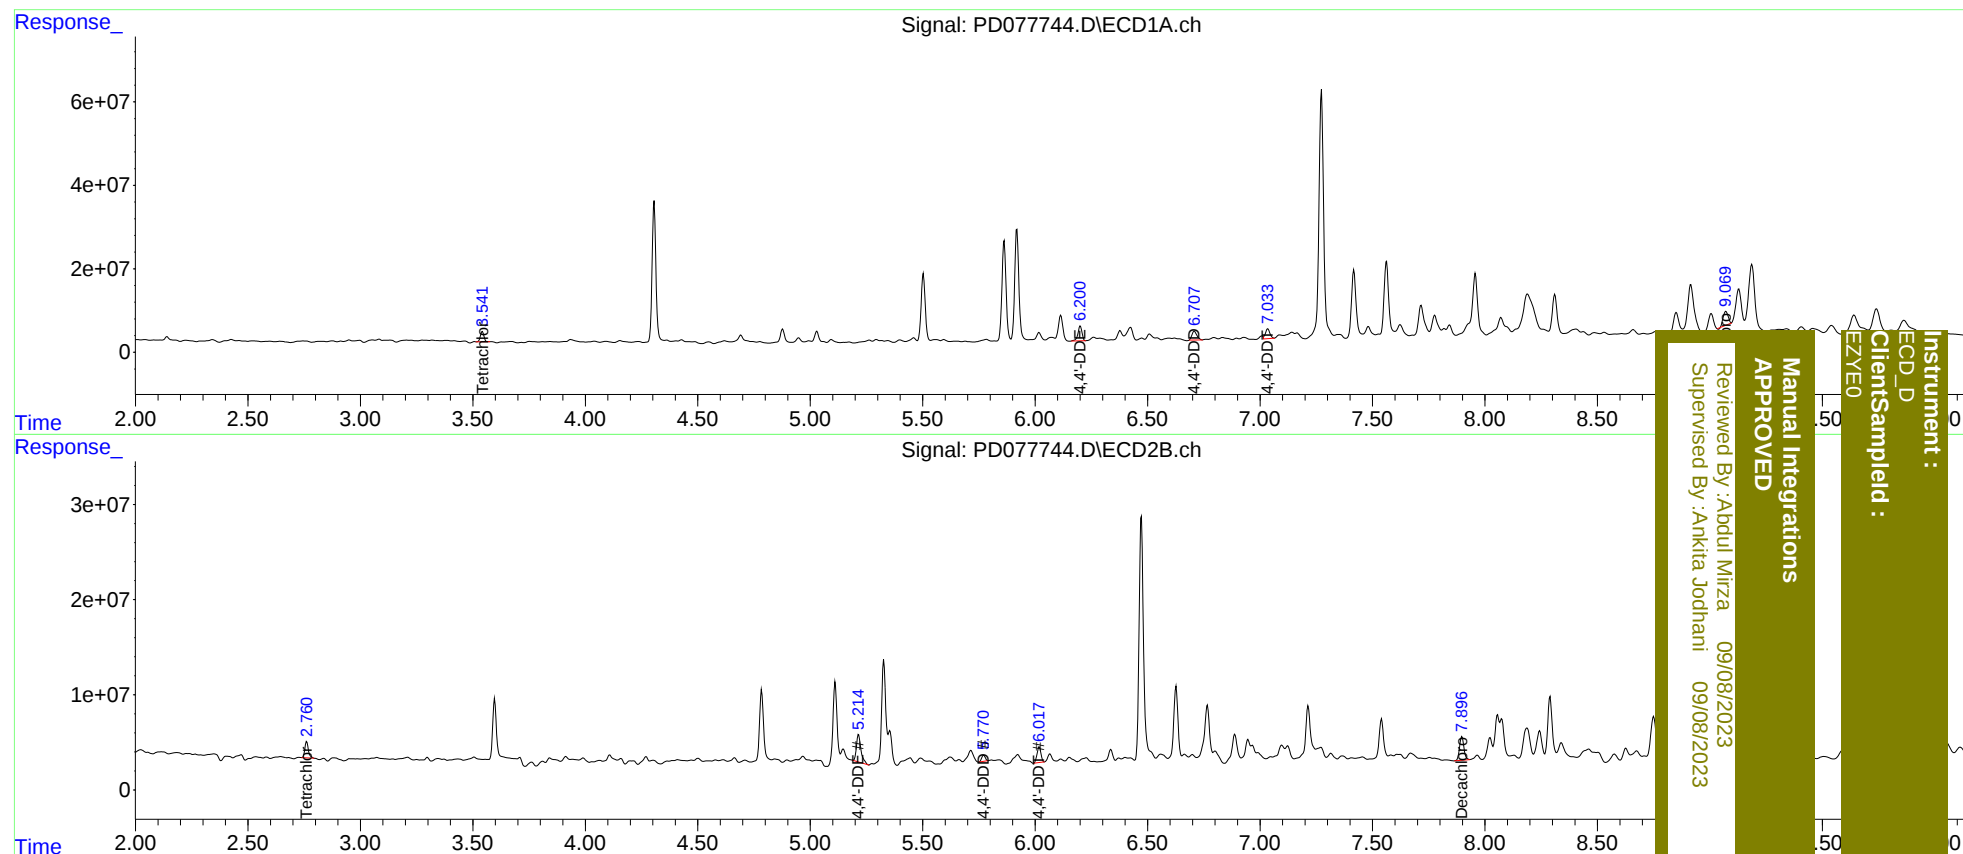

Instrument :
ECD_D
ClientSampled :
EZYE0

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/08/2023
Supervised By :Ankita Jodhani 09/08/2023