

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090723\
 Data File : PD077749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2023 13:43
 Operator : AR\AJ
 Sample : 04235-12MS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYW8MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/08/2023
 Supervised By :Ankita Jodhani 09/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 00:33:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.761	18261519	9784470	7.196	6.621
27)	SA Decachlor...	9.075	7.900	43463511	15750827	13.913	9.726 #
Target Compounds							
2)	A alpha-BHC	3.997	3.262	77251175	43064319	18.042m	18.999
3)	MA gamma-BHC...	4.331	3.593	77598100	62154347	19.192	28.787 #
4)	MA Heptachlor	4.921	3.930	72430359	67118545	17.333m	30.189 #
5)	MB Aldrin	5.264	4.210	83828550	50319449	20.080	22.450m
6)	B beta-BHC	4.529	3.889	28673098	18107580	15.607	18.326
7)	B delta-BHC	4.777	4.118	67395017	46105265	16.784	20.684
8)	B Heptachlo...	5.690	4.712	116.8E6	33425903	30.216	15.914 #
9)	A Endosulfan I	6.080	5.083	55034813	28720629	16.395	16.001
10)	B trans-Chl...	5.947	4.961	64049248	27088241	17.202m	13.565m
11)	B cis-Chlor...	6.029	5.027	67458220	30632887	17.503	14.979
12)	B 4,4'-DDE	6.202	5.215	600.1E6	278.2E6	169.267	146.432
13)	MA Dieldrin	6.355	5.347	178.2E6	90184488	47.621	43.643m
14)	MA Endrin	6.586	5.623	135.7E6	63412150	43.970	34.683m
15)	B Endosulfa...	6.805	5.917	141.8E6	67586487	42.825	37.347
16)	A 4,4'-DDD	6.723	5.770	225.8E6	48552758	84.897m	36.073 #
17)	MA 4,4'-DDT	7.036	6.019	141.9E6	113.2E6	51.783	80.058 #
18)	B Endrin al...	6.937	6.096	95357637	40621409	36.697	28.878m
19)	B Endosulfa...	7.170	6.318	122.0E6	99431764	40.263m	60.180 #
20)	A Methoxychlor	7.511	6.597	313.3E6	147.5E6	200.888	188.989
21)	B Endrin ke...	7.658	6.825	117.4E6	61602584	34.106	32.152m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090723\
Data File : PD077749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2023 13:43
Operator : AR\AJ
Sample : 04235-12MS
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 00:33:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

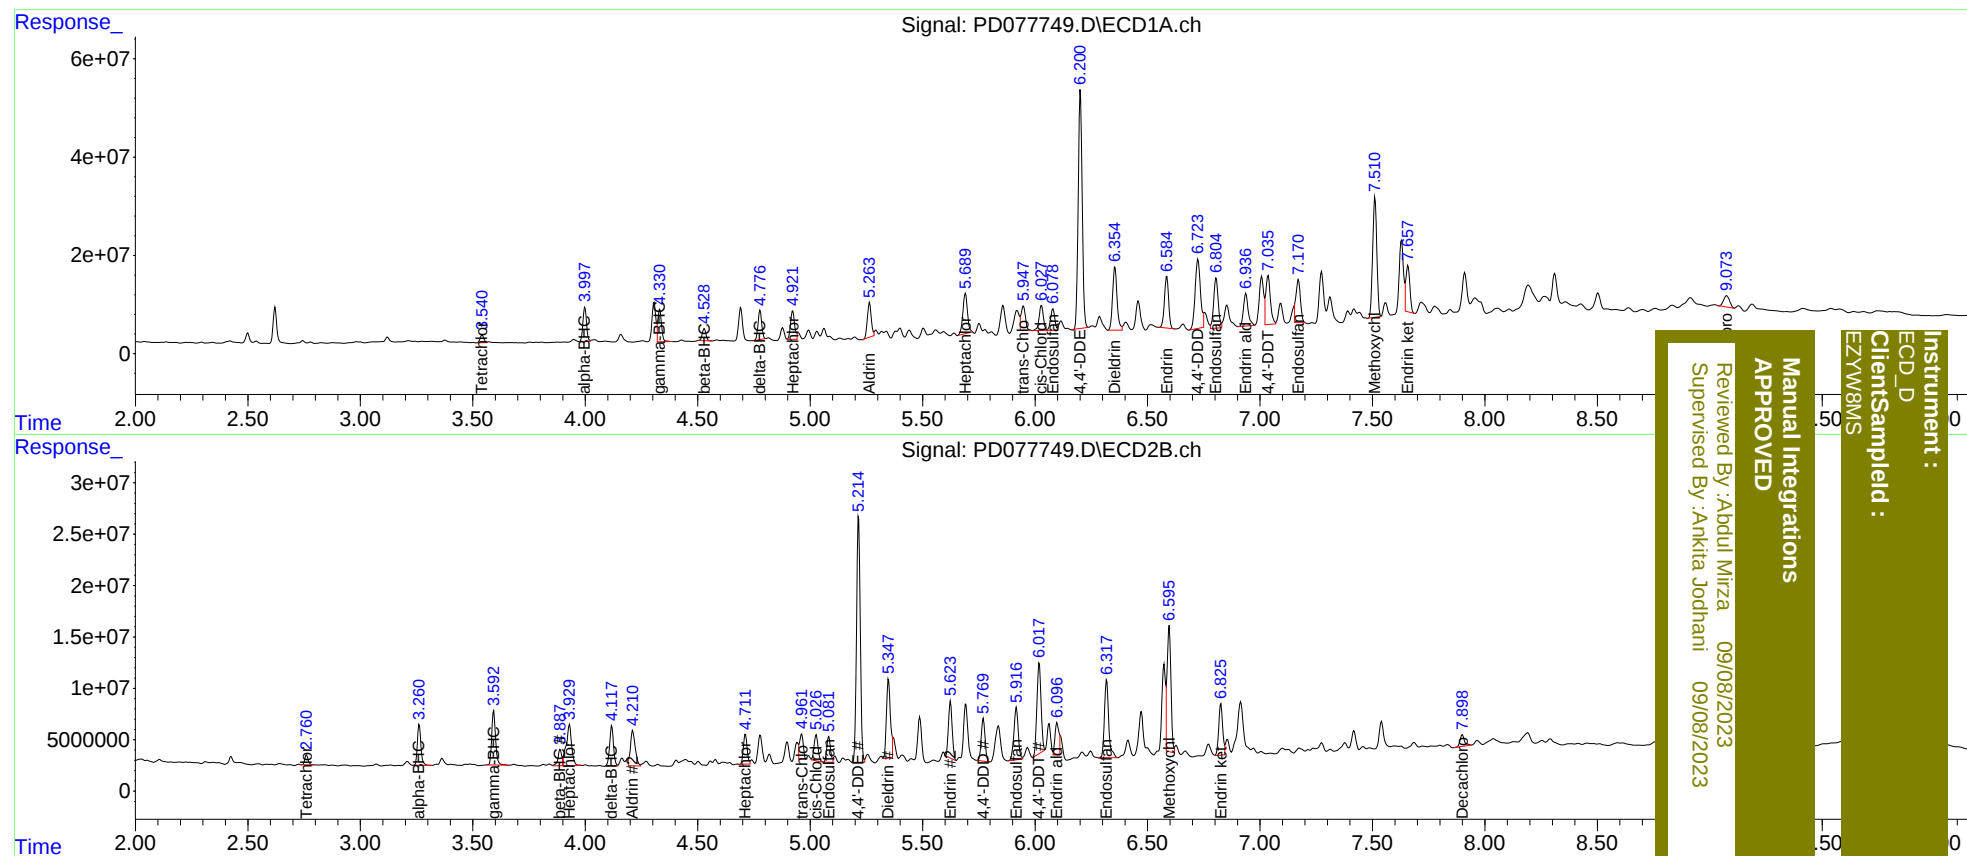

Instrument :
ECD_D
ClientSampled :
EZVW/BMS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 09/08/2023
Supervised By: Ankita Jodhani 09/08/2023