

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090723\
 Data File : PD077746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Sep 2023 13:03
 Operator : AR\AJ
 Sample : 04235-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYK0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/08/2023
 Supervised By : Ankita Jodhani 09/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 00:33:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	2.762	26610155	21916844	10.486	14.830 #
27)	SA Decachlor...	9.075	7.898	77015578	33005202	24.654	20.380
Target Compounds							
15)	B Endosulfa...	6.798	5.910	27988541	16091804	8.453	8.892
17)	MA 4,4'-DDT	7.005	6.015	101.2E6	69048034	36.924m	48.854 #
19)	B Endosulfa...	7.145	6.314	72058666	50800890	23.779m	30.747m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090723\
Data File : PD077746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Sep 2023 13:03
Operator : AR\AJ
Sample : 04235-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 00:33:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

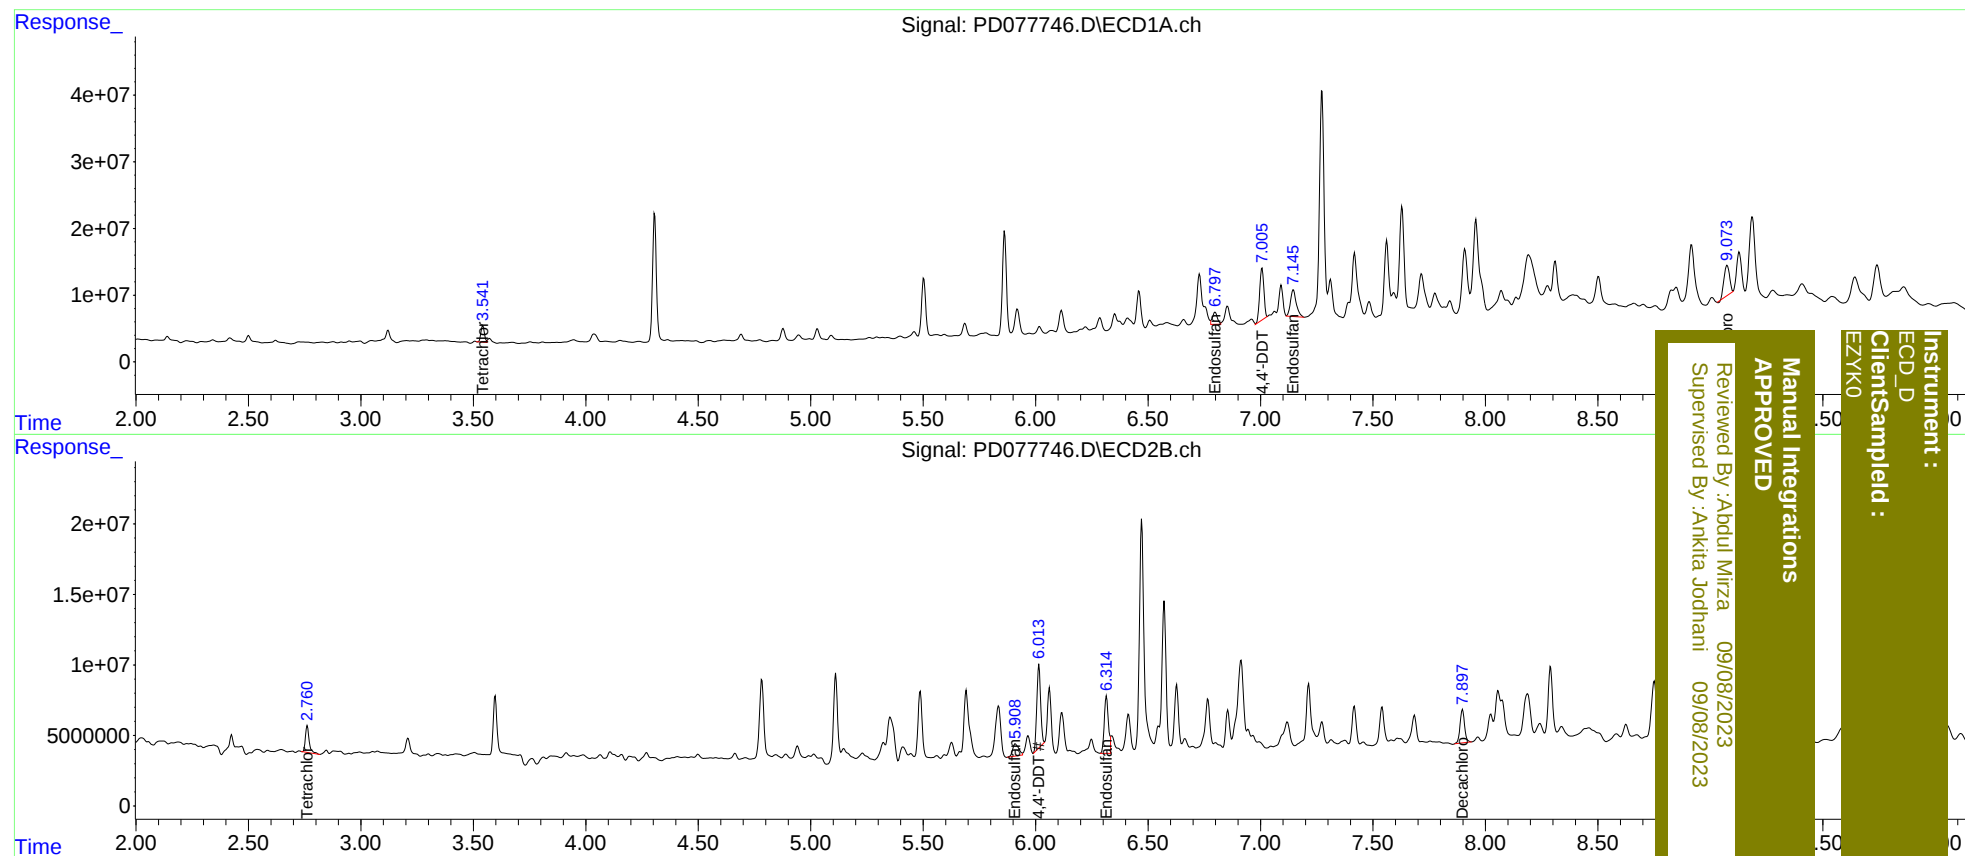

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/08/2023
Supervised By: Ankita Jodhani 09/08/2023

Instrument :
ECD_D
ClientSampled :
EZYK0