

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090820\
 Data File : PD059116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2020 11:26
 Operator : DD\AJ
 Sample : PIBLK02
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 01:38:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 05 02:06:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.206	3.864	19588914	32887032	19.433	20.068
27) SA Decachlor...	7.838	8.857	33012013	45728645	33.685	34.001
Target Compounds						
4) MA Heptachlor	0.000	4.985f	0	3987185	N.D.	1.893
8) B Heptachlo...	0.000	5.755f	0	659986	N.D.	0.329


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090820\
Data File : PD059116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2020 11:26
Operator : DD\AJ
Sample : PIBLK02
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 01:38:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 05 02:06:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

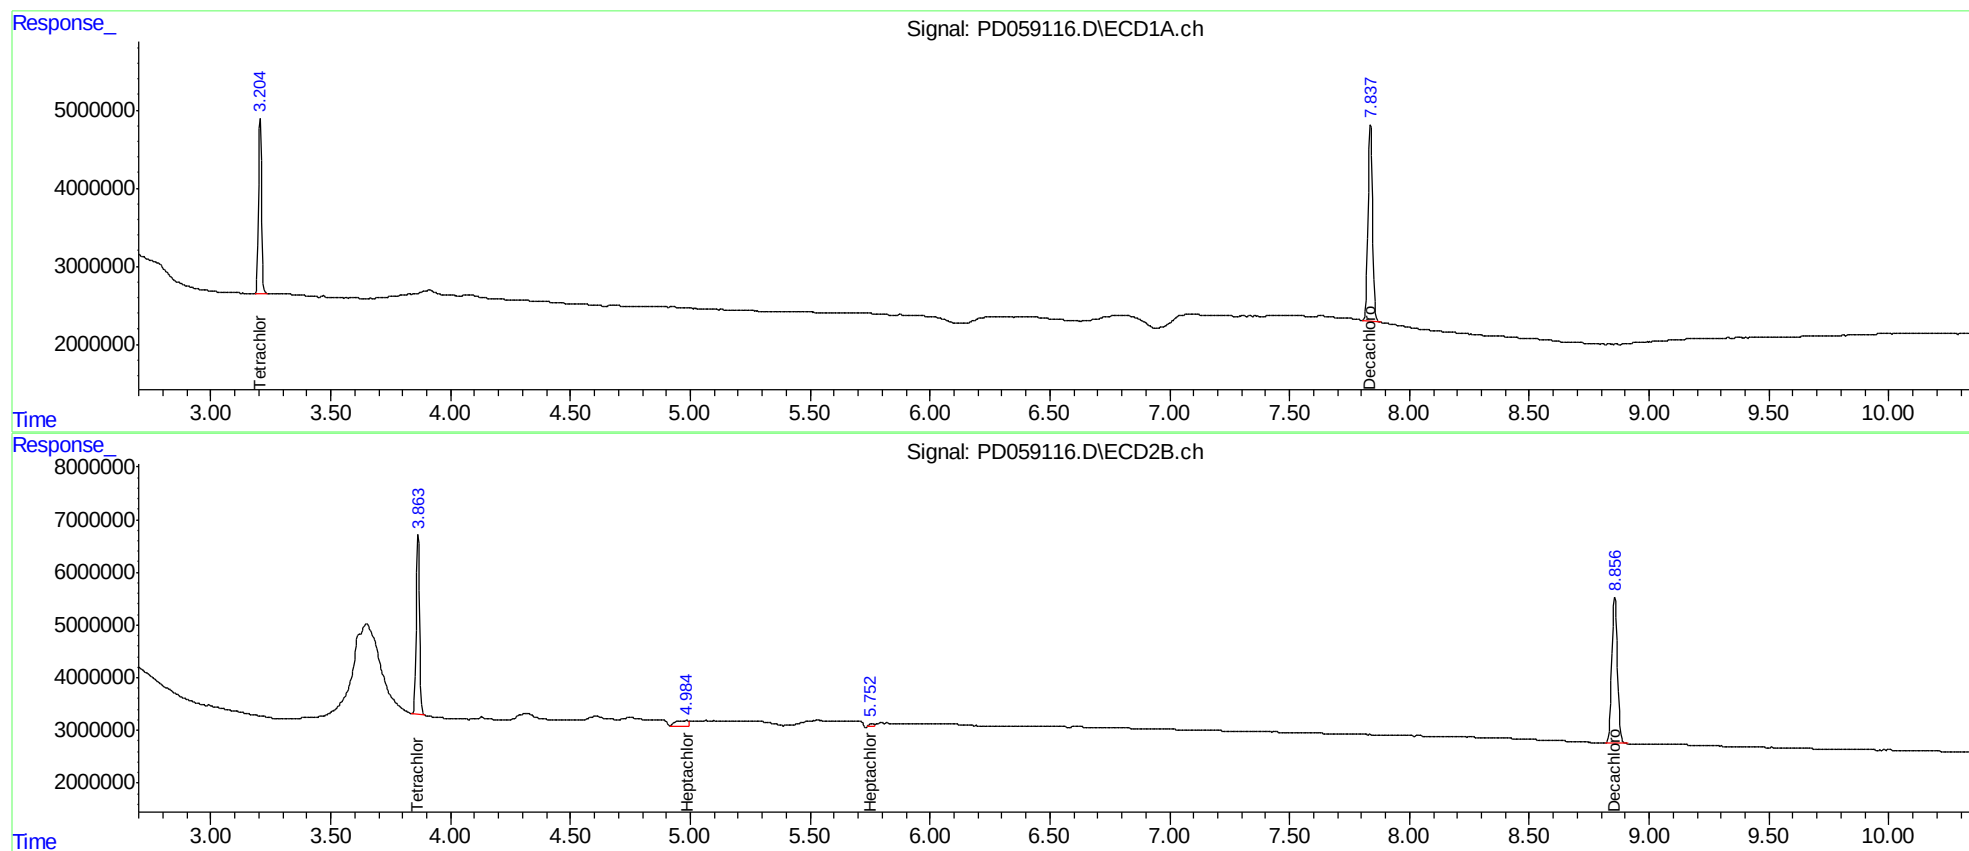


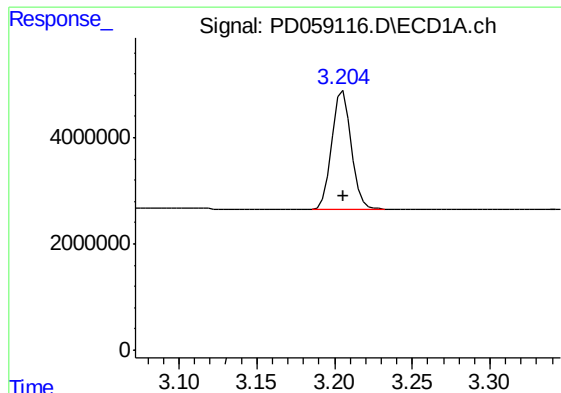

#1 Tetrachloro-m-xylene


R.T.: 3.206 min
Delta R.T.: 0.000 min
Response: 19588914
Conc: 19.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK06

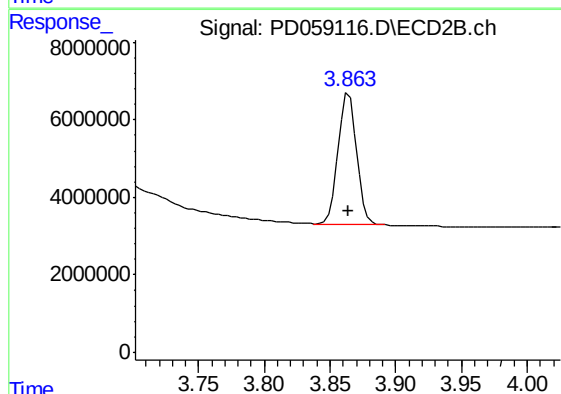


#1 Tetrachloro-m-xylene

R.T.: 3.864 min
Delta R.T.: 0.000 min
Response: 32887032
Conc: 20.07 ng/ml

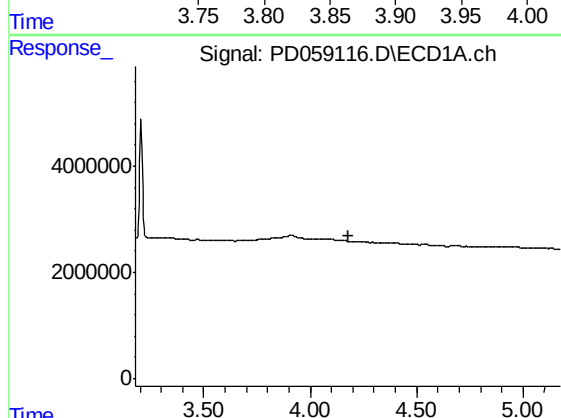


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.178 min
Response: 0
Conc: N.D.

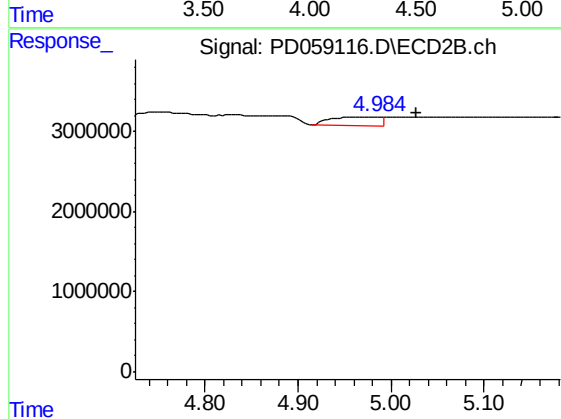

#4 Heptachlor


R.T.: 4.985 min
Delta R.T.: -0.042 min
Response: 3987185
Conc: 1.89 ng/ml

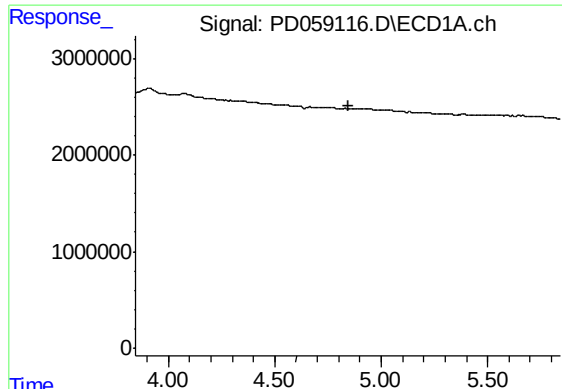

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.845 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK06

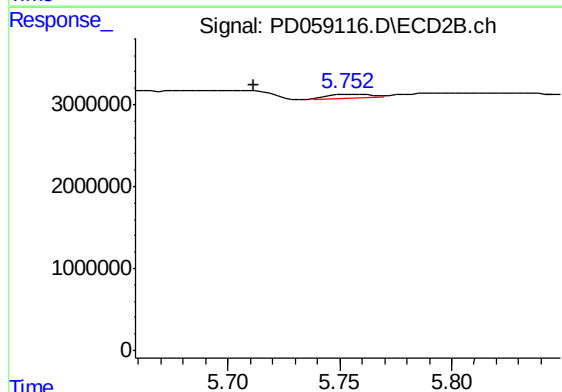


#8 Heptachlor epoxide

R.T.: 5.755 min
Delta R.T.: 0.044 min
Response: 659986
Conc: 0.33 ng/ml

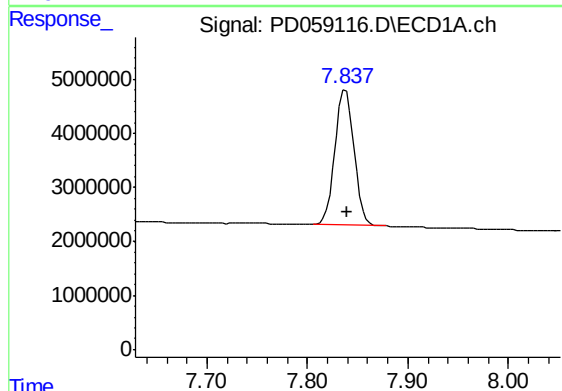

#27 Decachlorobiphenyl

R.T.: 7.838 min
Delta R.T.: -0.002 min
Response: 33012013
Conc: 33.68 ng/ml

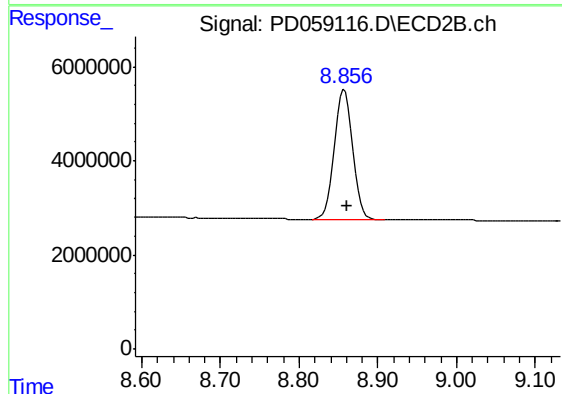

#27 Decachlorobiphenyl

R.T.: 8.857 min
Delta R.T.: -0.003 min
Response: 45728645
Conc: 34.00 ng/ml