

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090821\
 Data File : PD065623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2021 12:19
 Operator : AR\AJ
 Sample : M3640-03DL 2X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 HP-627DL

Manual Integrations
 APPROVED

mohammad
 9/9/2021 9:22:02 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 07:10:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 04 01:23:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.489	4.012	34172642	49106219	34.869m	6.700 #
28) SA Decachlor...	8.253	9.085	28654066	26019648	16.620m	4.876m#
Target Compounds						
11) B alpha-Chl...	5.485	6.189	104.8E6	75134562	69.647	10.202 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090821\
Data File : PD065623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2021 12:19
Operator : AR\AJ
Sample : M3640-03DL 2X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
HP-627DL


Manual Integrations
APPROVED

mohammad
9/9/2021 9:22:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 07:10:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Sat Sep 04 01:23:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

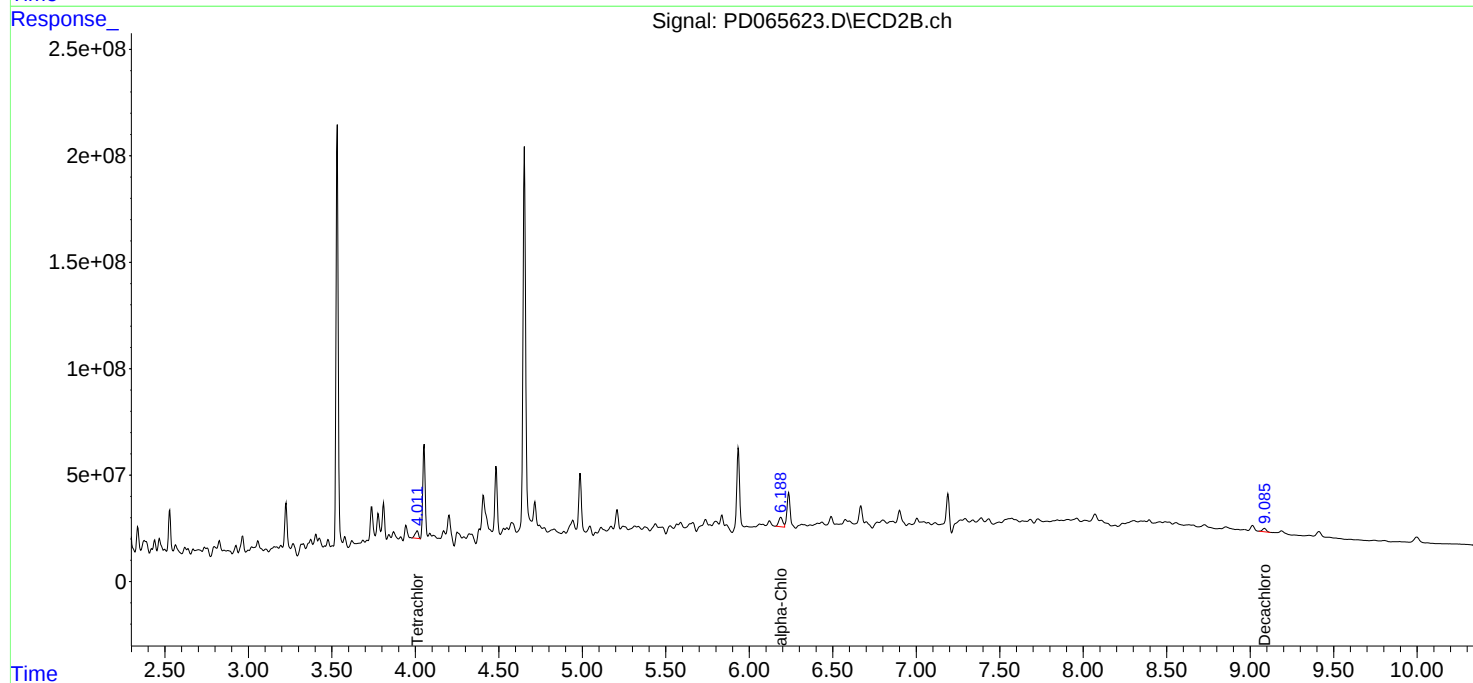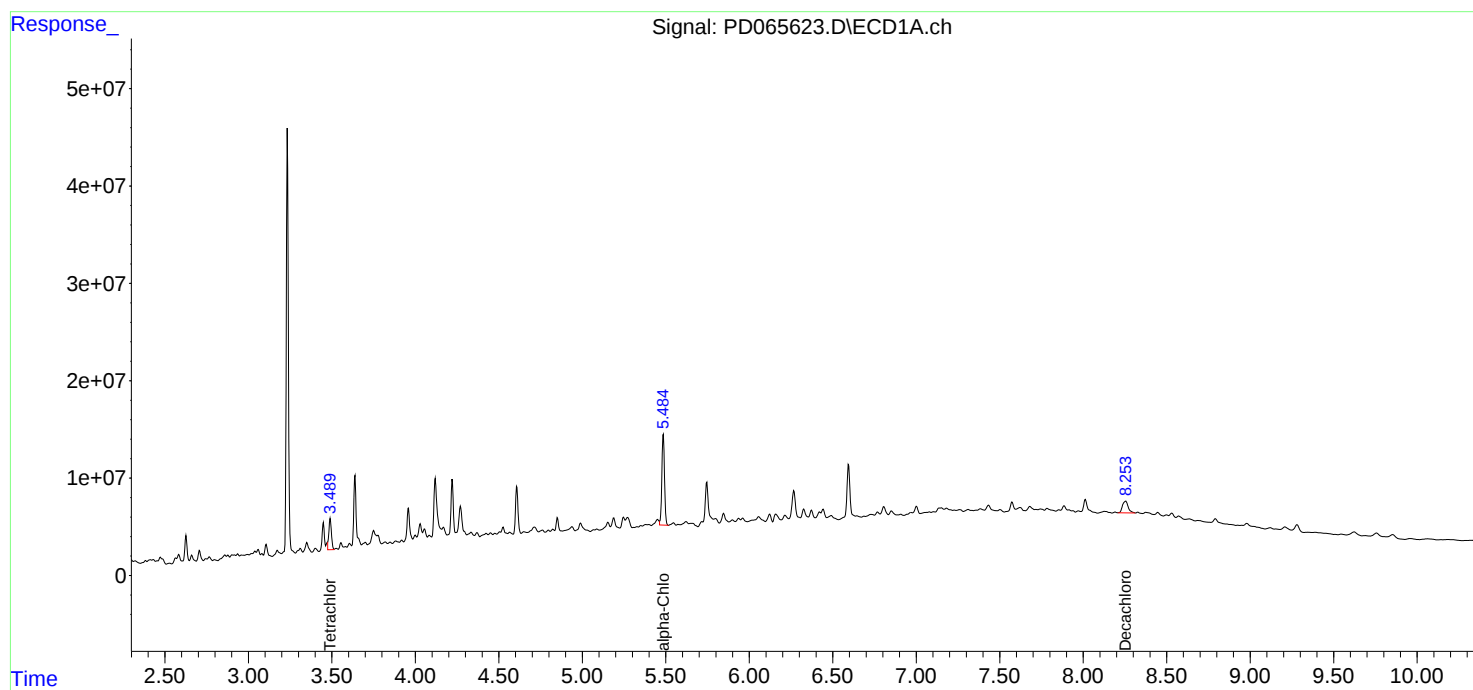

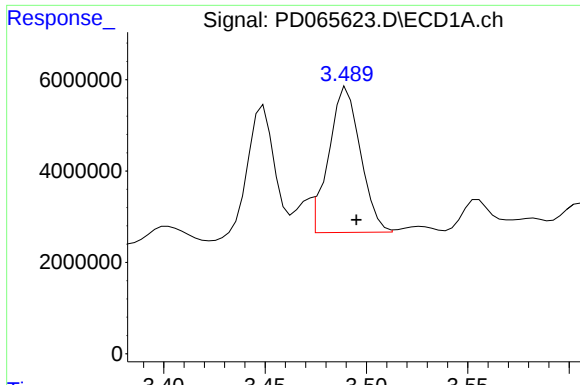


#1 Tetrachloro-m-xylene

R.T.: 3.489 min
Delta R.T.: -0.006 min
Response: 34172642
Conc: 34.87 ng/ml m

Instrument :
ECD_D
ClientSampleId :
HP-627DL


Manual Integrations
APPROVED

mohammad
9/9/2021 9:22:02 AM

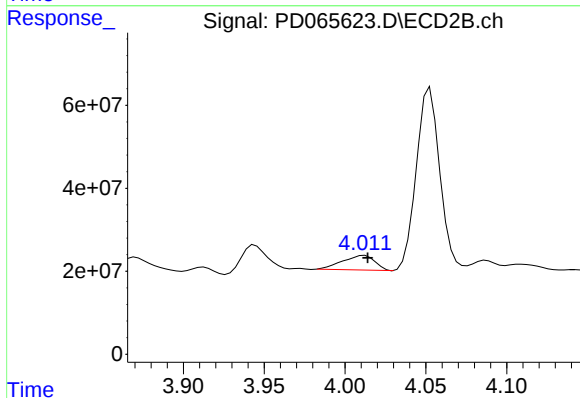


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: -0.002 min
Response: 49106219
Conc: 6.70 ng/ml

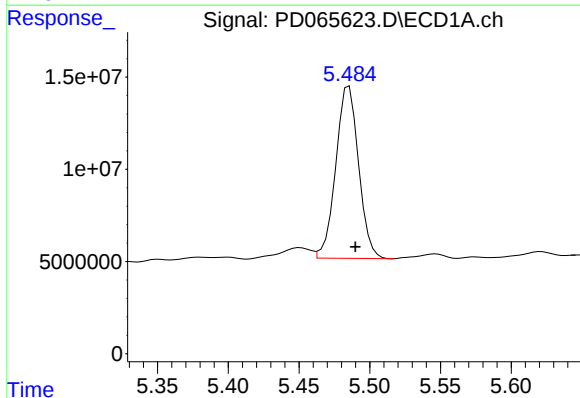


#11 alpha-Chlordane

R.T.: 5.485 min
Delta R.T.: -0.005 min
Response: 104843883
Conc: 69.65 ng/ml

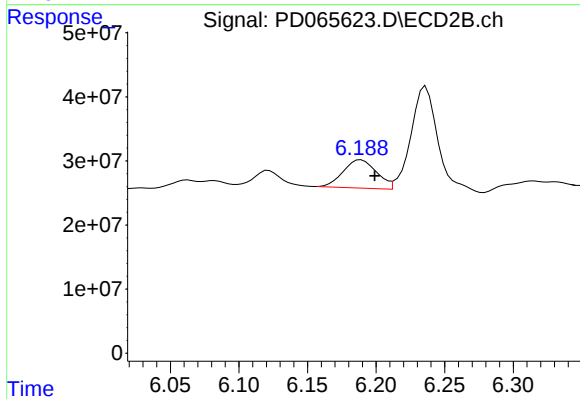

#11 alpha-Chlordane

R.T.: 6.189 min
Delta R.T.: -0.010 min
Response: 75134562
Conc: 10.20 ng/ml

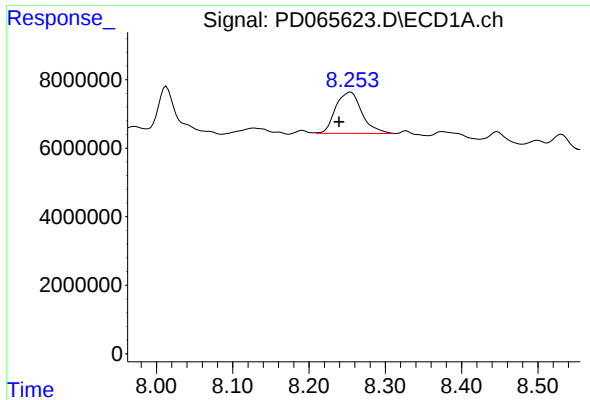


#28 Decachlorobiphenyl

R.T.: 8.253 min
Delta R.T.: 0.014 min
Response: 28654066
Conc: 16.62 ng/ml m

Instrument :
ECD_D
ClientSampleId :
HP-627DL

Manual Integrations
APPROVED

mohammad
9/9/2021 9:22:02 AM

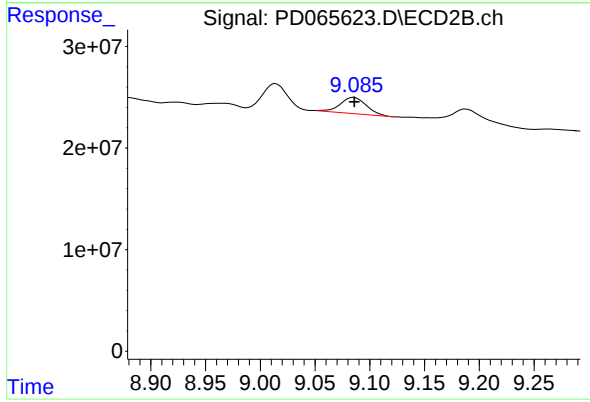

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: 0.000 min
Response: 26019648
Conc: 4.88 ng/ml m