

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090920\
 Data File : PD059127.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2020 11:57
 Operator : DD\AJ
 Sample : 50/100 MS-MSD TEST
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 50/100 MS-MSD TEST

Manual Integrations
 APPROVED

Ankita
 9/10/2020 1:09:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 02:00:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 05 02:06:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
3) MA	gamma-BHC...	3.904	4.529	61361079	100.7E6	38.741m 45.692
4) MA	Heptachlor	4.185	5.028	42853112	90438055	38.155 42.928
5) MB	Aldrin	4.420	5.328	53835586	87138850	41.360 42.226
13) MA	Dieldrin	5.416	6.320	85263239	164.2E6	75.763 88.684
14) MA	Endrin	5.667	6.536	68252119	128.5E6	73.639 79.728
17) MA	4,4'-DDT	6.039	6.962	68496516	126.4E6	80.784 86.182

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090920\
Data File : PD059127.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2020 11:57
Operator : DD\AJ
Sample : 50/100 MS-MSD TEST
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 02:00:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 05 02:06:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

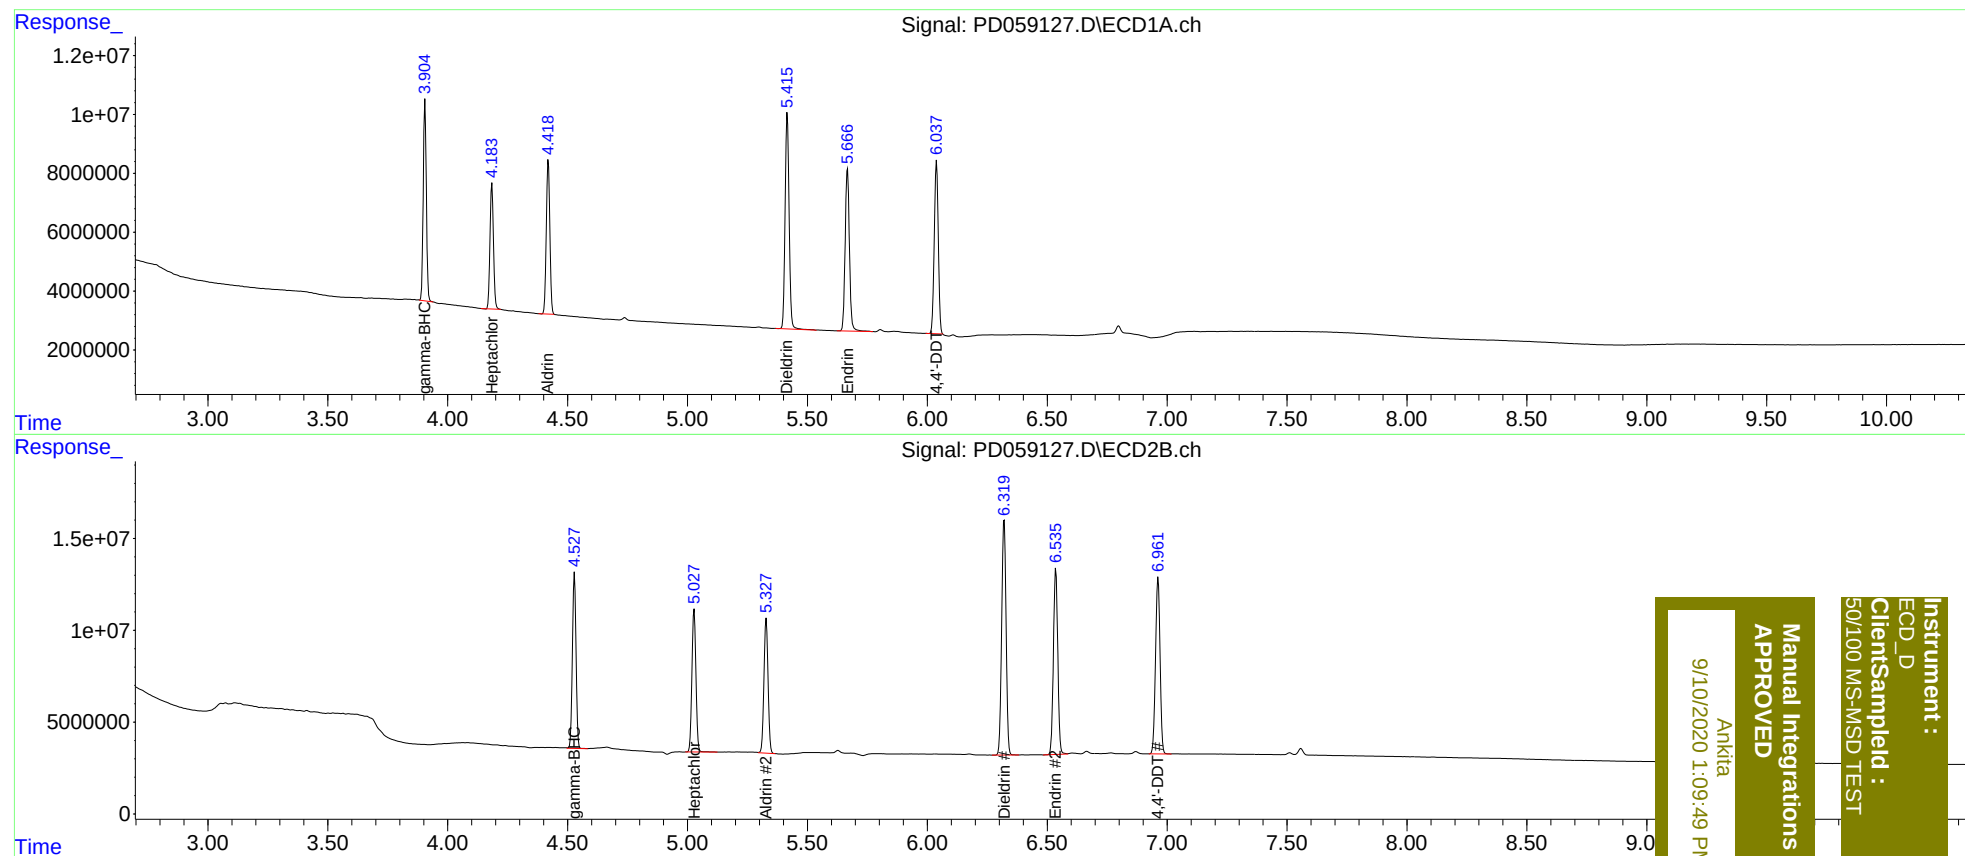

Manual Integrations
APPROVED

Ankita
9/10/2020 1:09:49 PM

Instrument :
ECD_D
ClientSample :
50/100 MS-MSD TEST