

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090921\
 Data File : PD065628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2021 09:32
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:32:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 09 15:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.012	19942878	177.0E6	20.350	24.147
28)	SA Decachlor...	8.238	9.086	33690472	117.3E6	19.541	21.976
Target Compounds							
8)	B Heptachlo...	0.000	5.909f	0	738506	N.D.	0.103 #
15)	B Endosulfa...	0.000	6.948	0	717948	N.D.	0.112 #
23)	Chlordane-1	4.393f	0.000	2594443	0	62.744	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090921\
Data File : PD065628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2021 09:32
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:32:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 09 15:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

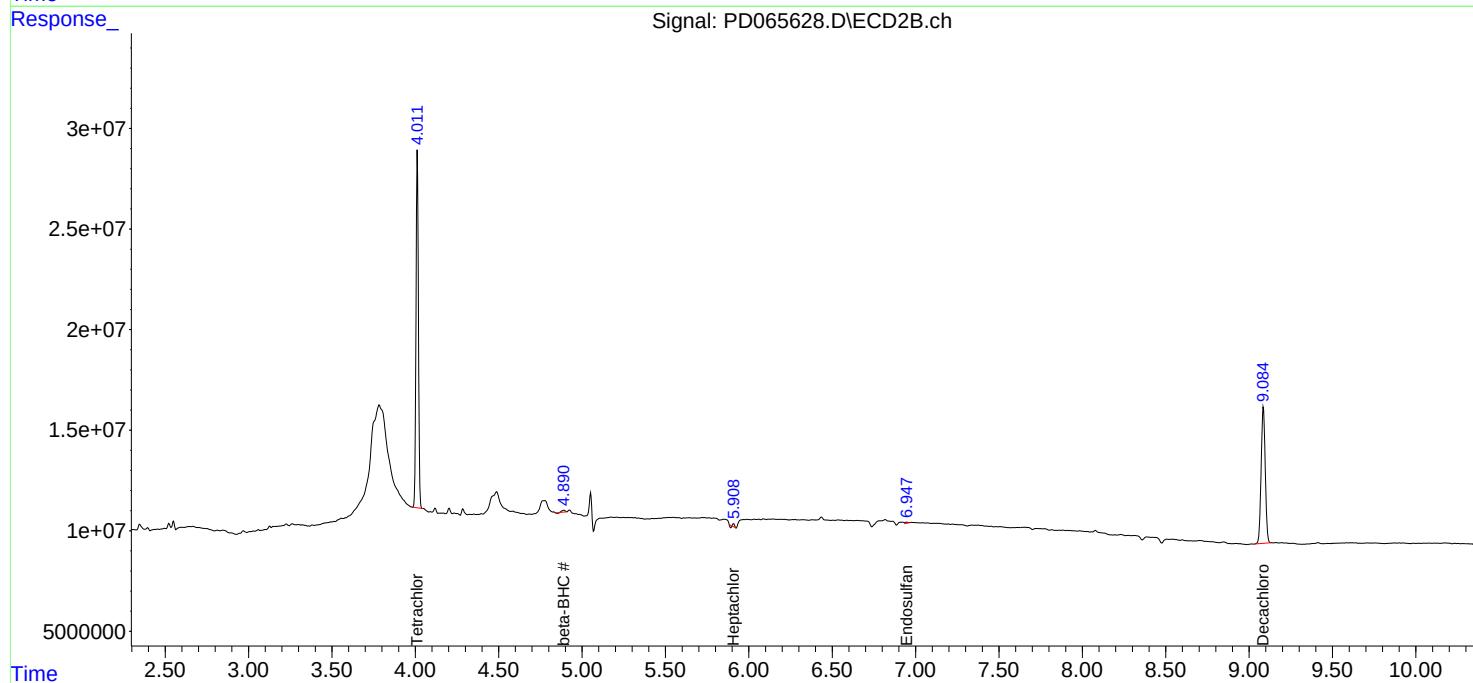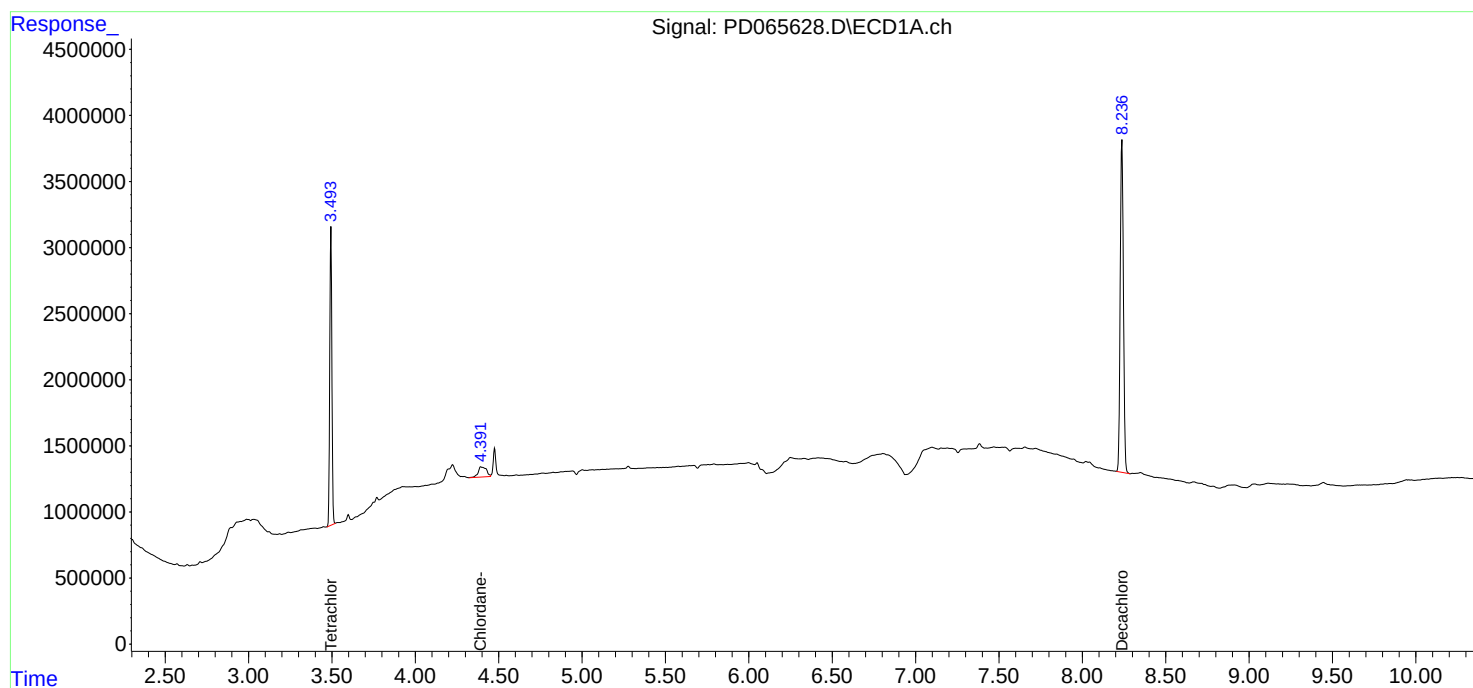


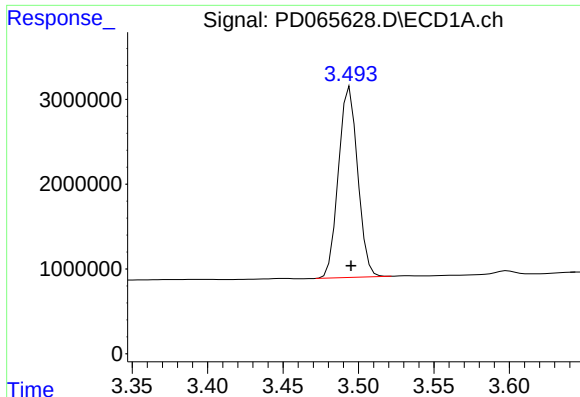

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 19942878
Conc: 20.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

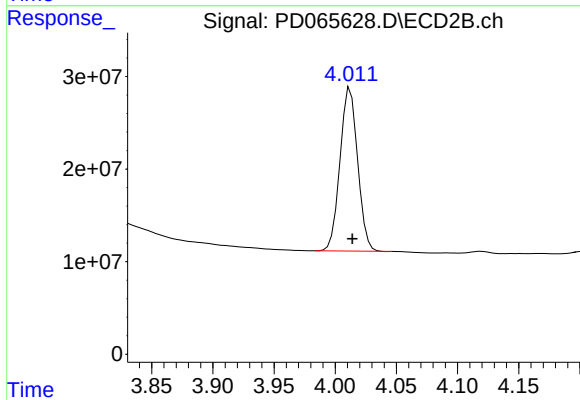


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: -0.002 min
Response: 176984076
Conc: 24.15 ng/ml

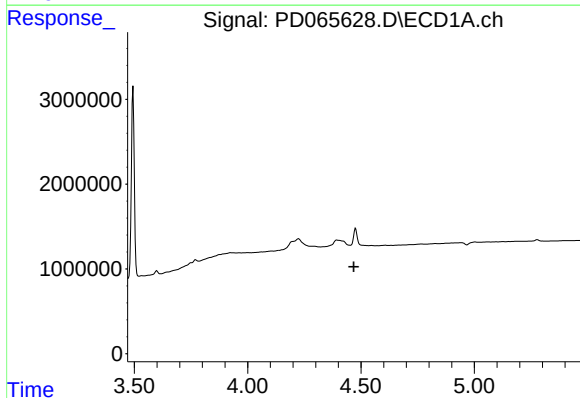


#6 beta-BHC

R.T.: 4.476 min
Delta R.T.: 0.008 min
Response: 2417093
Conc: N.D.

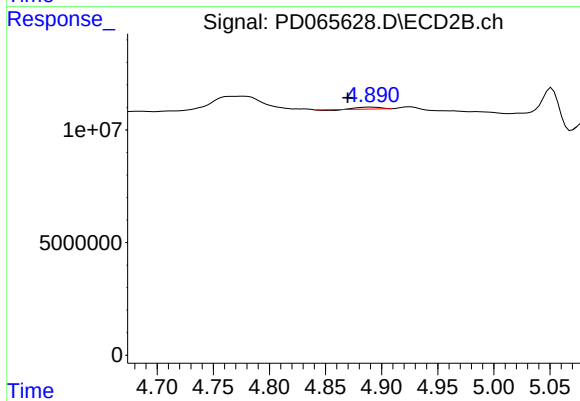

#6 beta-BHC


R.T.: 4.891 min
Delta R.T.: 0.021 min
Response: 1114640
Conc: 0.24 ng/ml

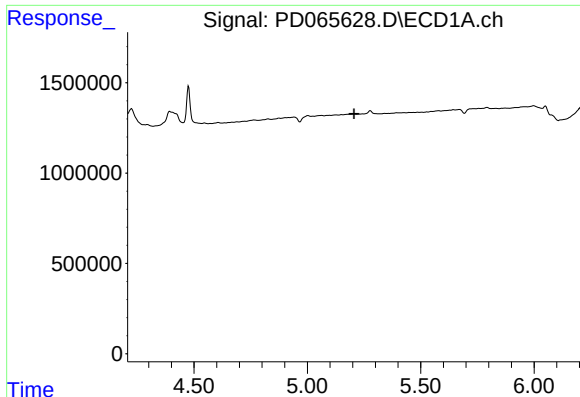

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.206 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

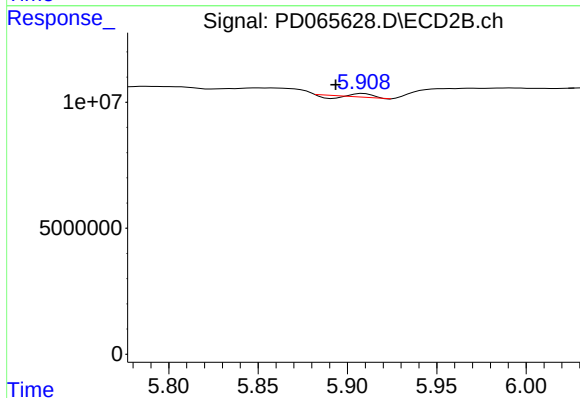


#8 Heptachlor epoxide

R.T.: 5.909 min
Delta R.T.: 0.016 min
Response: 738506
Conc: 0.10 ng/ml

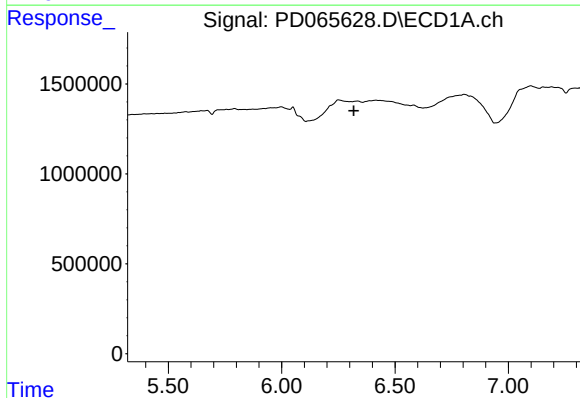


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.318 min
Response: 0
Conc: N.D.

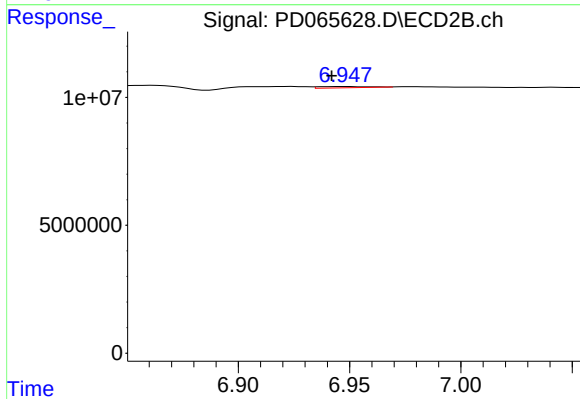

#15 Endosulfan II


R.T.: 6.948 min
Delta R.T.: 0.006 min
Response: 717948
Conc: 0.11 ng/ml

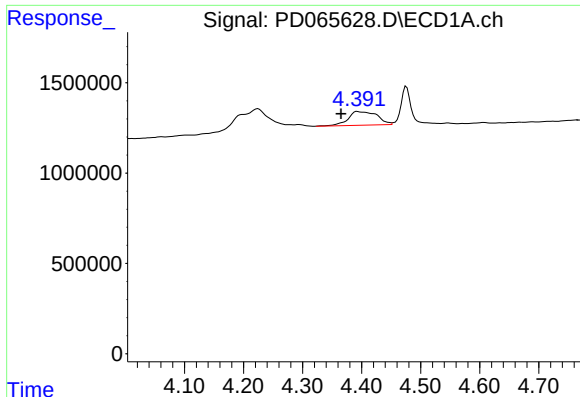

#23 Chlordane-1


R.T.: 4.393 min
Delta R.T.: 0.027 min
Response: 2594443
Conc: 62.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

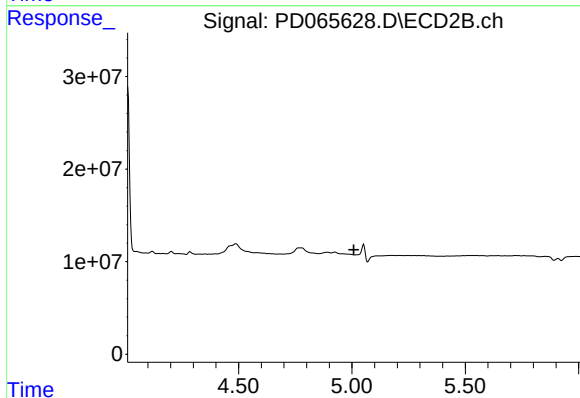


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.008 min
Response: 0
Conc: N.D.

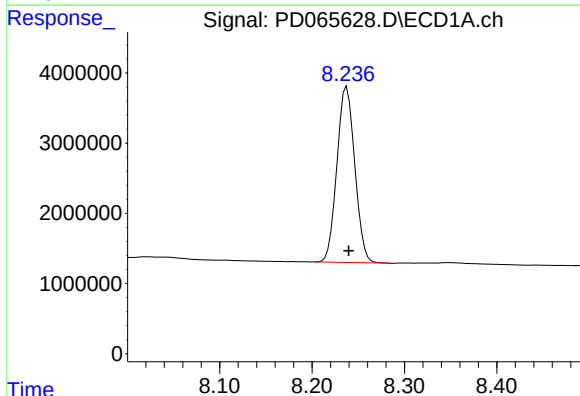

#28 Decachlorobiphenyl

R.T.: 8.238 min
Delta R.T.: -0.002 min
Response: 33690472
Conc: 19.54 ng/ml

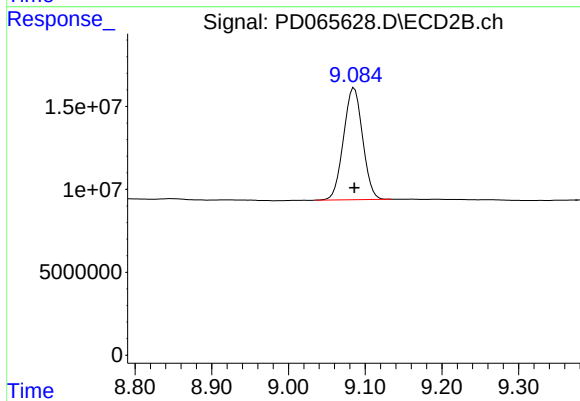

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 117261913
Conc: 21.98 ng/ml