

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090921\
 Data File : PD065636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2021 13:41
 Operator : AR\AJ
 Sample : M3681-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:35:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 09 15:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.495	4.014	14462381	120.0E6	14.757	16.376
28)	SA Decachlor...	8.239	9.087	14842065	60517668	8.609	11.341 #
Target Compounds							
7)	B delta-BHC	0.000	5.108f	0	2039890	N.D.	0.219 #
9)	A Endosulfan I	5.571f	0.000	1220830	0	0.861	N.D. #
10)	B gamma-Chl...	0.000	6.128	0	1384666	N.D.	0.184 #
11)	B alpha-Chl...	0.000	6.198	0	2454720	N.D.	0.333 #
16)	A 4,4'-DDD	0.000	6.851	0	3922343	N.D.	0.628 #
22)	Mirex	7.368	0.000	947918	0	0.605	N.D. #
25)	Chlordane-3	0.000	6.128	0	1384666	N.D.	1.341 #
26)	Chlordane-4	0.000	6.198	0	2454720	N.D.	2.034 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090921\
Data File : PD065636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2021 13:41
Operator : AR\AJ
Sample : M3681-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:35:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 09 15:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

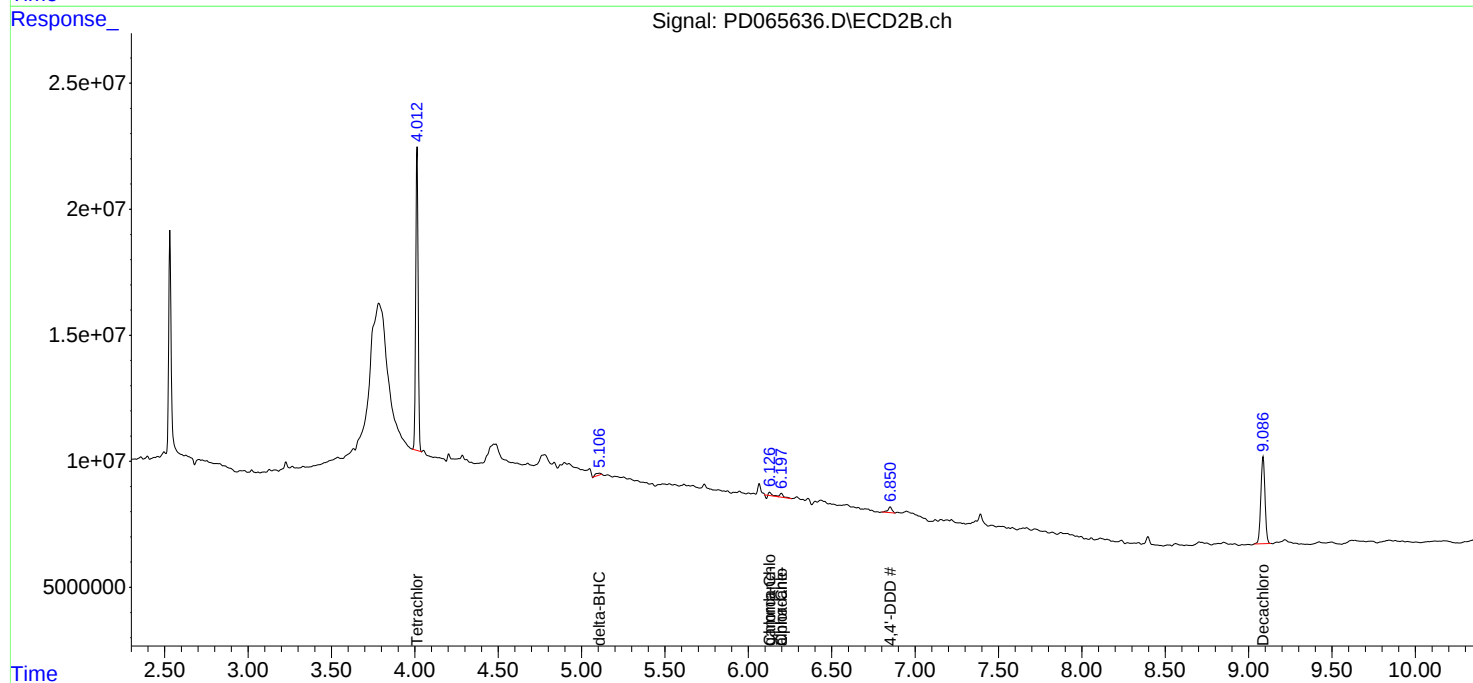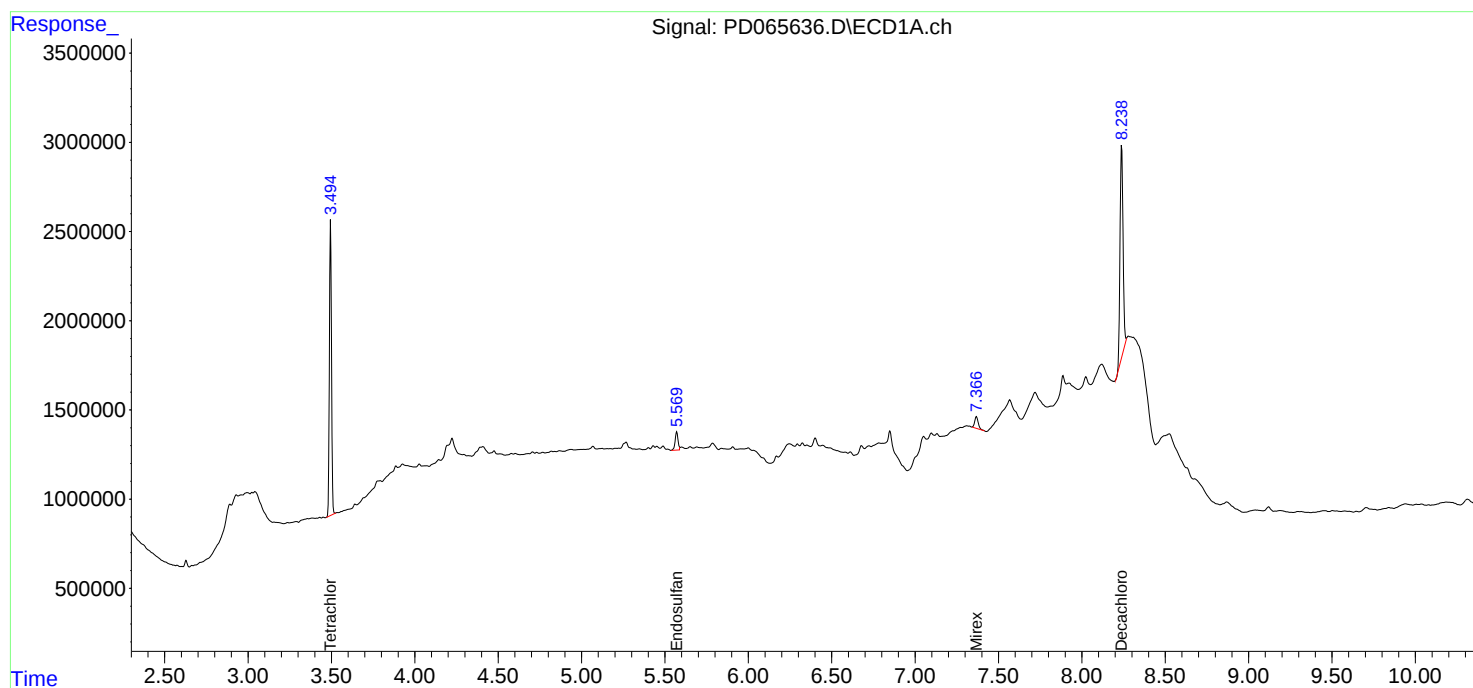


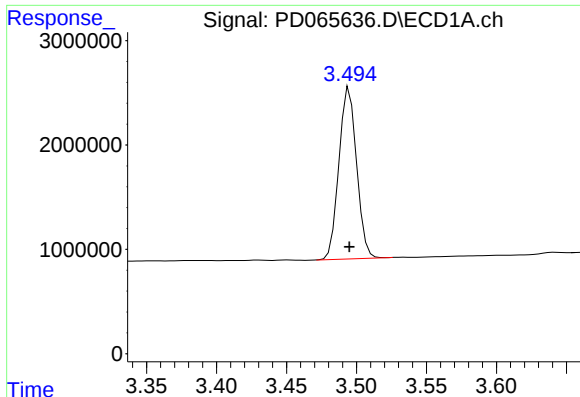

#1 Tetrachloro-m-xylene


R.T.: 3.495 min
Delta R.T.: 0.000 min
Response: 14462381
Conc: 14.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

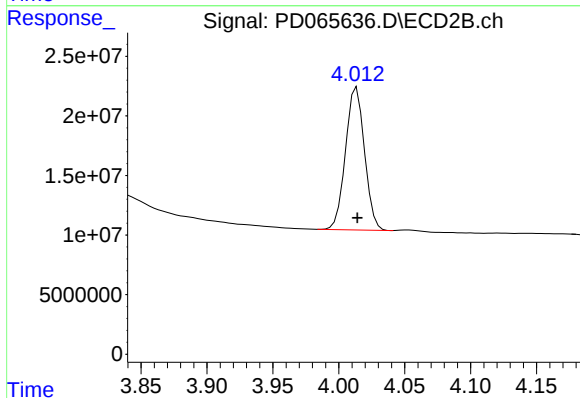


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.000 min
Response: 120026141
Conc: 16.38 ng/ml

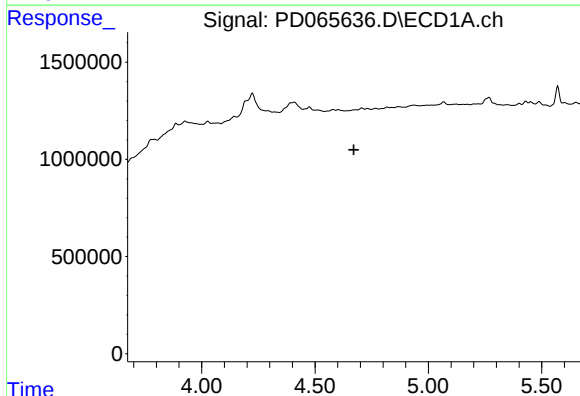


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.671 min
Response: 0
Conc: N.D.

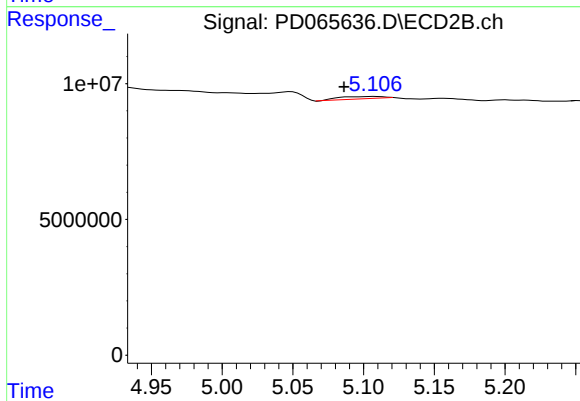

#7 delta-BHC


R.T.: 5.108 min
Delta R.T.: 0.022 min
Response: 2039890
Conc: 0.22 ng/ml

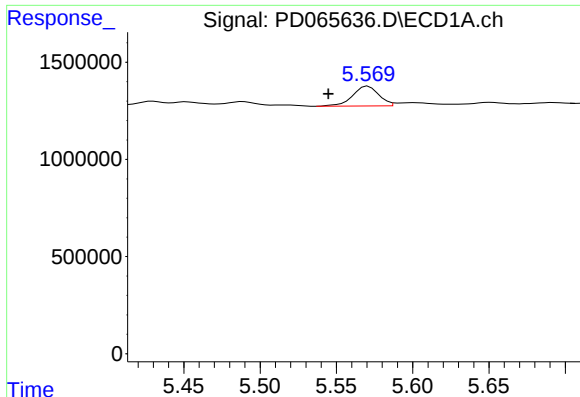

#9 Endosulfan I


R.T.: 5.571 min
Delta R.T.: 0.026 min
Response: 1220830
Conc: 0.86 ng/ml

Instrument :
ECD_D
ClientSampleId :

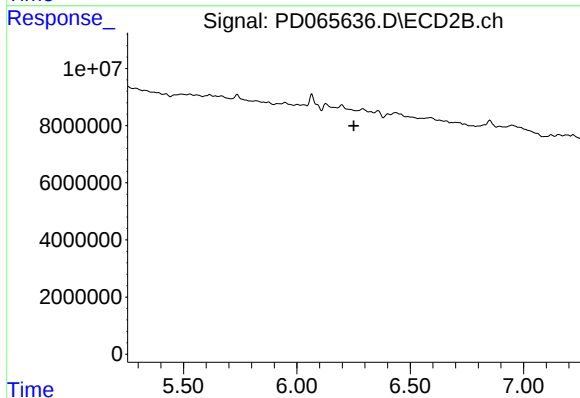


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.252 min
Response: 0
Conc: N.D.

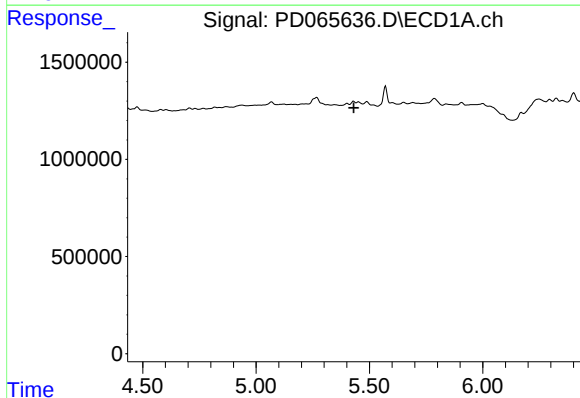


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.431 min
Response: 0
Conc: N.D.

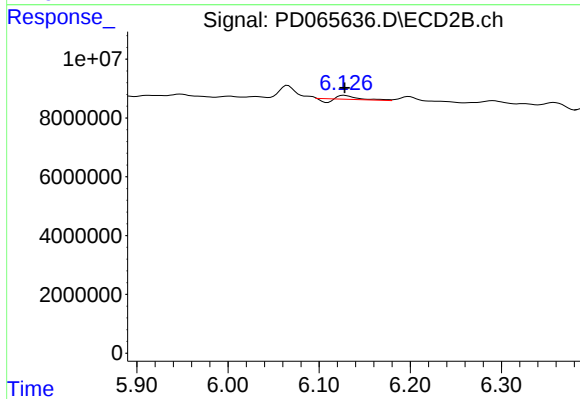

#10 gamma-Chlordane


R.T.: 6.128 min
Delta R.T.: 0.000 min
Response: 1384666
Conc: 0.18 ng/ml

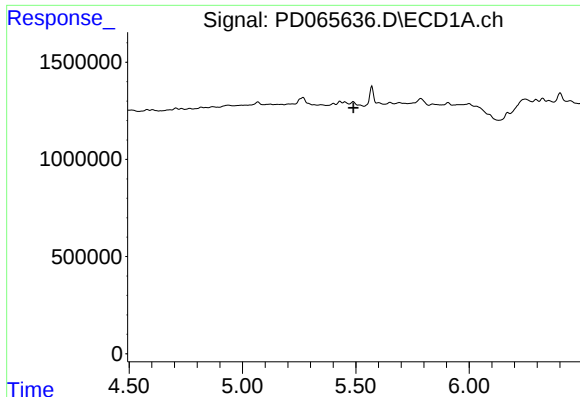

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

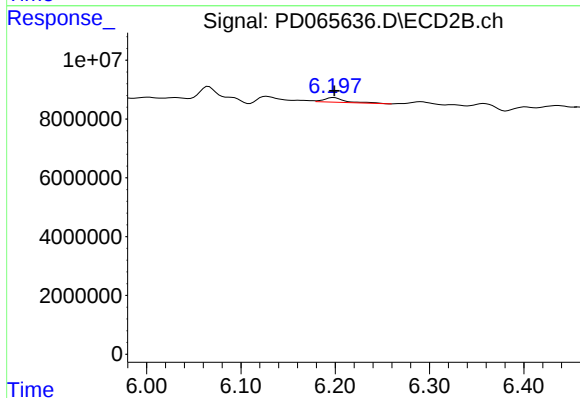


#11 alpha-Chlordane

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 2454720
Conc: 0.33 ng/ml

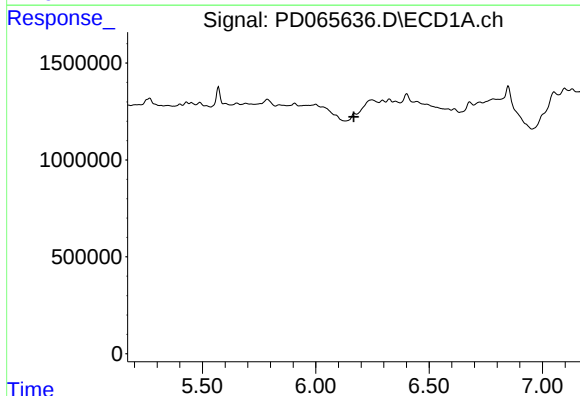


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.167 min
Response: 0
Conc: N.D.

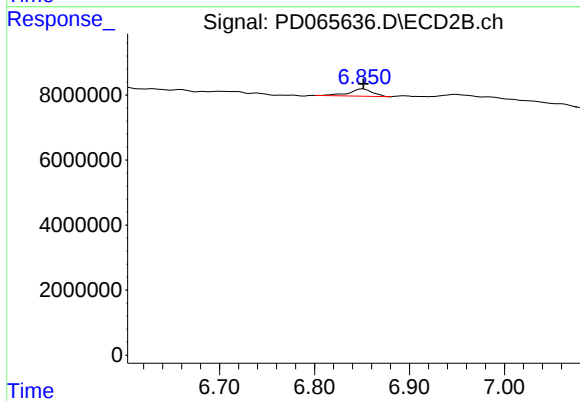

#16 4,4'-DDD


R.T.: 6.851 min
Delta R.T.: 0.000 min
Response: 3922343
Conc: 0.63 ng/ml

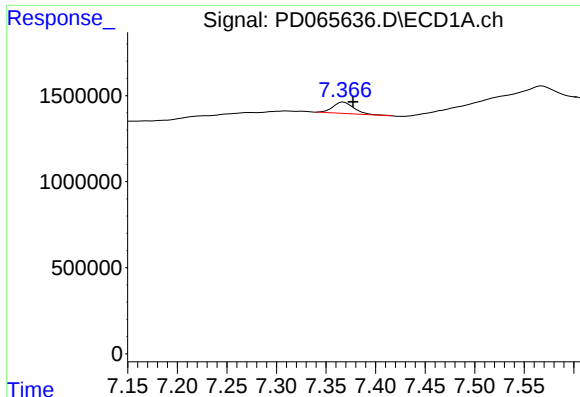

#22 Mirex


R.T.: 7.368 min
Delta R.T.: -0.010 min
Response: 947918
Conc: 0.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

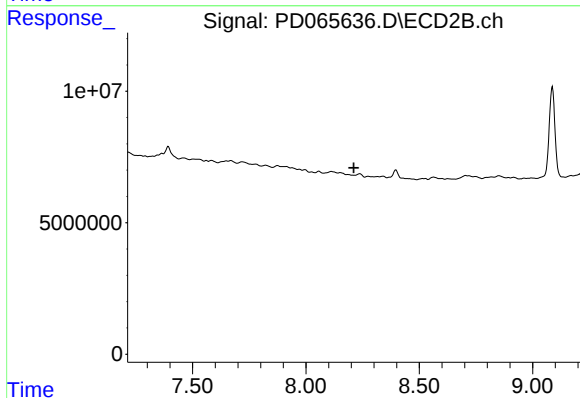


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.211 min
Response: 0
Conc: N.D.

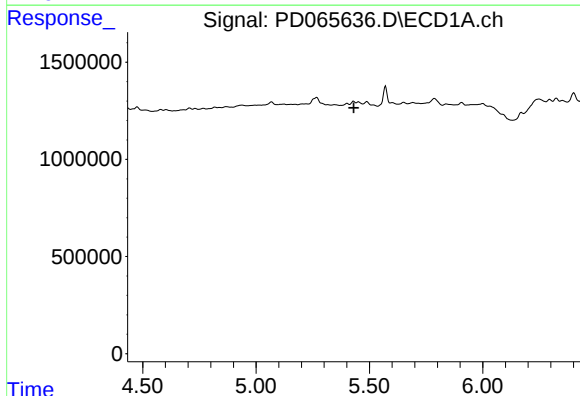


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.431 min
Response: 0
Conc: N.D.

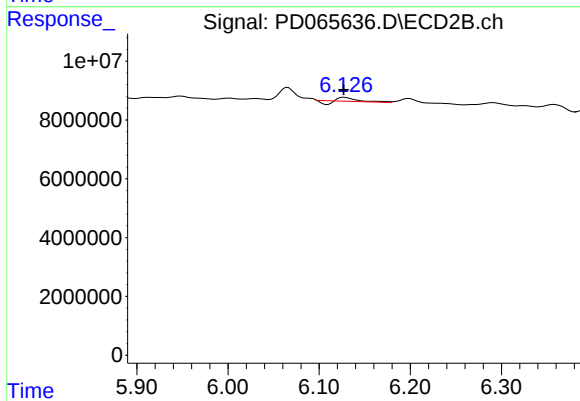

#25 Chlordane-3


R.T.: 6.128 min
Delta R.T.: 0.000 min
Response: 1384666
Conc: 1.34 ng/ml

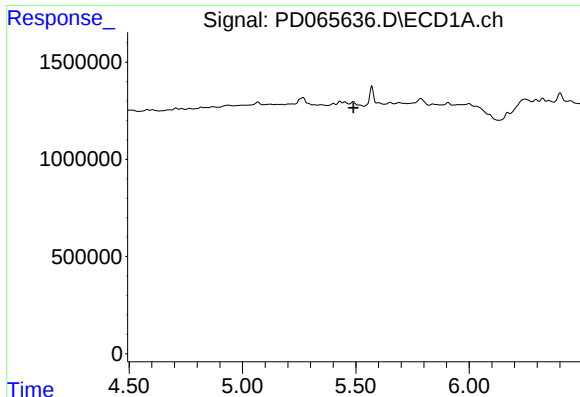

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

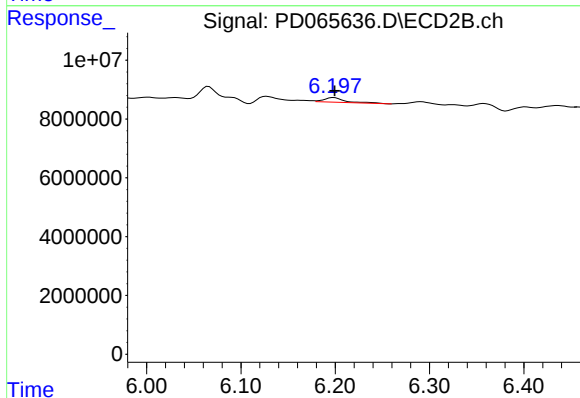


#26 Chlordane-4

R.T.: 6.198 min
Delta R.T.: -0.001 min
Response: 2454720
Conc: 2.03 ng/ml

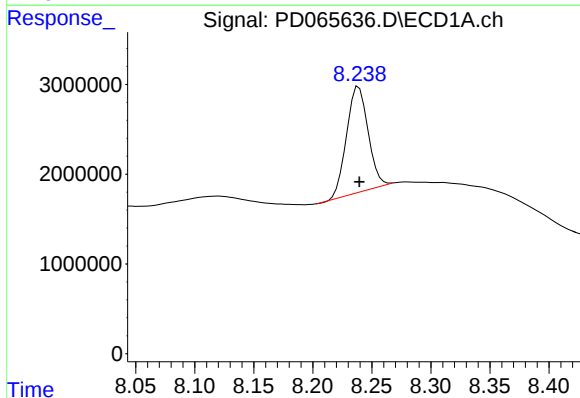

#28 Decachlorobiphenyl

R.T.: 8.239 min
Delta R.T.: 0.000 min
Response: 14842065
Conc: 8.61 ng/ml

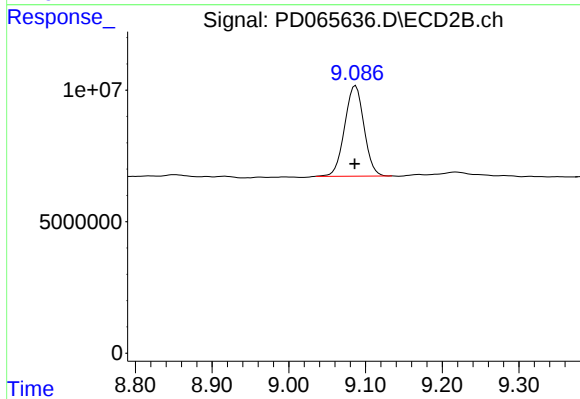

#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: 0.001 min
Response: 60517668
Conc: 11.34 ng/ml