

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090921\
 Data File : PD065644.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2021 16:23
 Operator : AR\AJ
 Sample : M3655-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:37:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 09 15:08:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.494	4.013	18932175	162.4E6	19.318	22.153
28)	SA Decachlor...	8.238	9.086	29230847	103.3E6	16.954	19.355
Target Compounds							
4)	MA Heptachlor	4.500f	0.000	9889228	0	6.516	N.D. #
6)	B beta-BHC	4.500f	4.893f	9889228	1994700	8.839	0.428 #
13)	MA Dieldrin	5.793	0.000	1169298	0	0.756	N.D. #
15)	B Endosulfa...	0.000	6.948	0	2167237	N.D.	0.338 #
23)	Chlordane-1	0.000	5.007	0	5775762	N.D.	19.804 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090921\
Data File : PD065644.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2021 16:23
Operator : AR\AJ
Sample : M3655-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:37:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090421.M
Quant Title : GC Extractables
QLast Update : Thu Sep 09 15:08:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

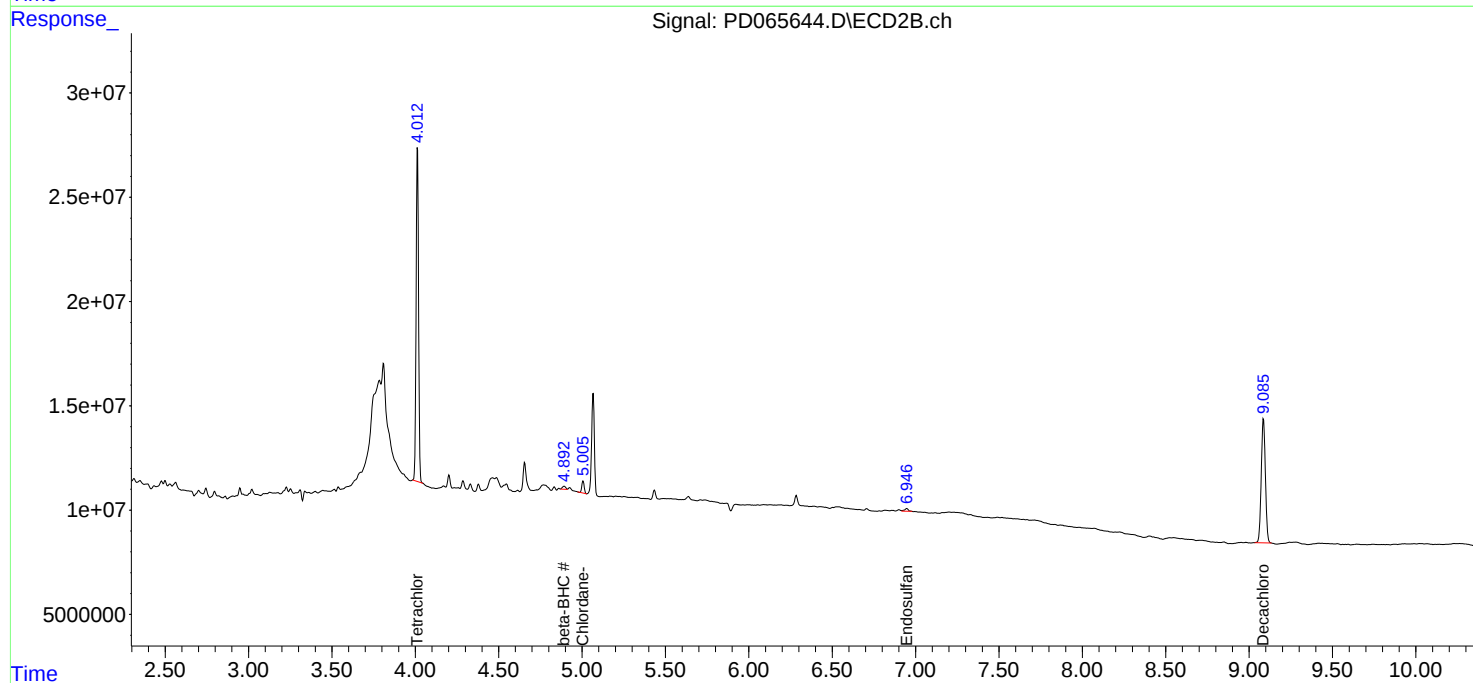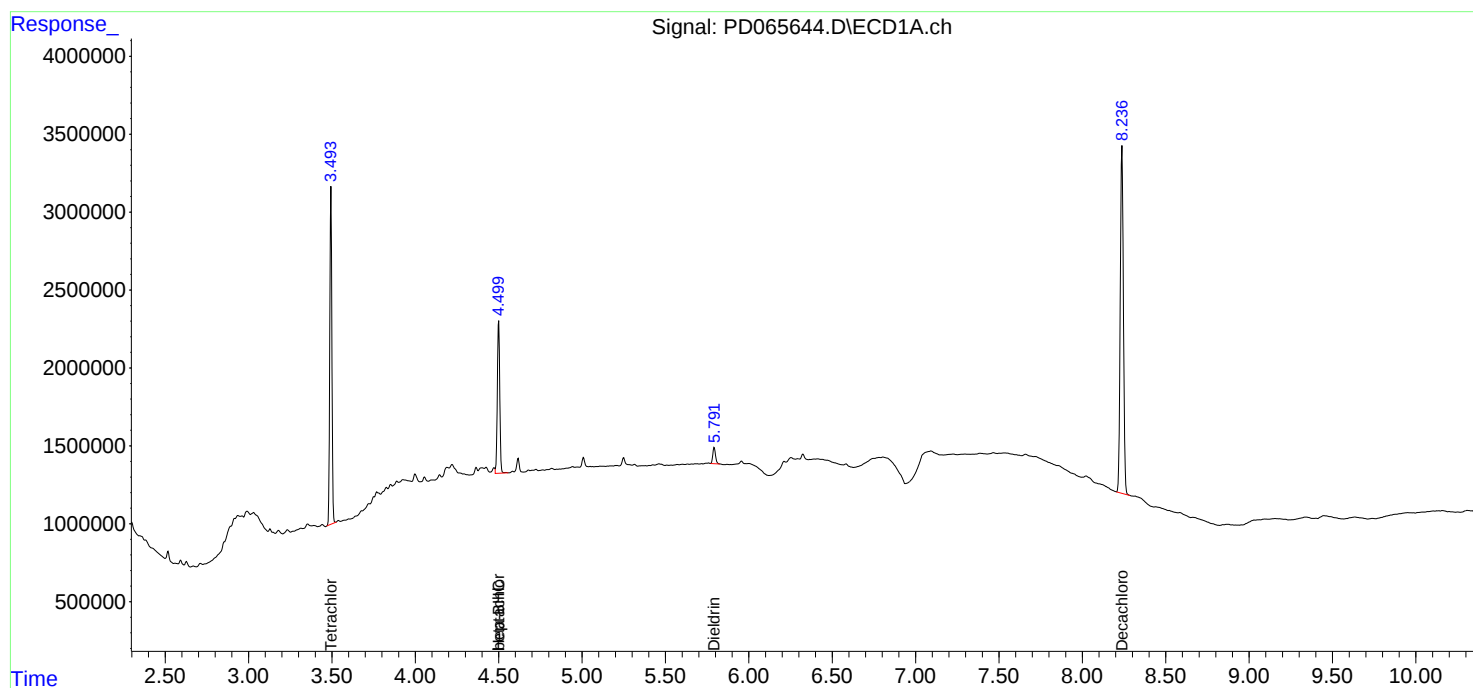


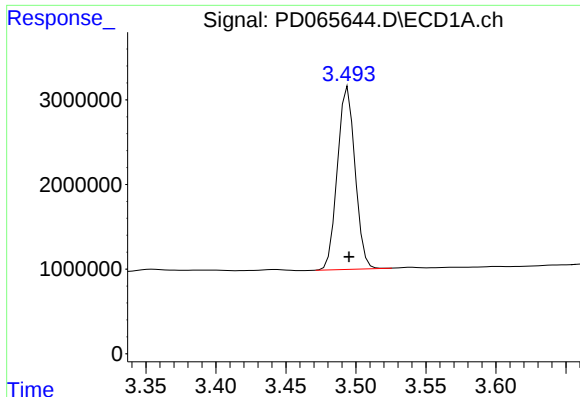

#1 Tetrachloro-m-xylene


R.T.: 3.494 min
Delta R.T.: 0.000 min
Response: 18932175
Conc: 19.32 ng/ml

Instrument :
ECD_D
ClientSampleId :

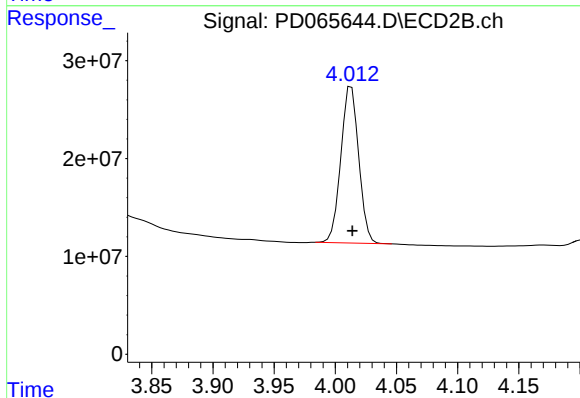


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 162370783
Conc: 22.15 ng/ml

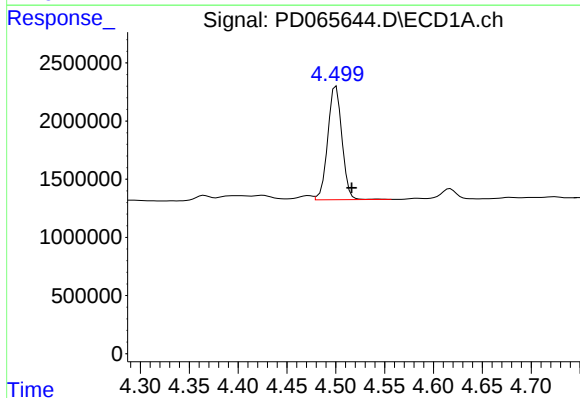


#4 Heptachlor

R.T.: 4.500 min
Delta R.T.: -0.016 min
Response: 9889228
Conc: 6.52 ng/ml

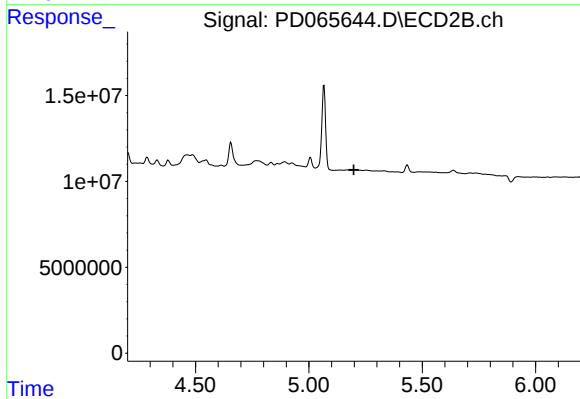

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.199 min
Response: 0
Conc: N.D.

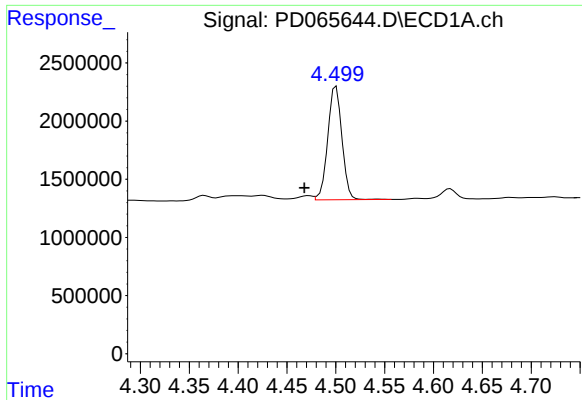

#6 beta-BHC


R.T.: 4.500 min
Delta R.T.: 0.032 min
Response: 9889228
Conc: 8.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

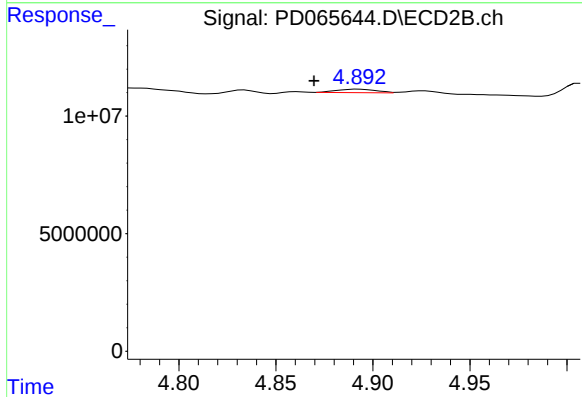


#6 beta-BHC

R.T.: 4.893 min
Delta R.T.: 0.023 min
Response: 1994700
Conc: 0.43 ng/ml

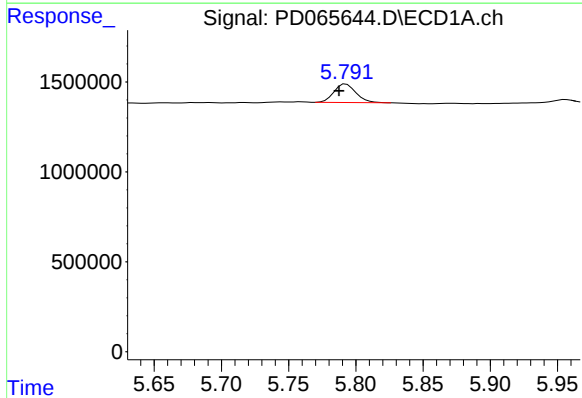


#13 Dieldrin

R.T.: 5.793 min
Delta R.T.: 0.005 min
Response: 1169298
Conc: 0.76 ng/ml

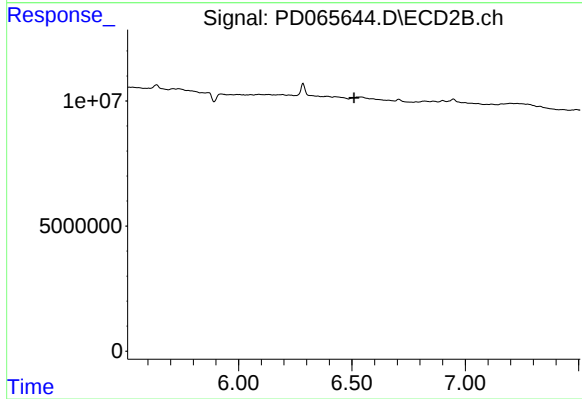

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.509 min
Response: 0
Conc: N.D.

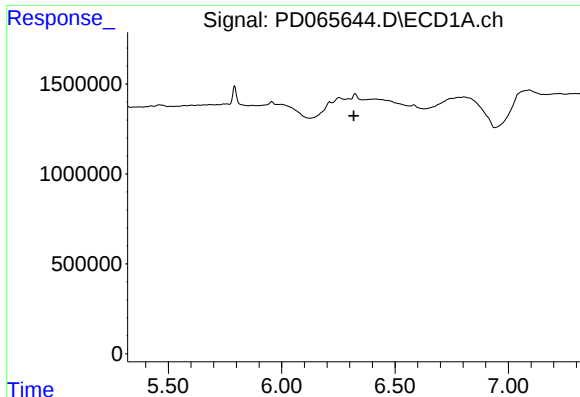

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

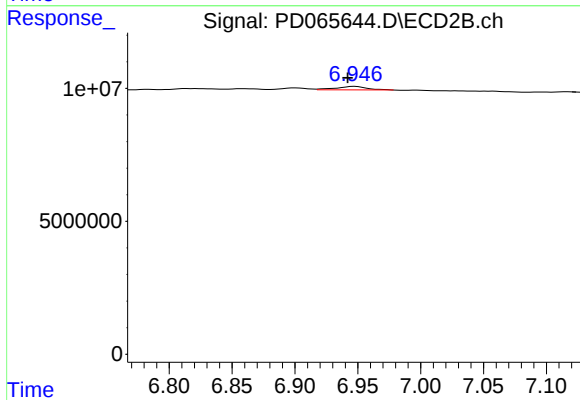


#15 Endosulfan II

R.T.: 6.948 min
Delta R.T.: 0.006 min
Response: 2167237
Conc: 0.34 ng/ml

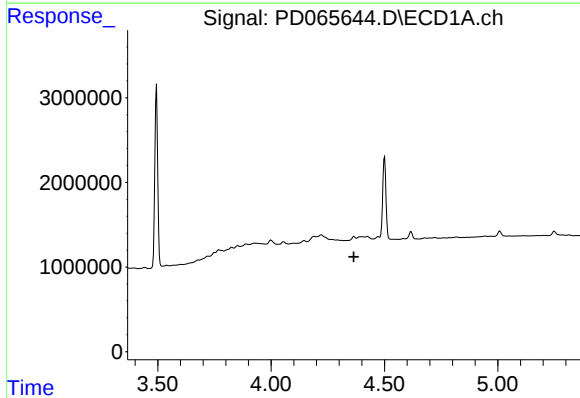


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.365 min
Response: 0
Conc: N.D.

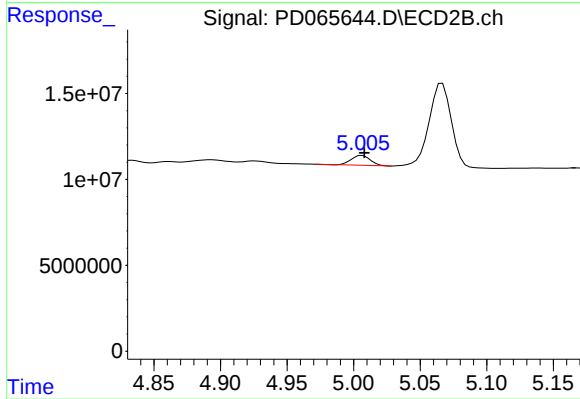

#23 Chlordane-1


R.T.: 5.007 min
Delta R.T.: -0.001 min
Response: 5775762
Conc: 19.80 ng/ml

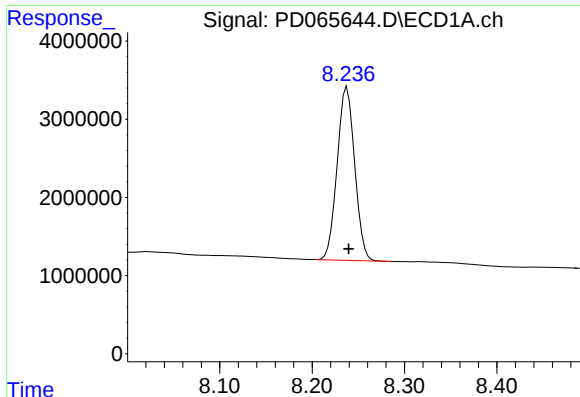

#28 Decachlorobiphenyl

R.T.: 8.238 min
Delta R.T.: -0.002 min
Response: 29230847
Conc: 16.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

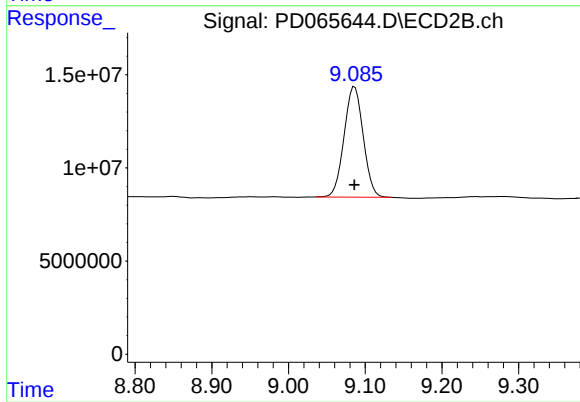

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 103279901
Conc: 19.36 ng/ml