

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090922\
 Data File : PD071784.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2022 12:52
 Operator : AR\AJ
 Sample : N4483-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW358

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/13/2022
 Supervised By : Ankita Jodhani 09/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 18:46:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 07:11:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	2.806	3.561	34639283	445.3E6	13.282	13.590m
2) SA Decachlor...	7.995	9.088	59516460	265.8E6	22.680	27.802
Target Compounds						
10) B trans-Chl...	5.037	5.969	17183096	188.4E6	5.075	11.132m#
11) B cis-Chlor...	5.100	6.047	22689765	247.0E6	6.803	15.155m#
12) B 4,4'-DDE	5.289	6.218	27755044	160.1E6	9.049m	10.970m
17) MA 4,4'-DDT	6.101	7.055	16895052	65249032	6.206	5.408

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD090922\
Data File : PD071784.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2022 12:52
Operator : AR\AJ
Sample : N4483-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 18:46:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082622CLP.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 07:11:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

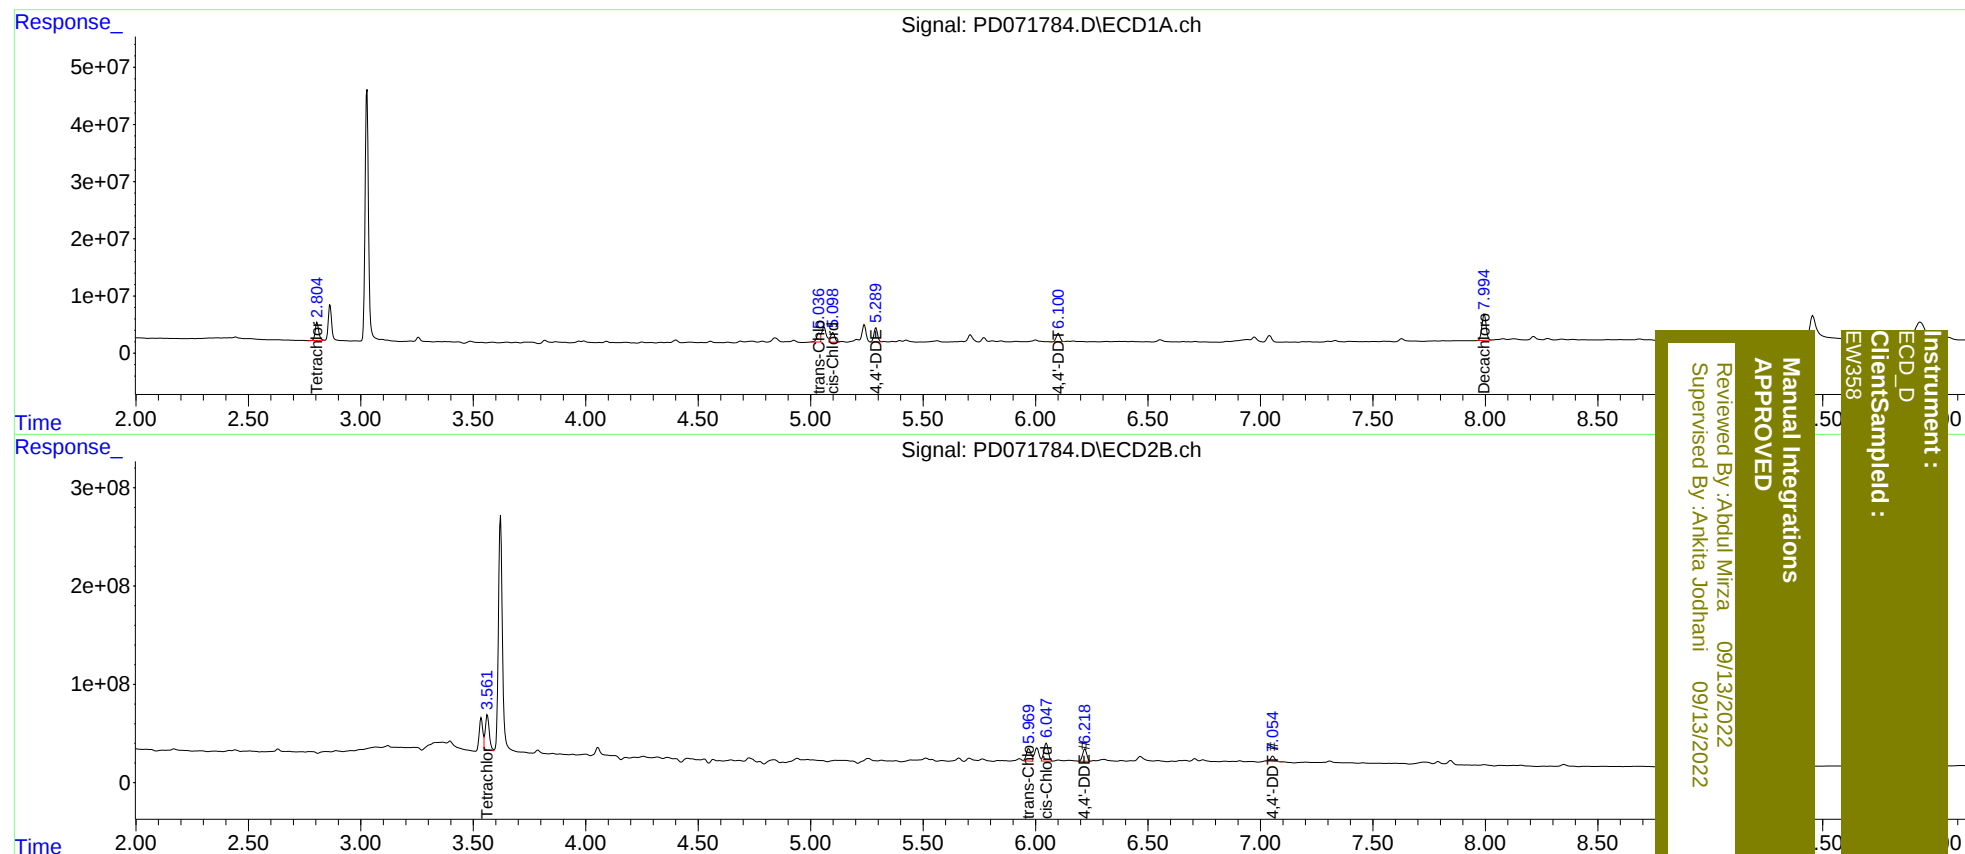

Instrument :
ECD_D
ClientSampled :
EW/358

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/13/2022
Supervised By : Ankita Jodhani 09/13/2022